

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
 Data File : BN011724.D
 Acq On : 05 Sep 2020 05:36
 Operator : CG/JU
 Sample : L3843-07
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Sep 05 06:44:28 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 05 05:40:34 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	3083	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	12040	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.38	164	6967	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.12	188	14982	0.40	ng/ul	0.00
16) Chrysene-d12	21.31	240	13830	0.40	ng/ul	0.00
20) Perylene-d12	23.56	264	14019	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.12	152	2952	0.17	ng/ul	0.00
14) Fluoranthene-d10	19.15	212	6709	0.16	ng/ul	0.00
Target Compounds				Ovalue		
3) Naphthalene	10.57	128	1934	0.055	ng/ul#	94
7) Acenaphthylene	14.09	152	4298	0.123	ng/ul	98
8) Acenaphthene	14.44	153	3401	0.125	ng/ul	98
9) Fluorene	15.43	166	1423	0.044	ng/ul#	98
12) Phenanthrene	17.16	178	7023	0.139	ng/ul	99
13) Anthracene	17.25	178	6393	0.153	ng/ul	99
15) Fluoranthene	19.18	202	34808	0.597	ng/ul	98
17) Pyrene	19.54	202	33683	0.623	ng/ul#	94
18) Benzo(a)anthracene	21.29	228	19996	0.431	ng/ul	98
19) Chrysene	21.35	228	26273	0.420	ng/ul	99
21) Benzo(b)fluoranthene	22.88	252	43940	0.721	ng/ul	95
22) Benzo(k)fluoranthene	22.88	252	43940	0.652	ng/ul	95
23) Benzo(a)pyrene	23.46	252	21993	0.430	ng/ul	93
24) Indeno(1,2,3-cd)pyrene	25.82	276	14383	0.208	ng/ul#	99
25) Dibenzo(a,h)anthracene	25.83	278	4710	0.083	ng/ul#	84
26) Benzo(a,h,i)perylene	26.51	276	12550	0.194	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
Data File : BN011724.D
Acq On : 05 Sep 2020 05:36
Operator : CG/JU
Sample : L3843-07
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Sep 05 06:44:28 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 05 05:40:34 2020
Response via : Initial Calibration

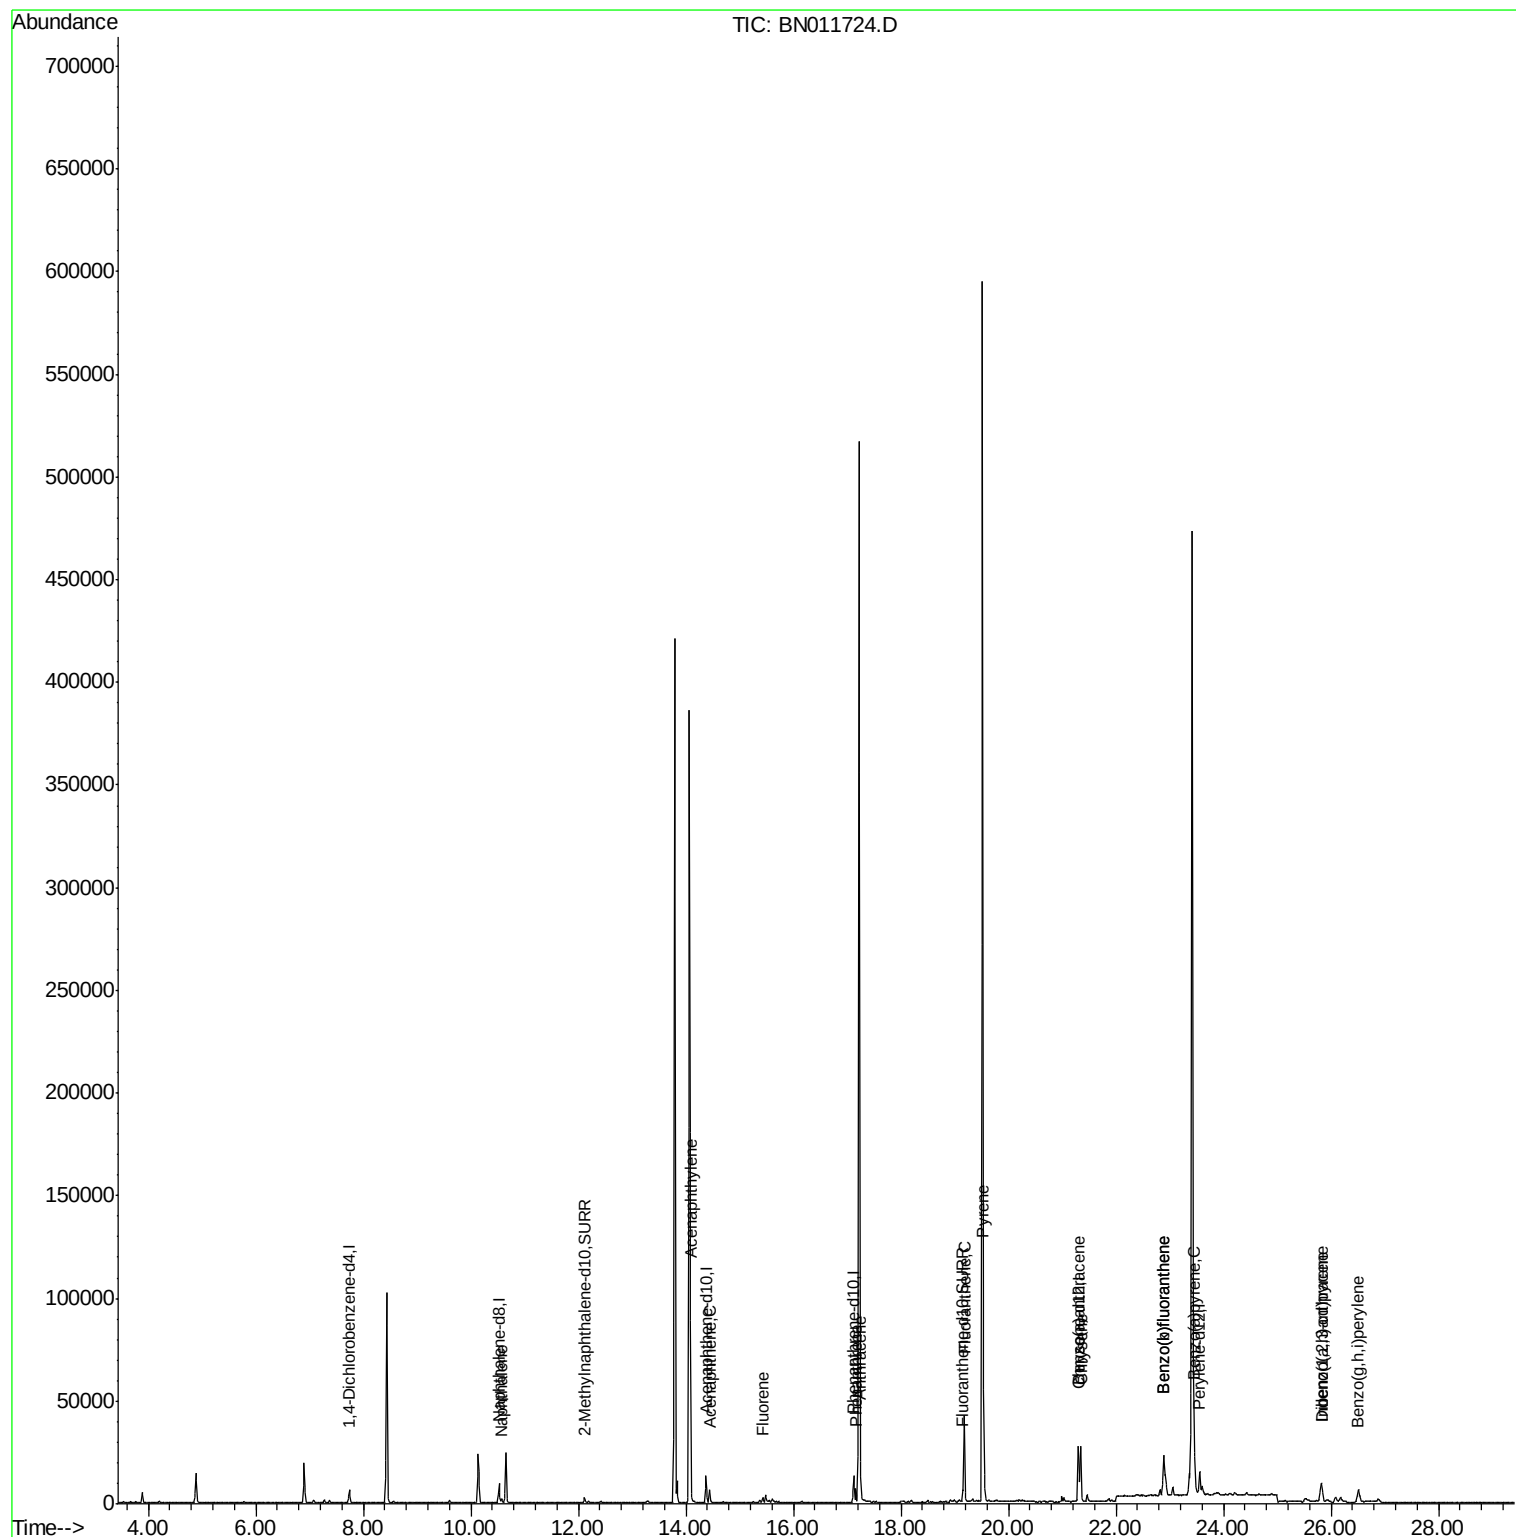

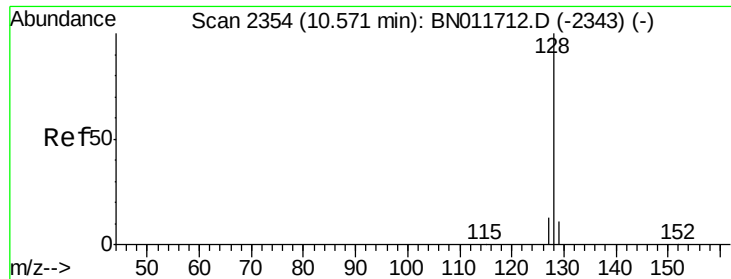

#3

Naphthalene

Concen: 0.055 ng/ul

RT: 10.57 min Scan# 2354

Delta R.T. -0.00 min

Lab File: BN011724.D

Acq: 05 Sep 2020 05:36

Instrument :

BNA_N

ClientSampleId :





Tot Ion:128 Resp: 1934

Ion Ratio Lower Upper

128 100

129 15.9 10.4 15.6#

127 16.4 11.4 17.0

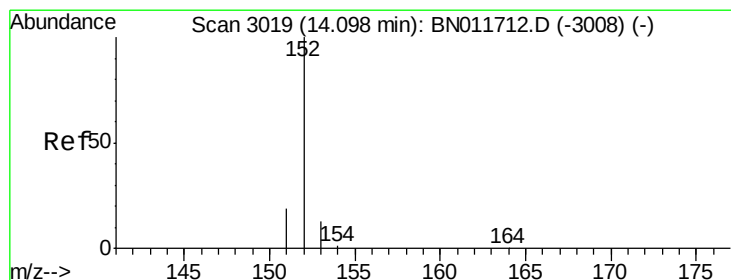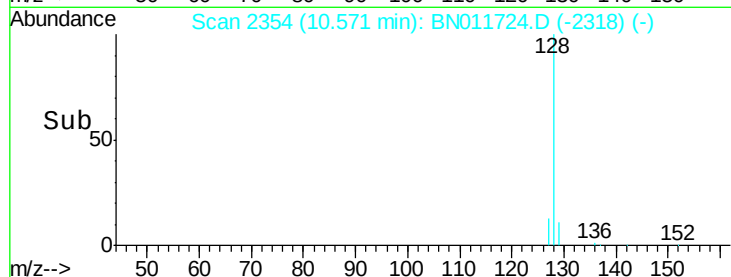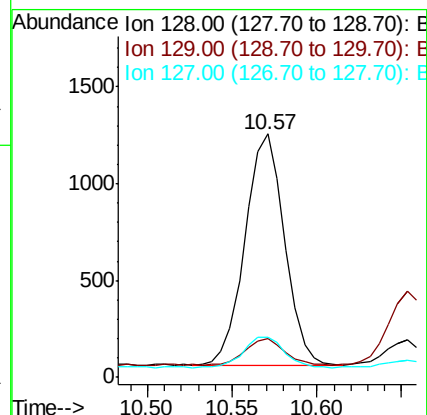

#7

Acenaphthylene

Concen: 0.123 ng/ul

RT: 14.09 min Scan# 3018

Delta R.T. -0.00 min

Lab File: BN011724.D

Acq: 05 Sep 2020 05:36




Tgt Ion:152 Resp: 4298


Ion Ratio Lower Upper

152 100

151 21.7 16.7 25.1

153 14.7 12.3 18.5

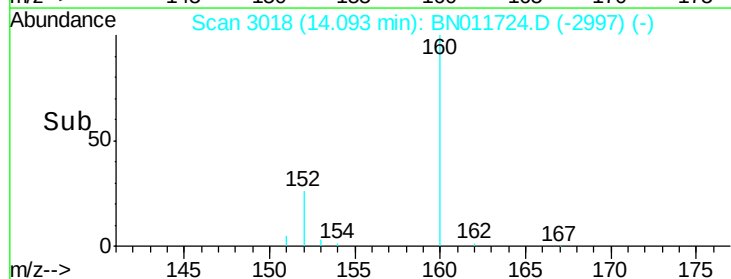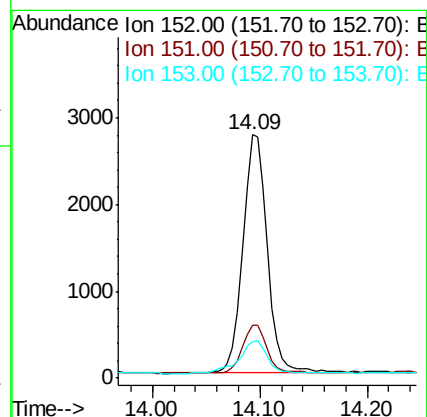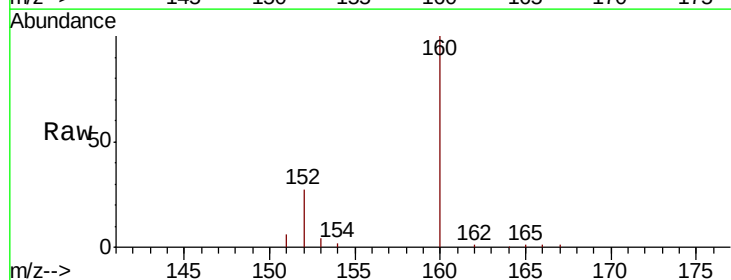

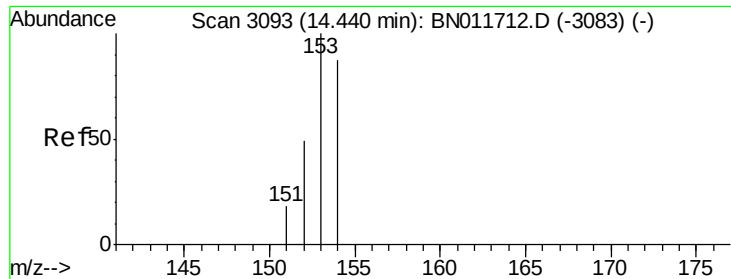

#8

Acenaphthene

Concen: 0.125 ng/ul

RT: 14.44 min Scan# 3093

Delta R.T. -0.00 min

Lab File: BN011724.D

Acq: 05 Sep 2020 05:36

Instrument :

BNA_N

ClientSampleId :


Tot Ion:153 Resp: 3401

Ion Ratio Lower Upper

153 100

152 49.5 41.0 61.6




154 89.4 70.2 105.2

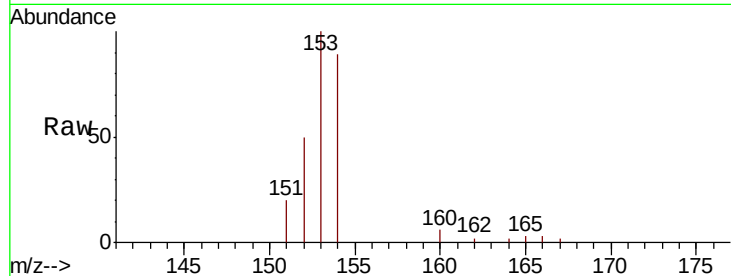

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

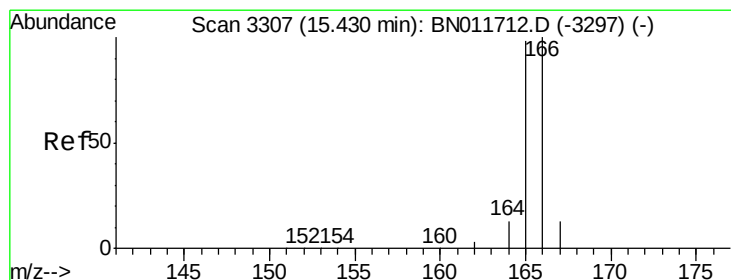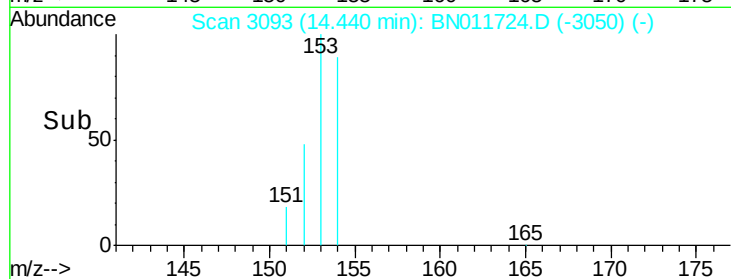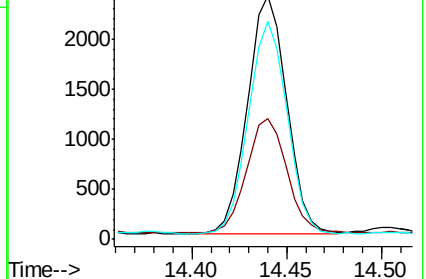

#9

Fluorene

Concen: 0.044 ng/ul

RT: 15.43 min Scan# 3307

Delta R.T. -0.00 min

Lab File: BN011724.D

Acq: 05 Sep 2020 05:36


Tgt Ion:166 Resp: 1423

Ion Ratio Lower Upper

166 100

165 97.0 77.7 116.5



167 20.2 12.5 18.7#




Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

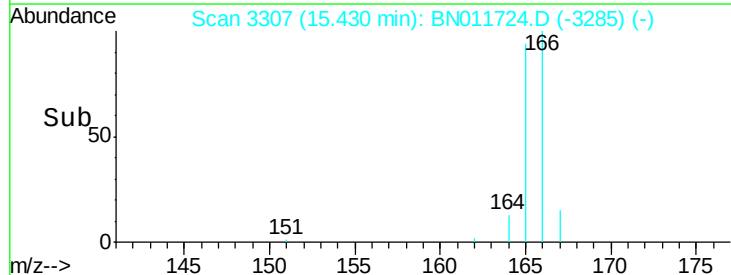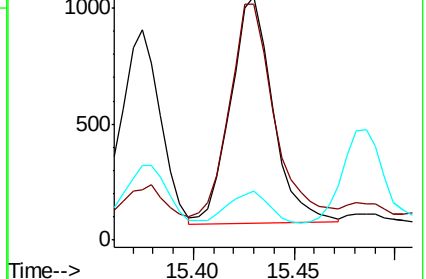

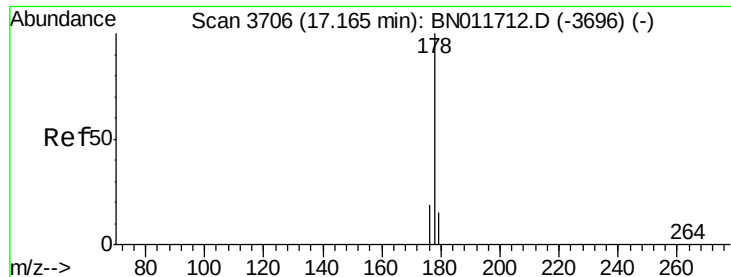

#12

Phenanthrene

Concen: 0.139 ng/ul

RT: 17.16 min Scan# 3706

Delta R.T. -0.00 min

Lab File: BN011724.D

Acq: 05 Sep 2020 05:36

Instrument :

BNA_N

ClientSampleId :


Tot Ion:178 Resp: 7023

Ion Ratio Lower Upper

178 100

179 17.5 13.8 20.8




176 19.5 16.3 24.5

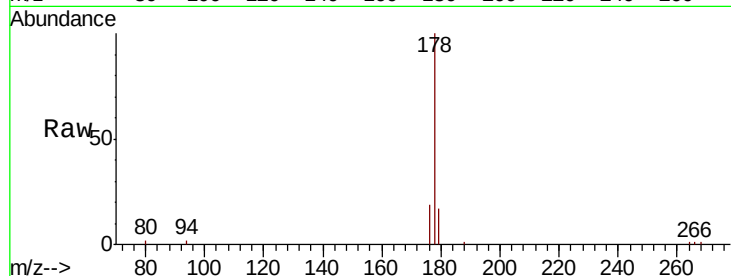

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

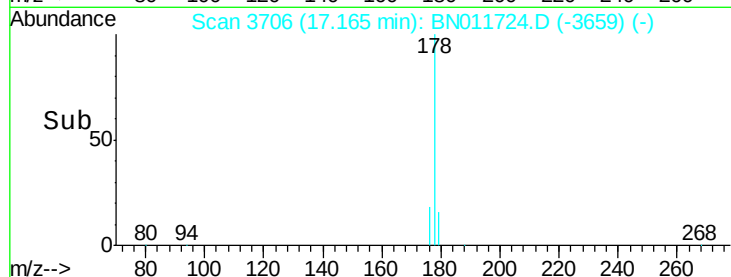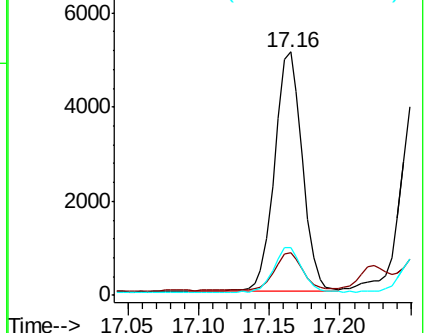

#13

Anthracene

Concen: 0.153 ng/ul

RT: 17.25 min Scan# 3727

Delta R.T. -0.00 min

Lab File: BN011724.D

Acq: 05 Sep 2020 05:36


Tgt Ion:178 Resp: 6393

Ion Ratio Lower Upper

178 100

179 17.5 14.2 21.2



176 19.0 15.8 23.8




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

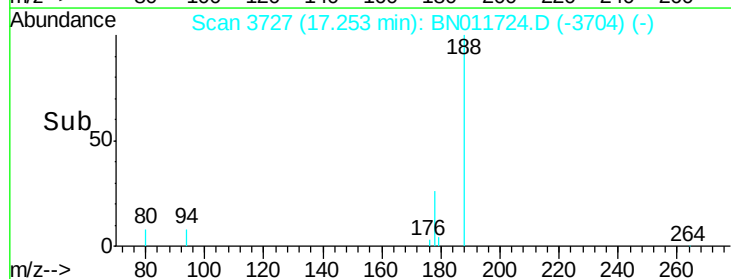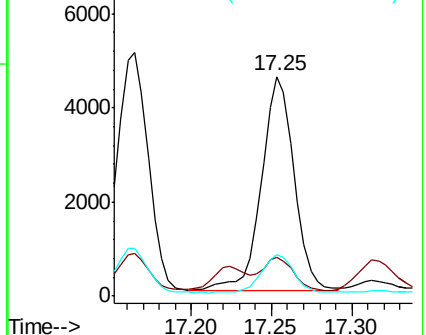

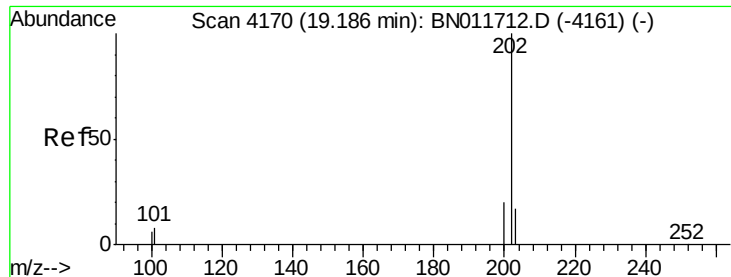

#15

Fluoranthene

Concen: 0.597 ng/ul

RT: 19.18 min Scan# 4169

Delta R.T. -0.00 min

Lab File: BN011724.D

Acq: 05 Sep 2020 05:36

Instrument :

BNA_N

ClientSampleId :


Tot Ion:202 Resp: 34808

Ion Ratio Lower Upper

202 100

101 9.5 0.0 28.3




100 7.3 0.0 27.1

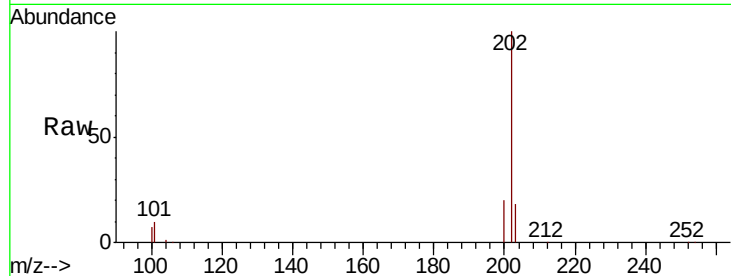

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

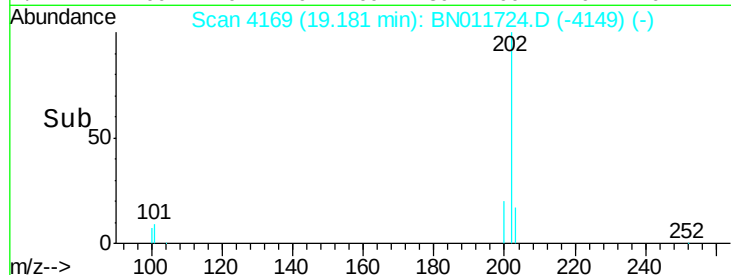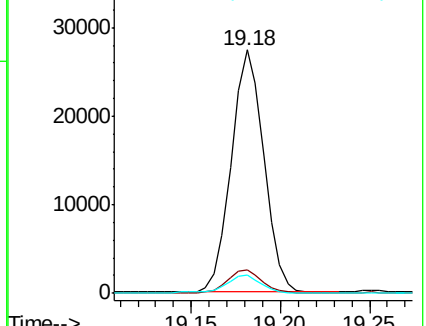

#17

Pyrene

Concen: 0.623 ng/ul

RT: 19.54 min Scan# 4247

Delta R.T. -0.00 min

Lab File: BN011724.D

Acq: 05 Sep 2020 05:36


Tgt Ion:202 Resp: 33683

Ion Ratio Lower Upper

202 100

101 11.7 7.3 10.9#



100 9.8 6.7 10.1




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

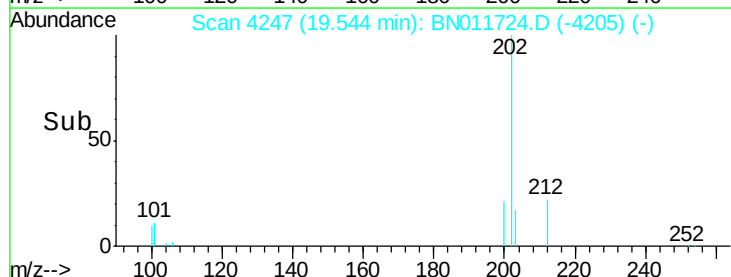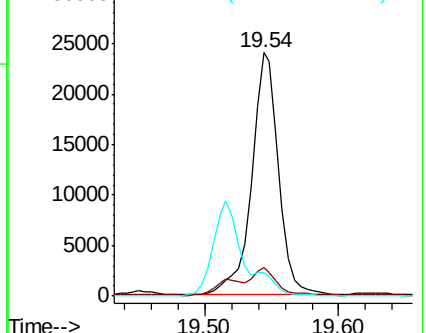

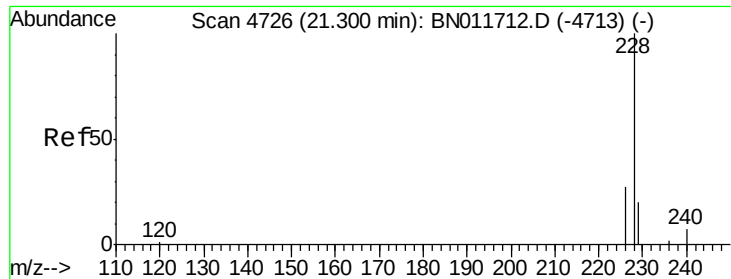

#18

Benzo(a)anthracene

Concen: 0.431 ng/ul

RT: 21.29 min Scan# 4724

Delta R.T. -0.01 min

Lab File: BN011724.D

Acq: 05 Sep 2020 05:36

Instrument :

BNA_N

ClientSampled :





Tot Ion:228 Resp: 19996

Ion Ratio Lower Upper

228 100

229 22.1 16.7 25.1

226 29.6 22.9 34.3

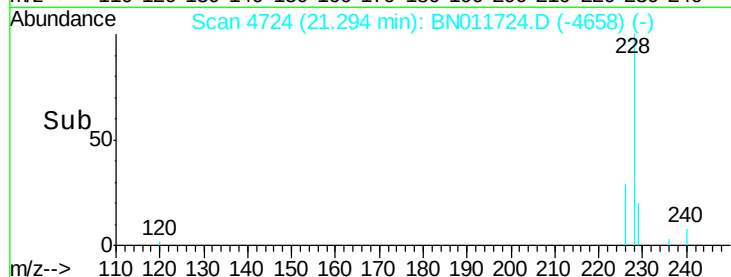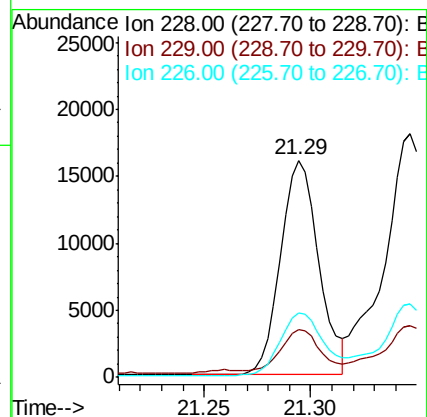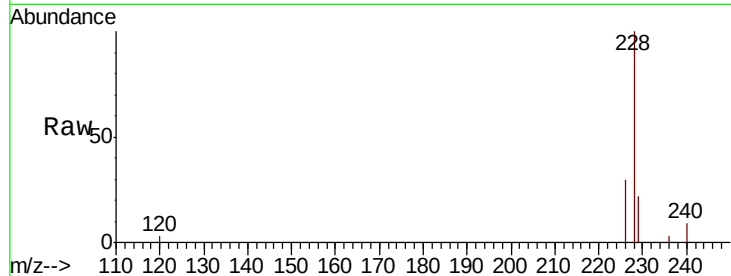

#19

Chrysene

Concen: 0.420 ng/ul

RT: 21.35 min Scan# 4742

Delta R.T. -0.01 min

Lab File: BN011724.D

Acq: 05 Sep 2020 05:36




Tgt Ion:228 Resp: 26273


Ion Ratio Lower Upper

228 100

226 30.0 24.1 36.1

229 21.3 16.4 24.6

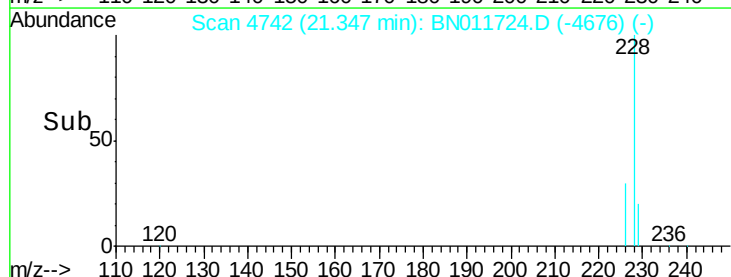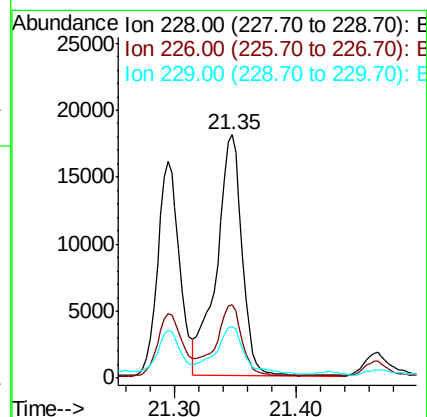

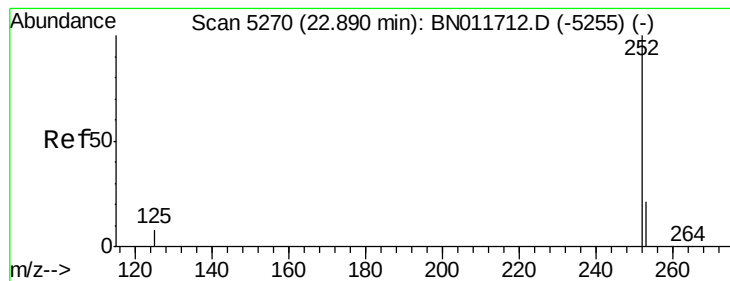

#21

Benzo(b)fluoranthene

Concen: 0.721 ng/ul

RT: 22.88 min Scan# 5268

Delta R.T. -0.01 min

Lab File: BN011724.D

Acq: 05 Sep 2020 05:36

Instrument :

BNA_N

ClientSampleId :


Tot Ion:252 Resp: 43940

Ion Ratio Lower Upper

252 100

253 24.7 0.0 54.8




125 13.1 0.0 22.2

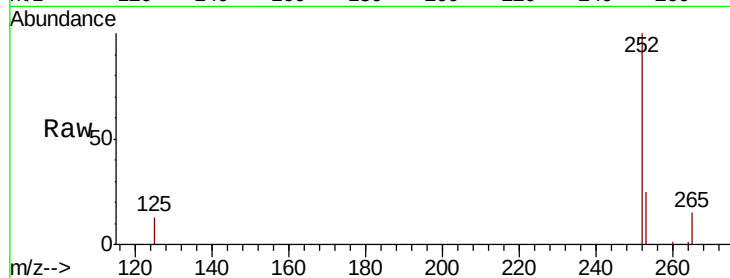

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

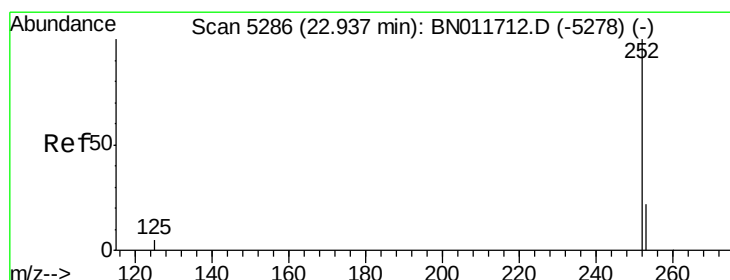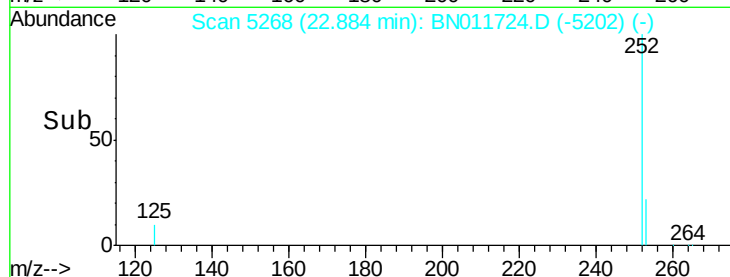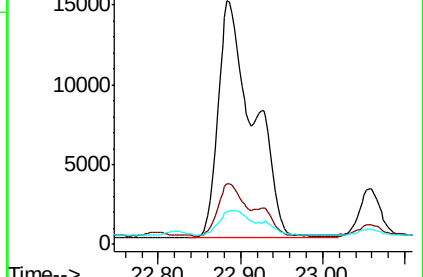

#22

Benzo(k)fluoranthene

Concen: 0.652 ng/ul

RT: 22.88 min Scan# 5268

Delta R.T. -0.05 min

Lab File: BN011724.D

Acq: 05 Sep 2020 05:36


Tgt Ion:252 Resp: 43940

Ion Ratio Lower Upper

252 100

253 24.7 21.8 32.6



125 13.1 9.1 13.7

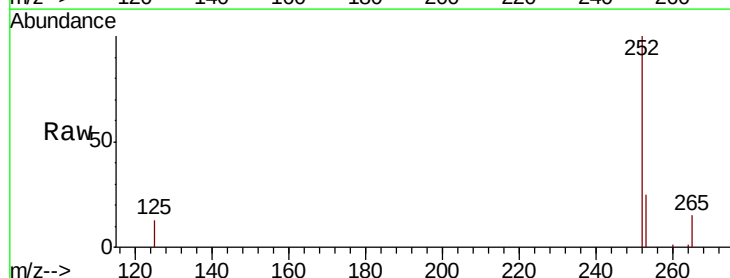


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

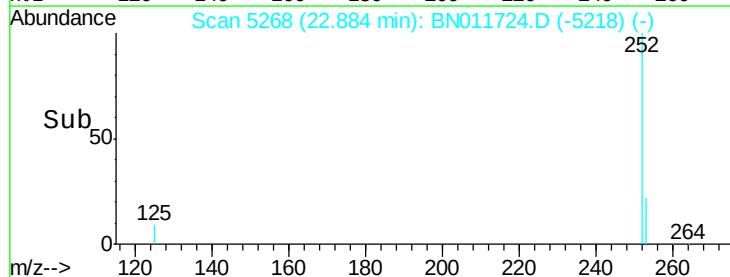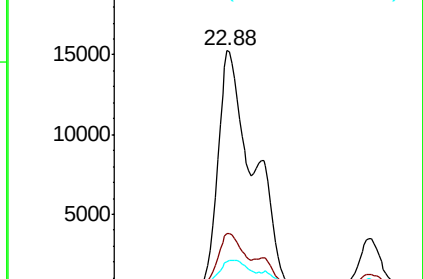

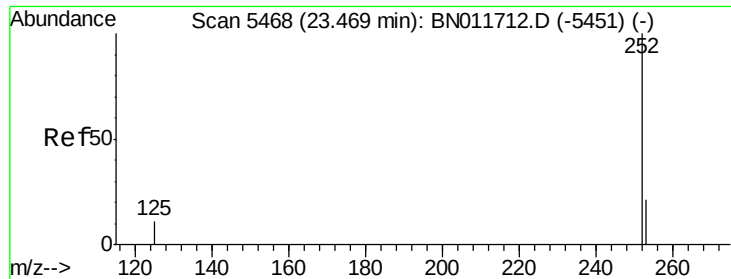

#23

Benzo(a)pyrene

Concen: 0.430 ng/ul

RT: 23.46 min Scan# 5465

Delta R.T. -0.01 min

Lab File: BN011724.D

Acq: 05 Sep 2020 05:36

Instrument :

BNA_N

ClientSampleId :


Tot Ion:252 Resp: 21993

Ion Ratio Lower Upper




252 100

253 25.7 24.4 36.6

125 15.5 11.1 16.7

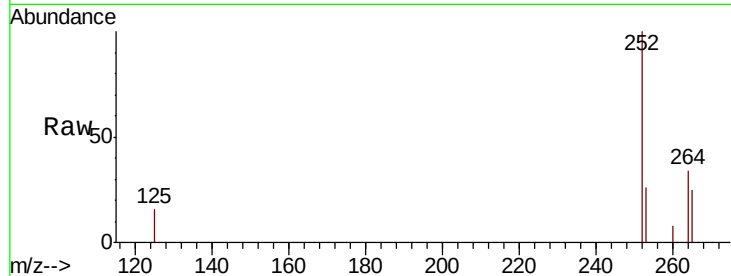

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

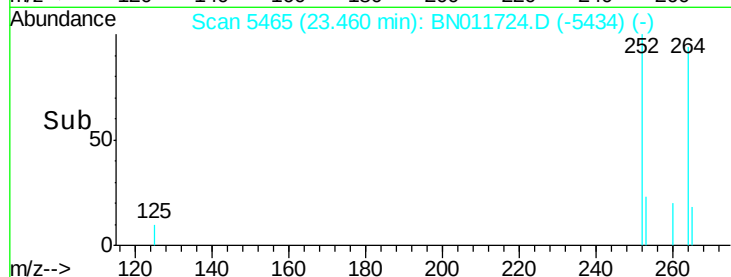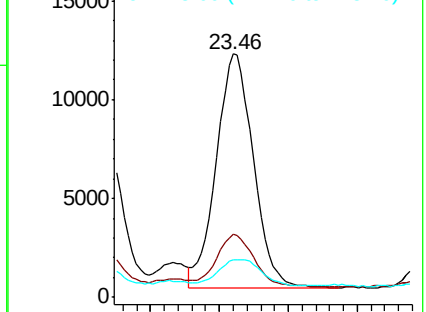

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.208 ng/ul

RT: 25.82 min Scan# 6236

Delta R.T. -0.01 min

Lab File: BN011724.D

Acq: 05 Sep 2020 05:36


Tgt Ion:276 Resp: 14383

Ion Ratio Lower Upper



276 100


138 19.4 15.8 23.6

227 0.0 0.2 0.2#



Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 227.00 (226.70 to 227.70): E



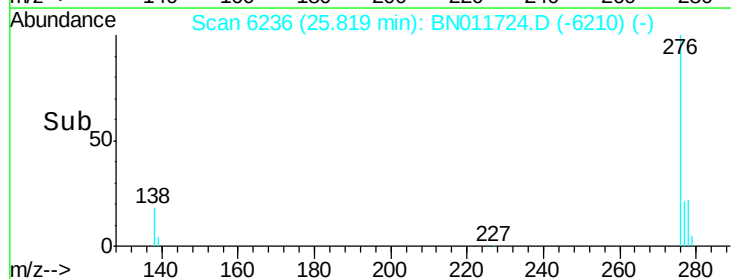
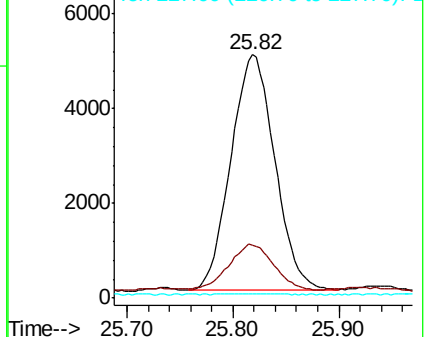


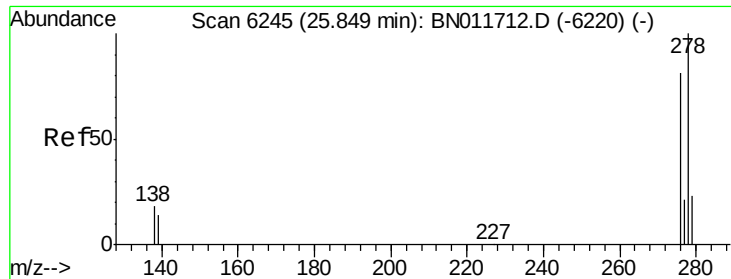

#25
Dibenzo(a,h)anthracene
Concen: 0.083 ng/ul
RT: 25.83 min Scan# 6240
Delta R.T. -0.02 min
Lab File: BN011724.D
Acq: 05 Sep 2020 05:36

Instrument :
BNA_N
ClientSampleId :

Tot Ion:278 Resp: 4710
Ion Ratio Lower Upper
278 100
139 22.4 12.1 18.1#
279 36.4 22.9 34.3#

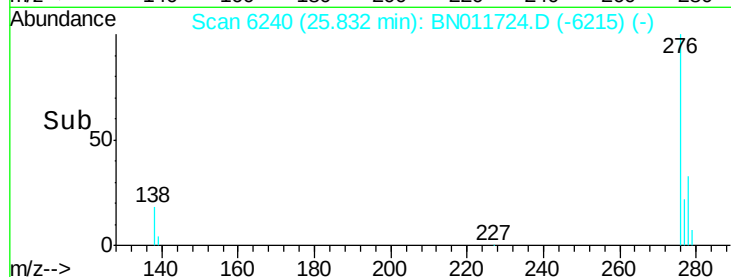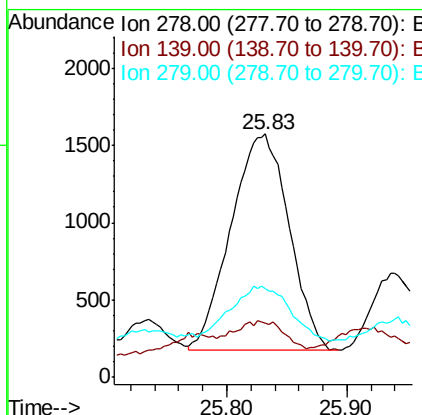

#26
Benzo(g,h,i)perylene
Concen: 0.194 ng/ul
RT: 26.51 min Scan# 6442
Delta R.T. -0.01 min
Lab File: BN011724.D
Acq: 05 Sep 2020 05:36

Tgt Ion:276 Resp: 12550
Ion Ratio Lower Upper
276 100
138 22.1 15.8 23.6
277 25.7 20.6 31.0

