


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
Data File : BN011717.D
Acq On : 05 Sep 2020 01:23
Operator : CG/JU
Sample : L3840-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AA5

Manual Integrations
APPROVED

mohammad
9/8/2020 1:47:21 PM

Quant Time: Sep 05 06:07:07 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 05 05:40:34 2020
Response via : Initial Calibration

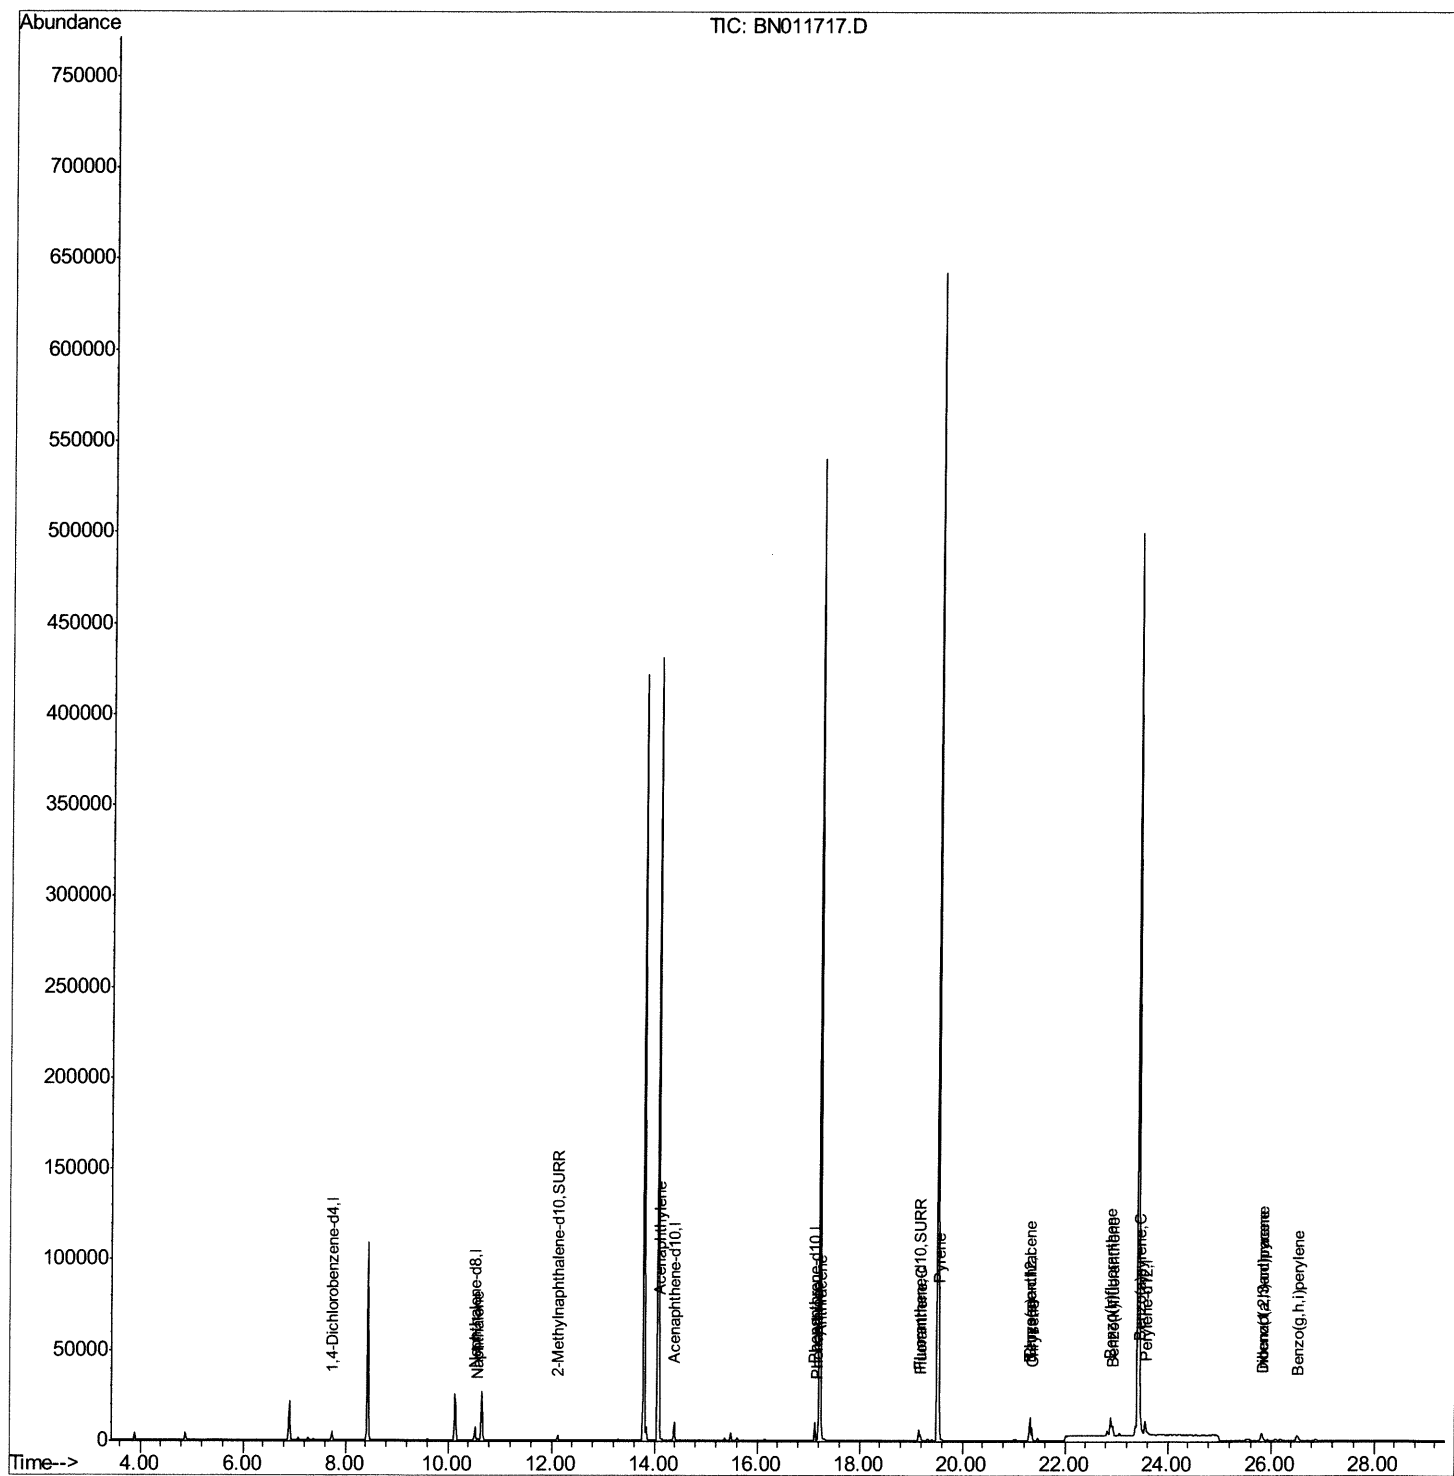

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
 Data File : BN011717.D
 Acq On : 05 Sep 2020 01:23
 Operator : CG/JU
 Sample : L3840-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA5

Manual Integrations
 APPROVED

mohammad
 9/8/2020 1:47:21 PM

Quant Time: Sep 05 06:01:31 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 05 05:40:34 2020
 Response via : Initial Calibration

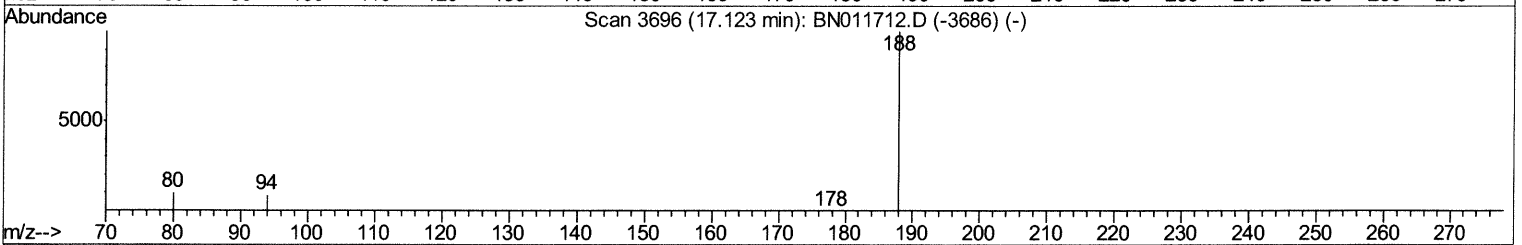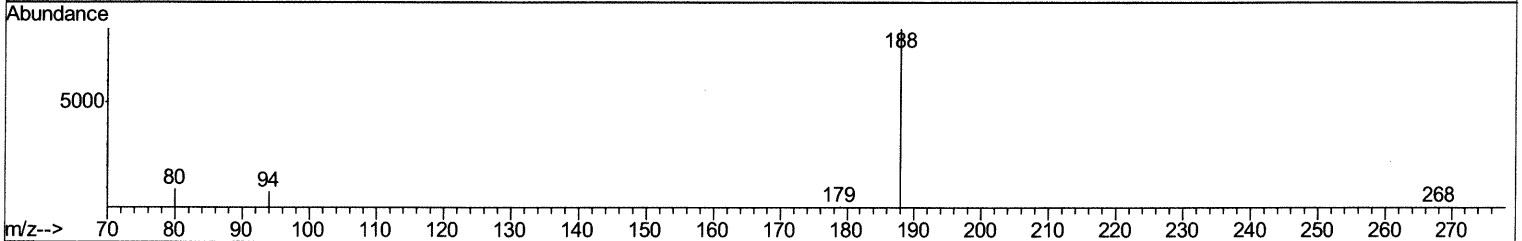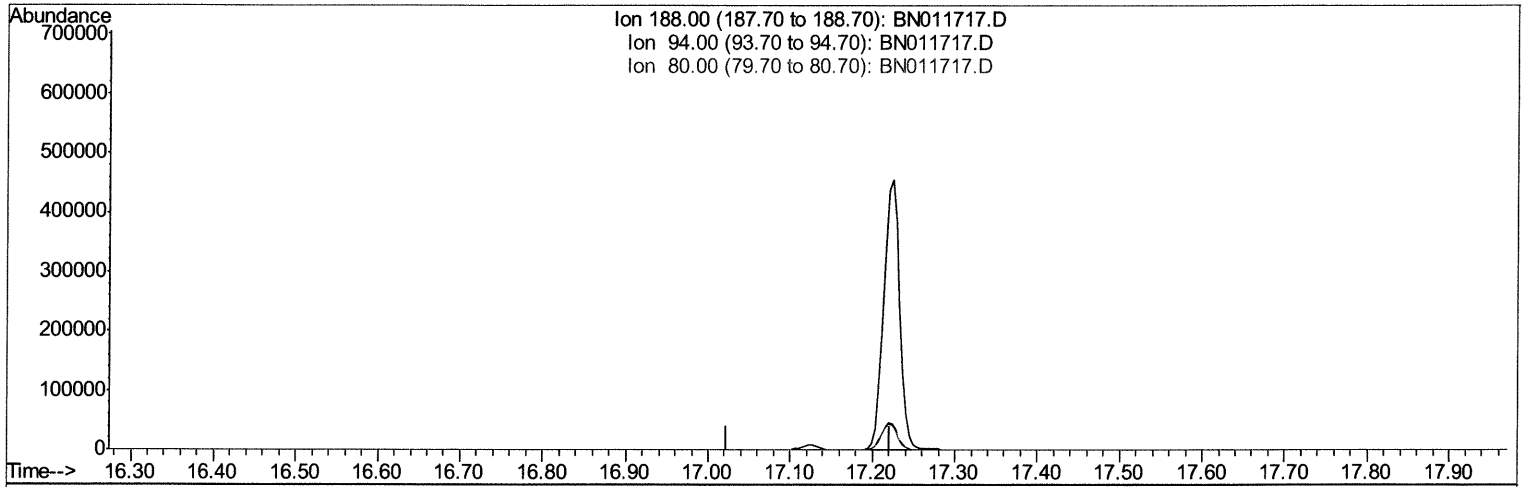

TIC: BN011717.D

(10) Phenanthrene-d10 (I)
 17.123min (-17.123) 0.00ng/ul
 response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	8.20	0.00#
80.00	9.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
 Data File : BN011717.D
 Acq On : 05 Sep 2020 01:23
 Operator : CG/JU
 Sample : L3840-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA5

Manual Integrations
 APPROVED

mohammad
 9/8/2020 1:47:21 PM

Quant Time: Sep 05 06:01:31 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 05 05:40:34 2020
 Response via : Initial Calibration

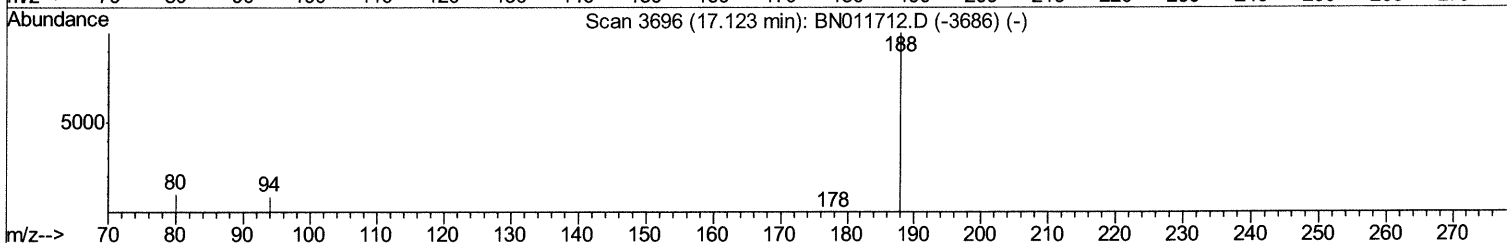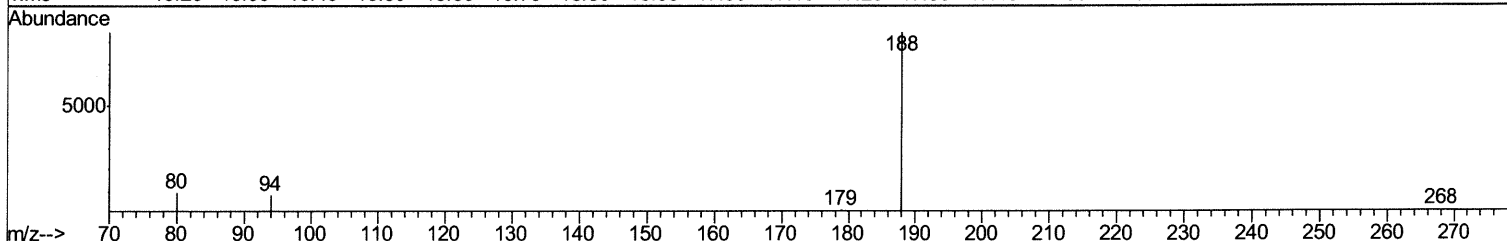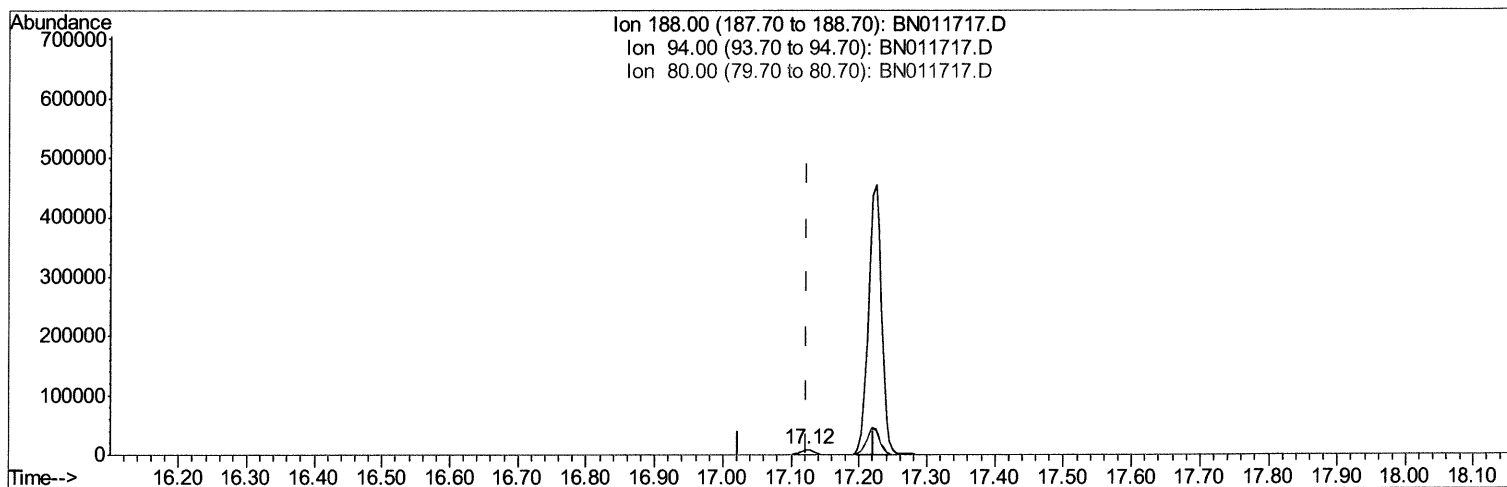

TIC: BN011717.D

(10) Phenanthrene-d10 (I)

17.123min (-0.000) 0.40ng/ul m 09/09/20 JY

response 11452

Ion	Exp%	Act%
188.00	100	100
94.00	8.20	9.17
80.00	9.00	10.52
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
 Data File : BN011717.D
 Acq On : 05 Sep 2020 01:23
 Operator : CG/JU
 Sample : L3840-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA5

Manual Integrations
 APPROVED

mohammad
 9/8/2020 1:47:21 PM

Quant Time: Sep 05 06:05:48 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 05 05:40:34 2020
 Response via : Initial Calibration

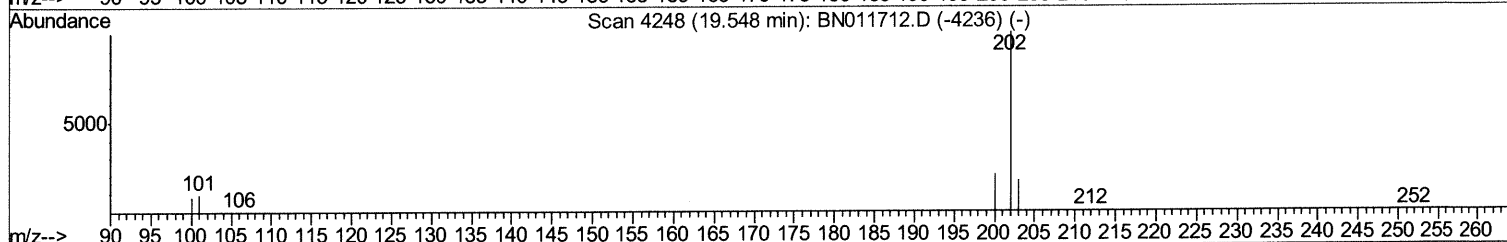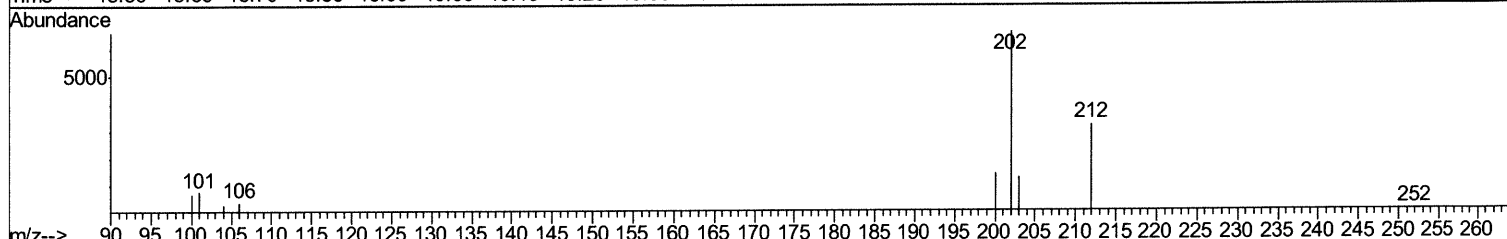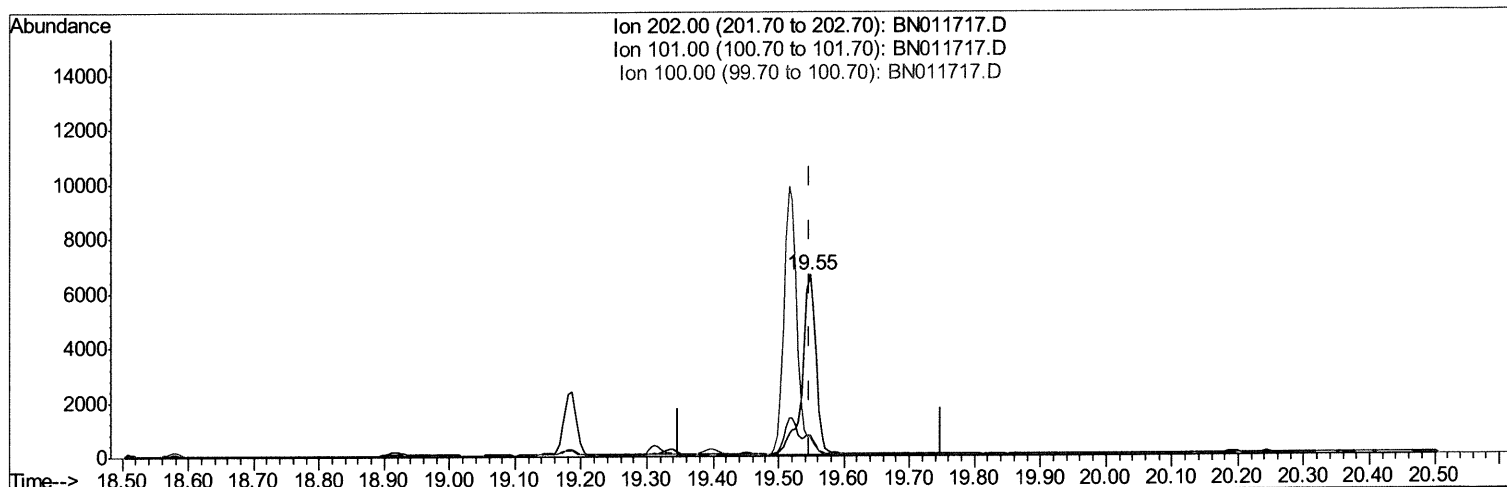

TIC: BN011717.D

(17) Pyrene

19.548min (-0.000) 0.25ng/ul

response 9819

Ion	Exp%	Act%
202.00	100	100
101.00	9.10	11.49#
100.00	8.40	10.19#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
 Data File : BN011717.D
 Acq On : 05 Sep 2020 01:23
 Operator : CG/JU
 Sample : L3840-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 C0AA5

Manual Integrations
APPROVED

mohammad
 9/8/2020 1:47:21 PM

Quant Time: Sep 05 06:05:48 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 05 05:40:34 2020
 Response via : Initial Calibration

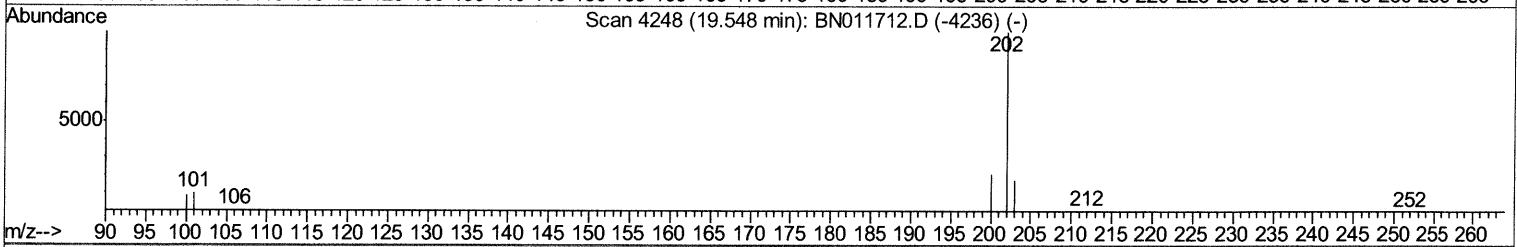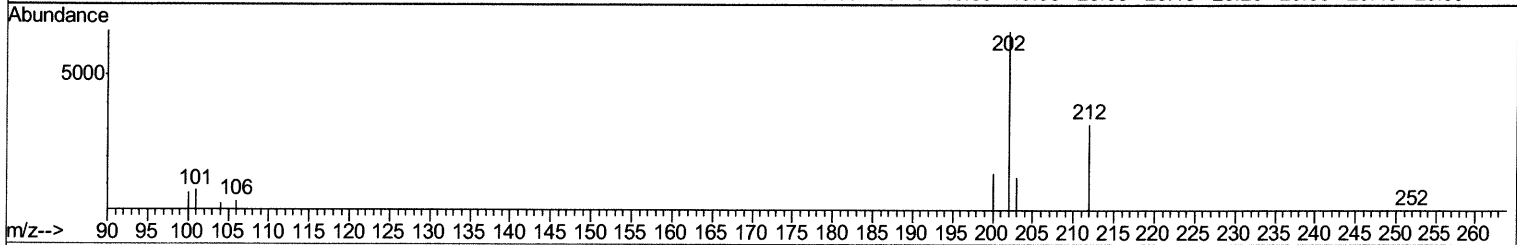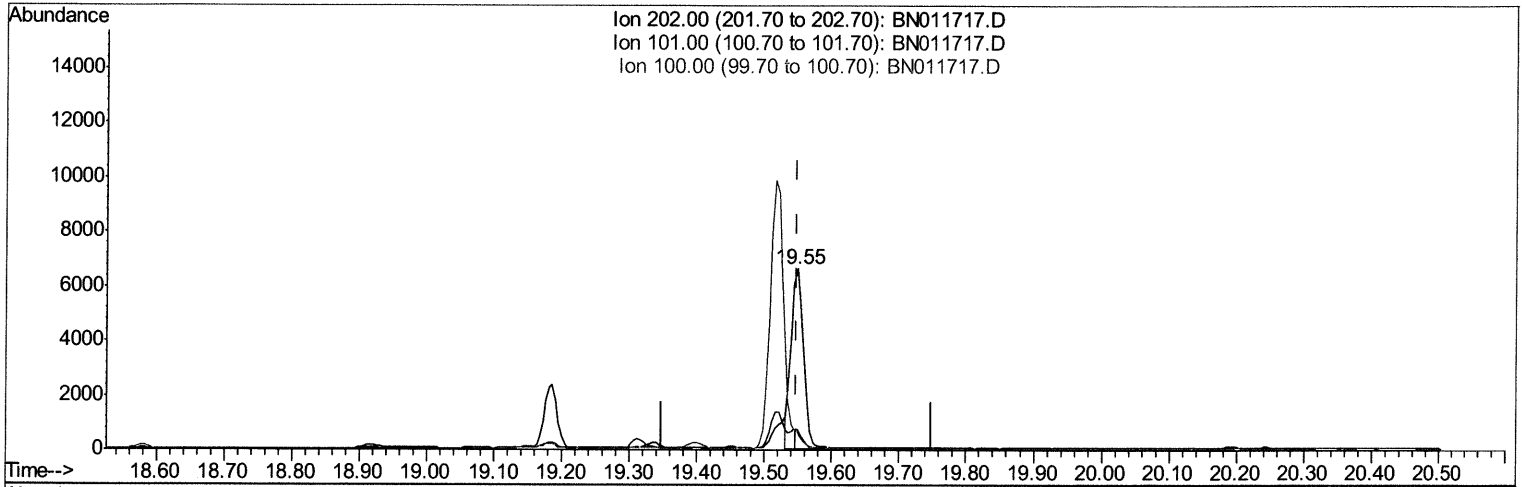

TIC: BN011717.D

(17) Pyrene

19.548min (-0.000) 0.22ng/ul m 09/09/20 JU

response 8587

Ion	Exp%	Act%
202.00	100	100
101.00	9.10	11.49#
100.00	8.40	10.19#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
 Data File : BN011717.D
 Acq On : 05 Sep 2020 01:23
 Operator : CG/JU
 Sample : L3840-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA5

Manual Integrations
 APPROVED

mohammad
 9/8/2020 1:47:21 PM

Quant Time: Sep 05 06:05:48 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 05 05:40:34 2020
 Response via : Initial Calibration

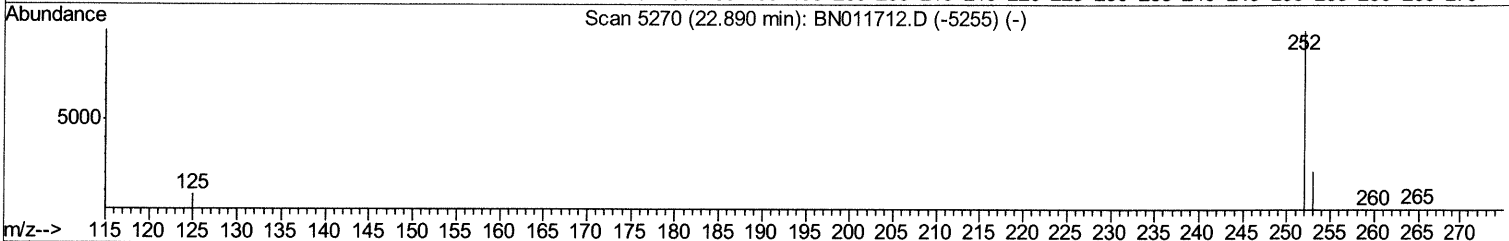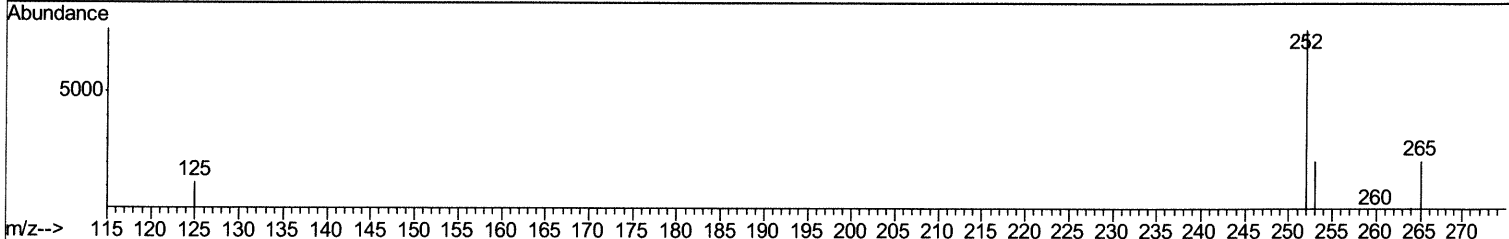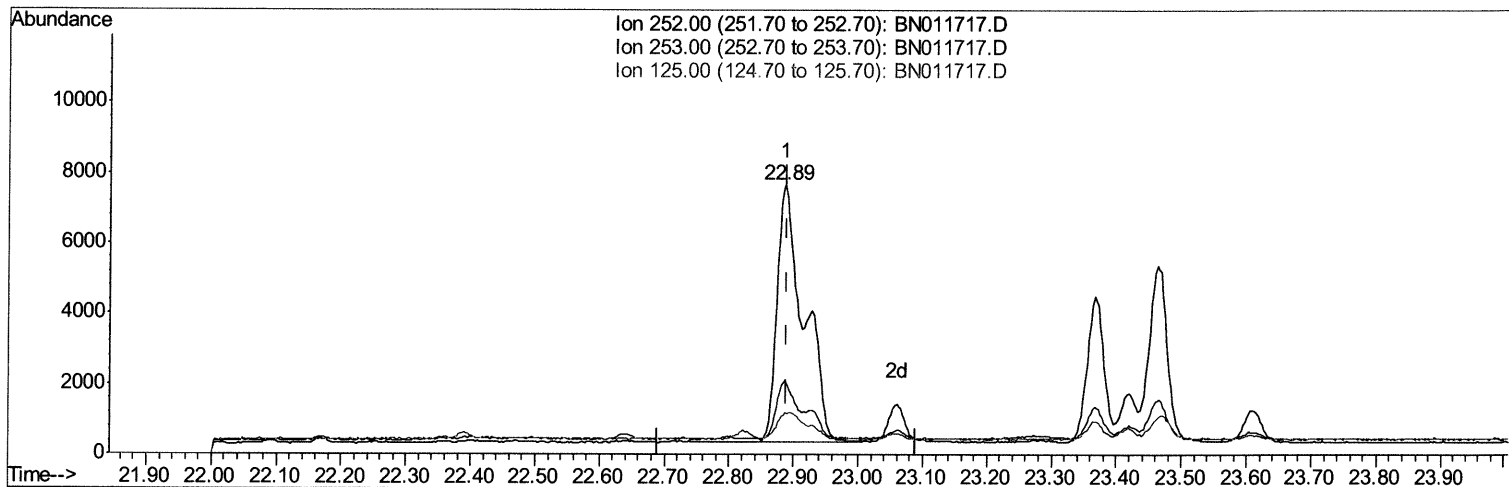

TIC: BN011717.D

(21) Benzo(b)fluoranthene
 22.887min (-0.003) 0.47ng/ul
 response 21315

Ion	Exp%	Act%
252.00	100	100
253.00	27.40	27.25
125.00	11.10	15.25
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
 Data File : BN011717.D
 Acq On : 05 Sep 2020 01:23
 Operator : CG/JU
 Sample : L3840-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA5

Manual Integrations
 APPROVED

mohammad
 9/8/2020 1:47:21 PM

Quant Time: Sep 05 06:05:48 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 05 05:40:34 2020
 Response via : Initial Calibration

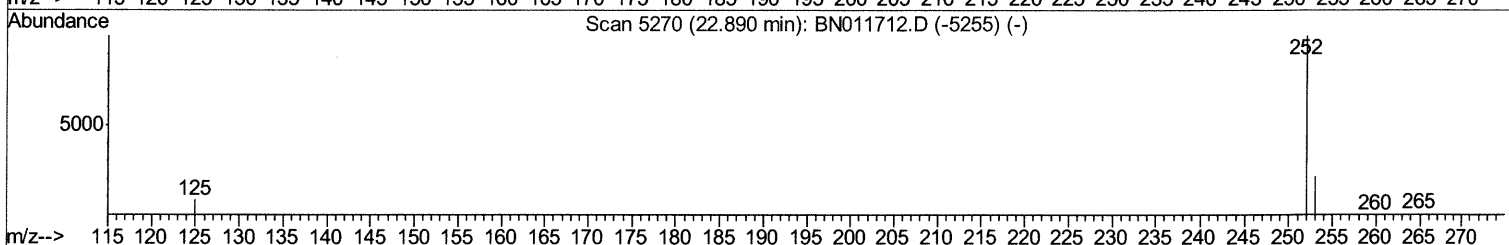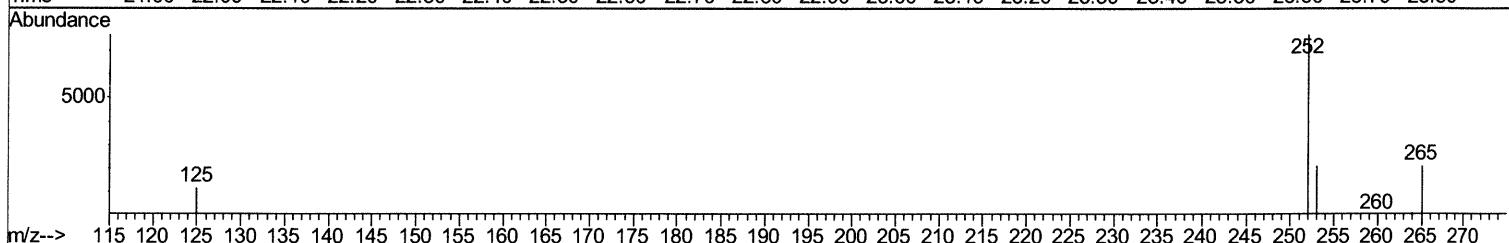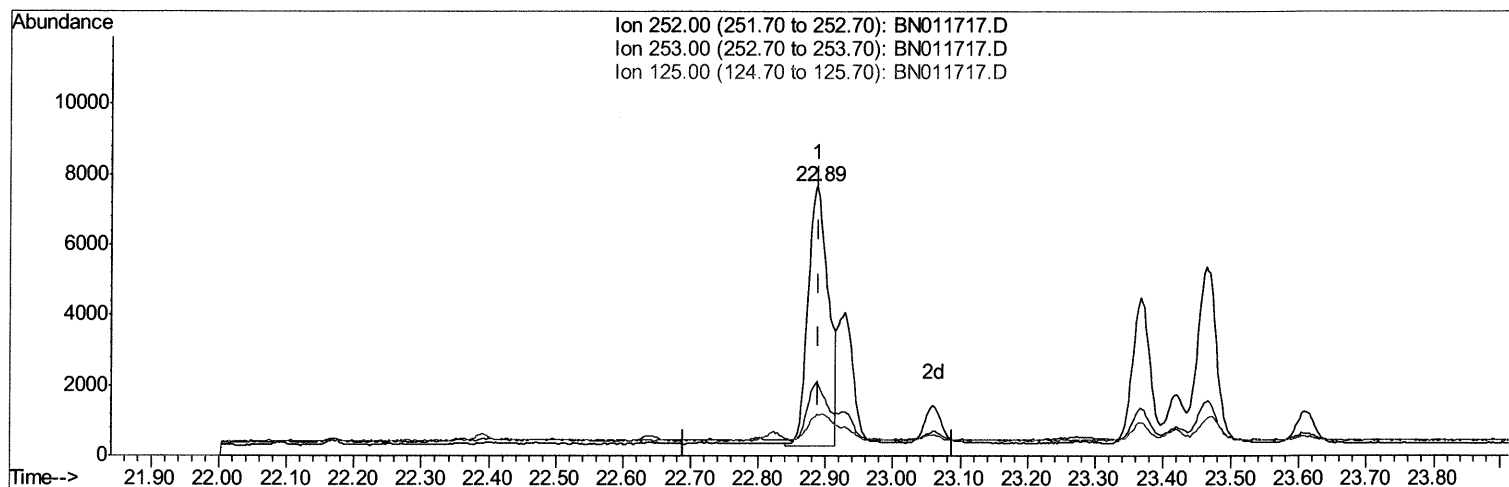

TIC: BN011717.D

(21) Benzo(b)fluoranthene

22.887min (-0.003) 0.34ng/ul m 09/09/20 JU

response 15277

Ion	Exp%	Act%
252.00	100	100
253.00	27.40	27.25
125.00	11.10	15.25
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
 Data File : BN011717.D
 Acq On : 05 Sep 2020 01:23
 Operator : CG/JU
 Sample : L3840-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 C0AA5

Manual Integrations
APPROVED

mohammad
 9/8/2020 1:47:21 PM

Quant Time: Sep 05 06:05:48 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 05 05:40:34 2020
 Response via : Initial Calibration

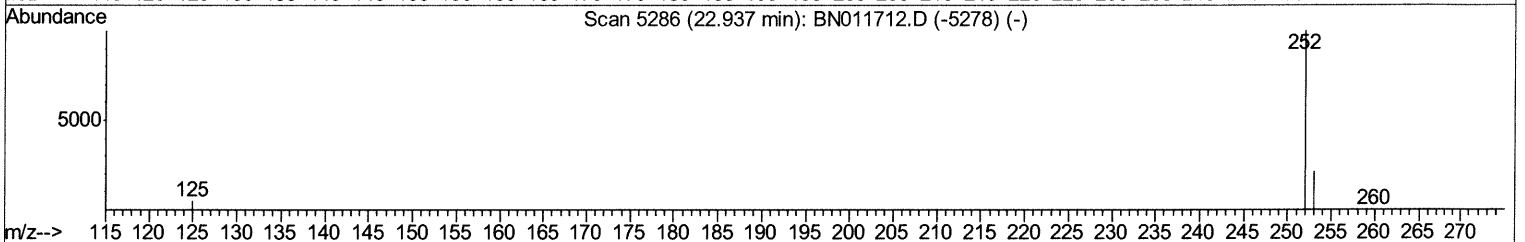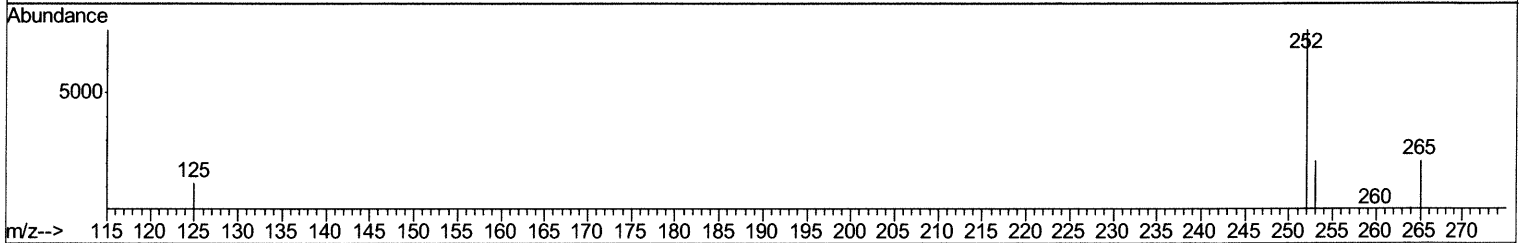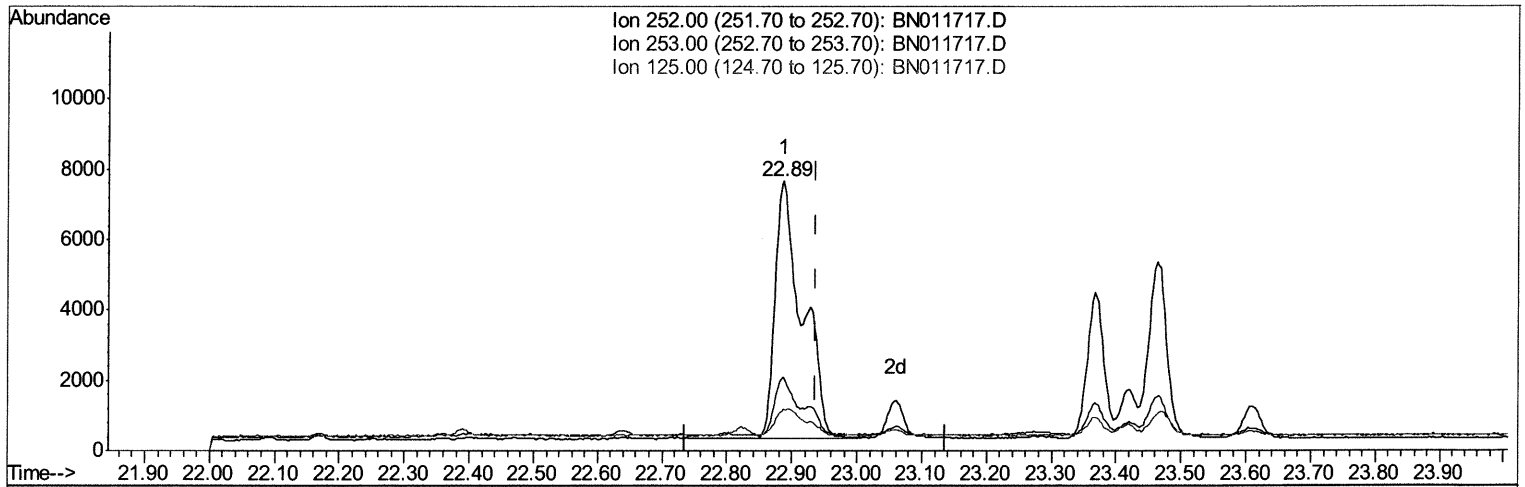

TIC: BN011717.D

(22) Benzo(k)fluoranthene
 22.887min (-0.050) 0.43ng/ul
 response 21315

Ion	Exp%	Act%
252.00	100	100
253.00	27.20	27.25
125.00	11.40	15.25#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
Data File : BN011717.D
Acq On : 05 Sep 2020 01:23
Operator : CG/JU
Sample : L3840-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AA5

Manual Integrations
APPROVED

mohammad
9/8/2020 1:47:21 PM

Quant Time: Sep 05 06:05:48 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 05 05:40:34 2020
Response via : Initial Calibration

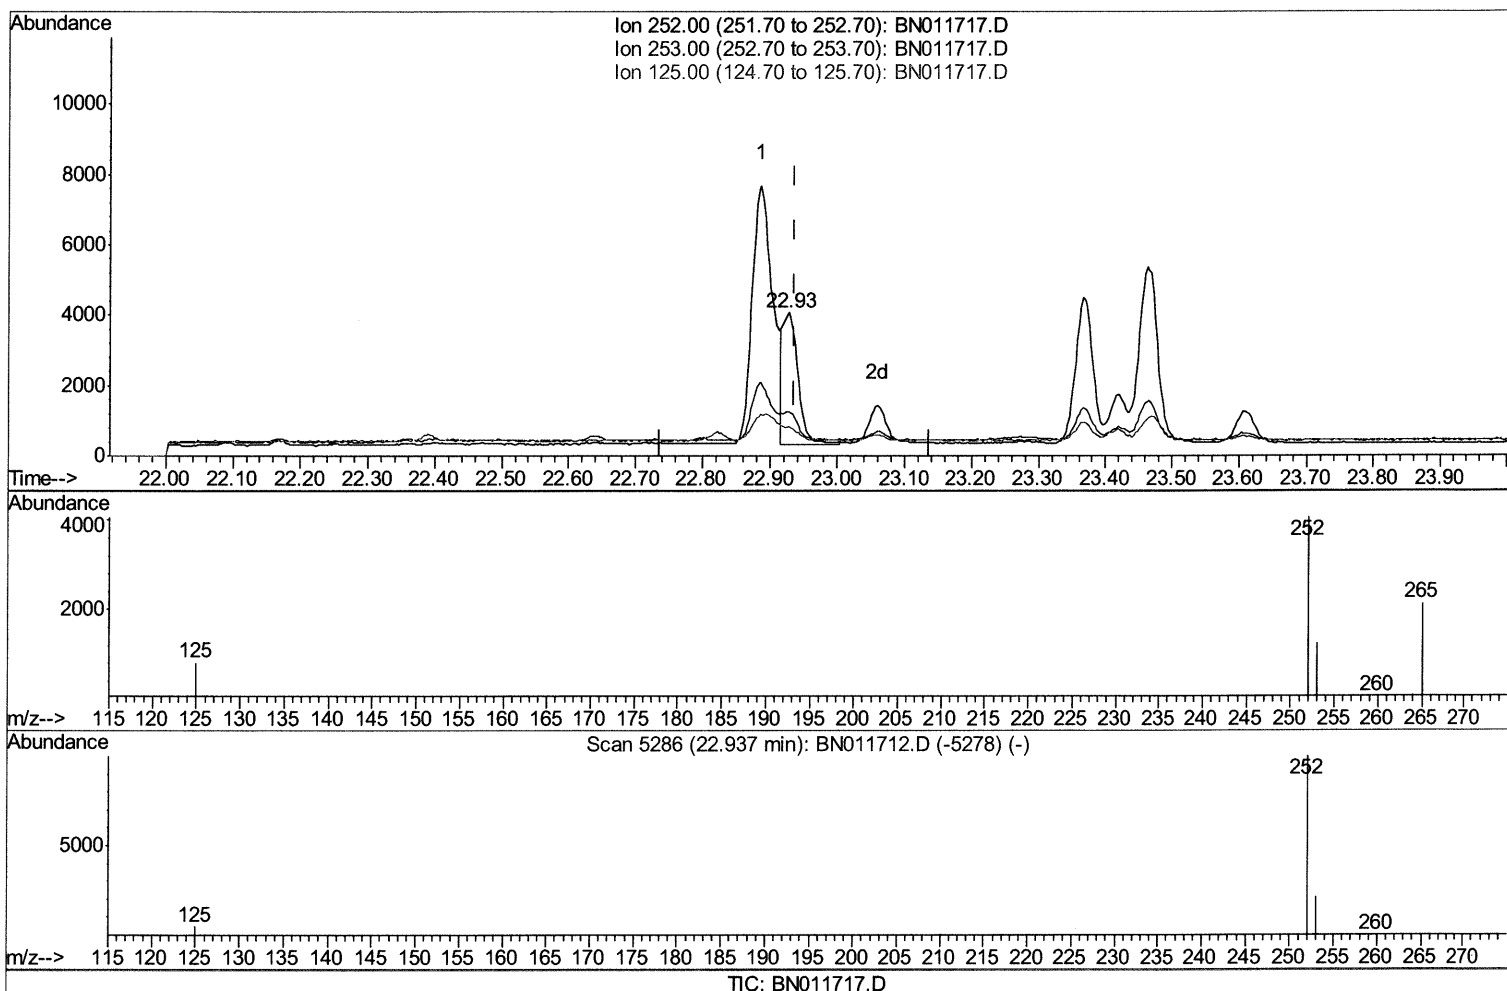

(22) Benzo(k)fluoranthene

22.928min (-0.009) 0.12ng/ul m 09/09/20 JY

response 5795

Ion	Exp%	Act%
252.00	100	100
253.00	27.20	30.97
125.00	11.40	20.20#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
 Data File : BN011717.D
 Acq On : 05 Sep 2020 01:23
 Operator : CG/JU
 Sample : L3840-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA5

Manual Integrations
 APPROVED

mohammad
 9/8/2020 1:47:21 PM

Quant Time: Sep 05 06:07:07 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 05 05:40:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	2417	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	9440	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.38	164	5353	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.12	188	11452m>	0.40	ng/ul>	0.00
16) Chrysene-d12	21.31	240	10093	0.40	ng/ul	0.00
20) Perylene-d12	23.56	264	10352	0.40	ng/ul	0.00

09/09/20 JU

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.12	152	3209	0.24	ng/ul	0.00
14) Fluoranthene-d10	19.15	212	6831	0.21	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Naphthalene	10.57	128	1147	0.042	ng/ul#	87
7) Acenaphthylene	14.10	152	1254	0.047	ng/ul#	91
12) Phenanthrene	17.16	178	1160	0.030	ng/ul#	90
13) Anthracene	17.25	178	1395	0.044	ng/ul#	91
15) Fluoranthene	19.19	202	3082	0.069	ng/ul	94
17) Pyrene	19.55	202	8587m>	0.218	ng/ul>	94
18) Benzo(a)anthracene	21.30	228	3132	0.092	ng/ul	92
19) Chrysene	21.35	228	6786	0.149	ng/ul	98
21) Benzo(b)fluoranthene	22.89	252	15277m3	0.340	ng/ul3	93
22) Benzo(k)fluoranthene	22.93	252	5795m3	0.116	ng/ul3	93
23) Benzo(a)pyrene	23.46	252	9589	0.254	ng/ul#	93
24) Indeno(1,2,3-cd)pyrene	25.82	276	6911	0.135	ng/ul	99
25) Dibenzo(a,h)anthracene	25.83	278	2005	0.048	ng/ul#	70
26) Benzo(a,h,i)perylene	26.51	276	6576	0.137	ng/ul	95

09/09/20 JU

09/09/20 JU

(#) = qualifier out of range (m) = manual integration (+) = signals summed