


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
Data File : BN011718.D
Acq On : 05 Sep 2020 02:00
Operator : CG/JU
Sample : L3840-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE5

Manual Integrations
APPROVED

mohammad
9/8/2020 1:47:24 PM

Quant Time: Sep 05 06:13:57 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 05 05:40:34 2020
Response via : Initial Calibration

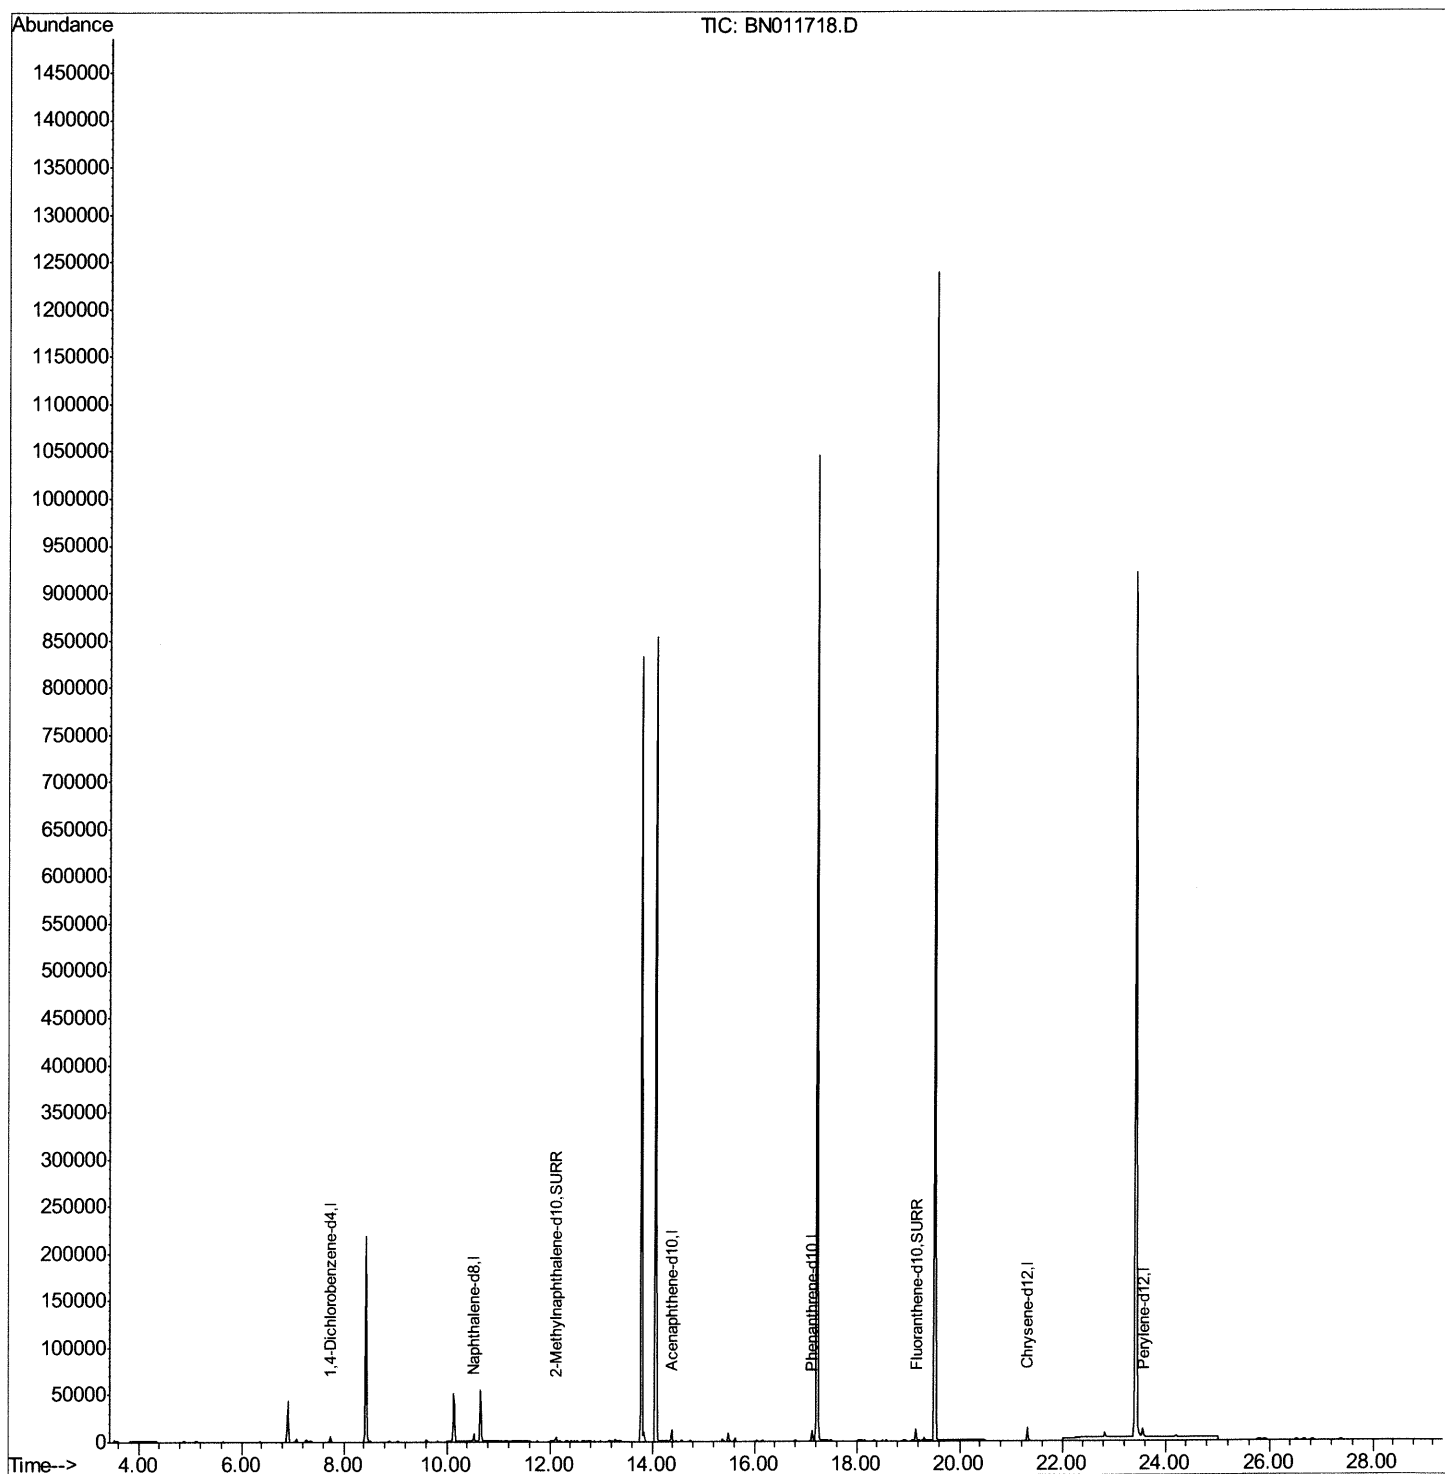

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
 Data File : BN011718.D
 Acq On : 05 Sep 2020 02:00
 Operator : CG/JU
 Sample : L3840-09
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE5

Manual Integrations
 APPROVED

mohammad
 9/8/2020 1:47:24 PM

Quant Time: Sep 05 06:01:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 05 05:40:34 2020
 Response via : Initial Calibration

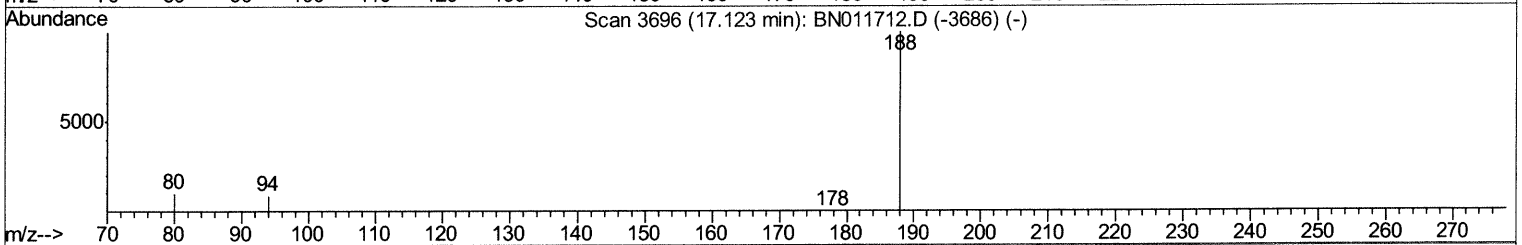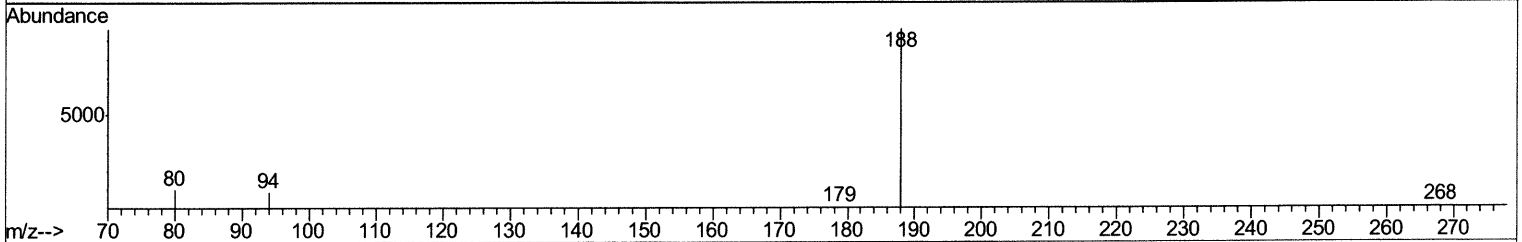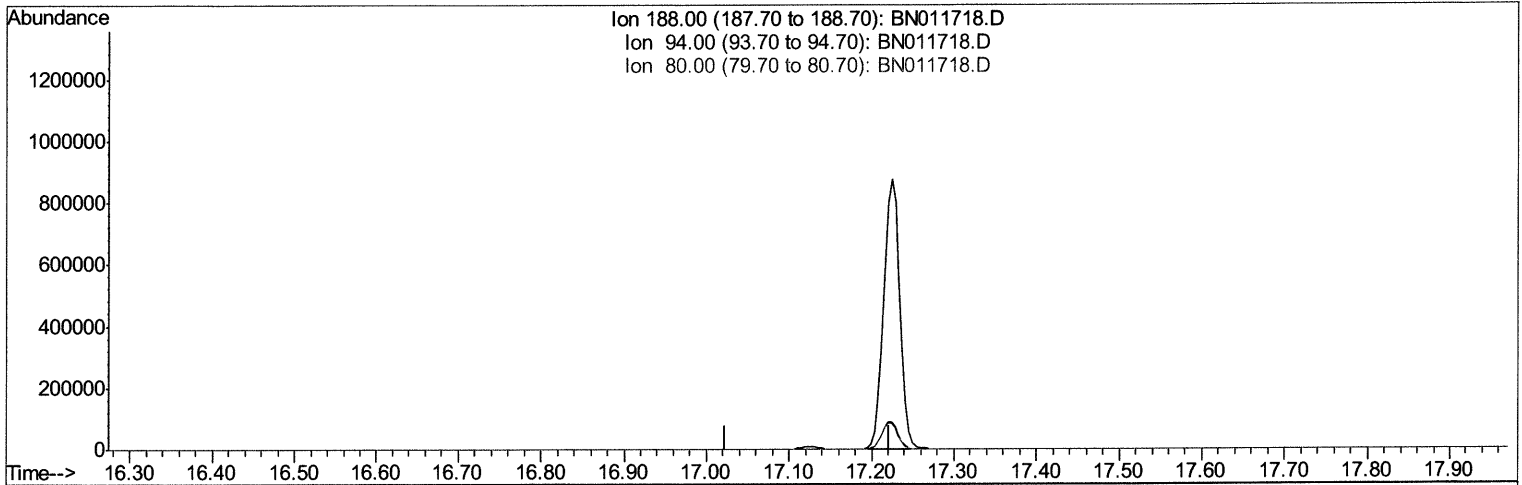

TIC: BN011718.D

(10) Phenanthrene-d10 (I)

17.123min (-17.123) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	8.20	0.00#
80.00	9.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
 Data File : BN011718.D
 Acq On : 05 Sep 2020 02:00
 Operator : CG/JU
 Sample : L3840-09
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE5

Manual Integrations
 APPROVED

mohammad
 9/8/2020 1:47:24 PM

Quant Time: Sep 05 06:01:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 05 05:40:34 2020
 Response via : Initial Calibration

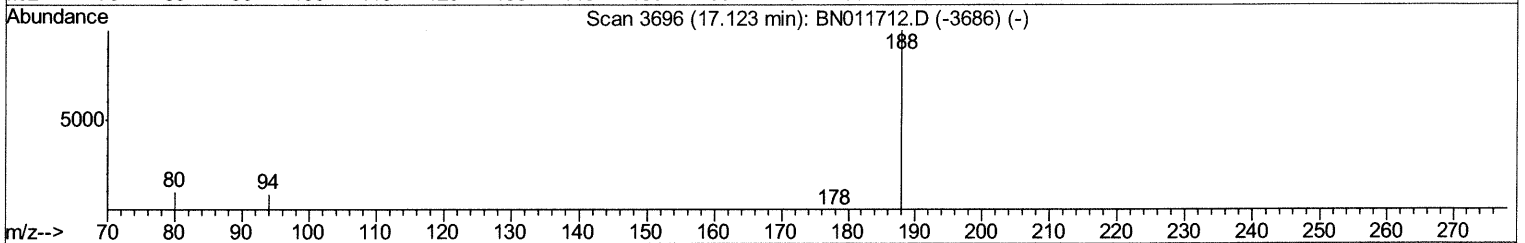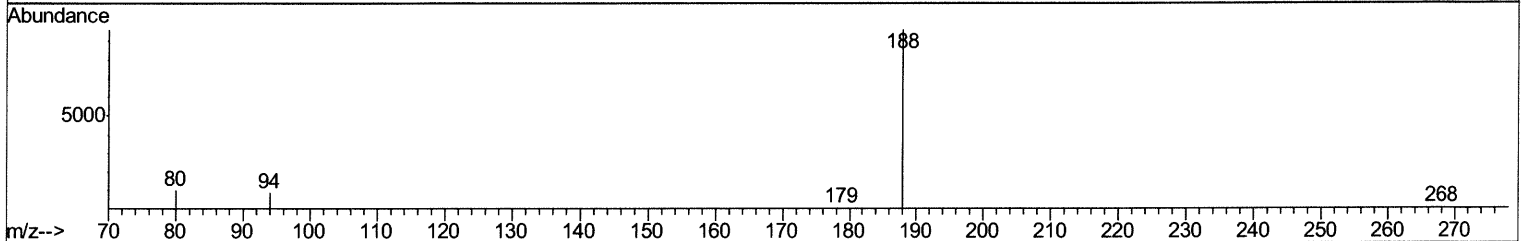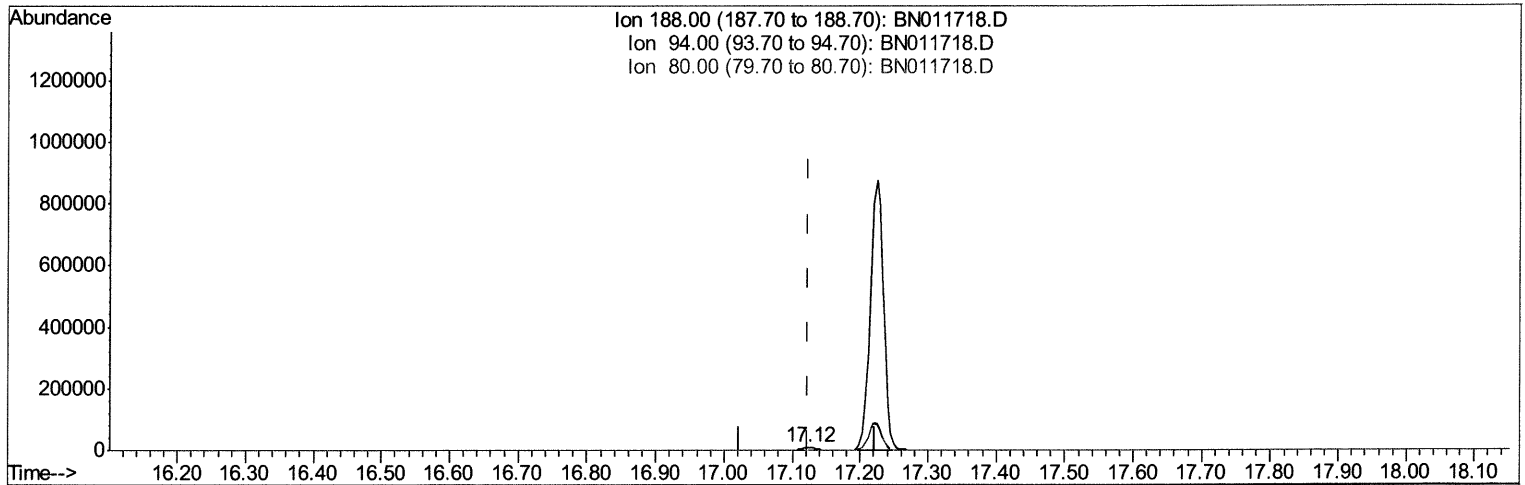

TIC: BN011718.D

(10) Phenanthrene-d10 (I)

17.123min (+0.000) 0.40ng/ul m 09/09/20 Jy

response 13159

Ion	Exp%	Act%
188.00	100	100
94.00	8.20	9.25
80.00	9.00	10.45
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
Data File : BN011718.D
Acq On : 05 Sep 2020 02:00
Operator : CG/JU
Sample : L3840-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE5

Manual Integrations
APPROVED

mohammad
9/8/2020 1:47:24 PM

Quant Time: Sep 05 06:13:57 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 05 05:40:34 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	2608	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	10344	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.38	164	6364	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.12	188	13159m>	0.40	ng/ul>	0.00
16) Chrysene-d12	21.31	240	11621	0.40	ng/ul	0.00
20) Perylene-d12	23.56	264	12130	0.40	ng/ul	0.00

09/09/20 JU

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.12	152	6428	0.44	ng/ul	0.00
14) Fluoranthene-d10	19.15	212	13397	0.36	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed