
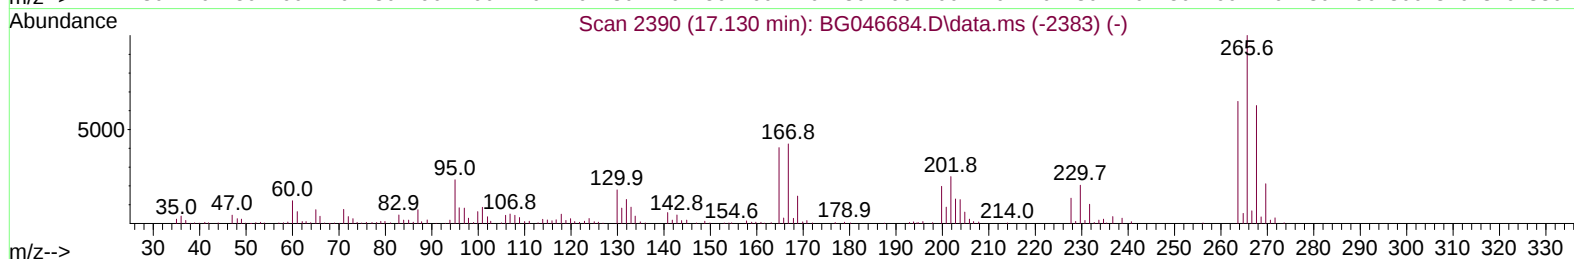
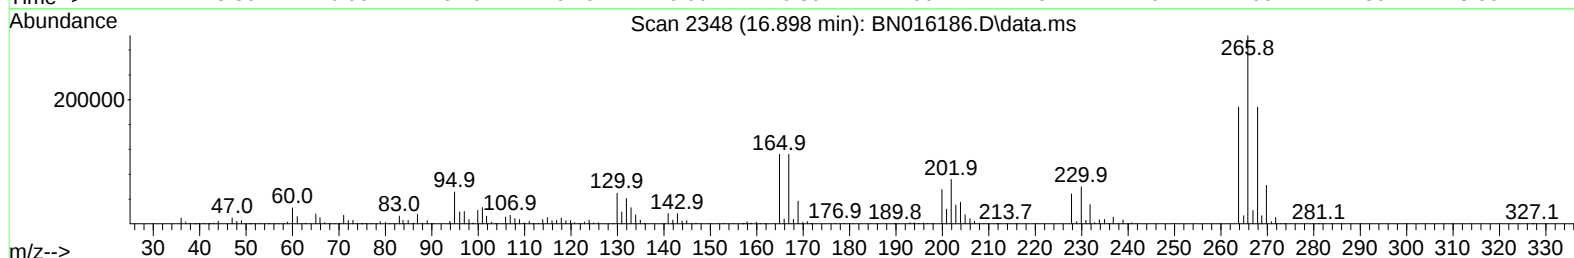


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090421\
Data File : BN016186.D
Acq On : 04 Sep 2021 10:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 02:24:08 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 17:12:56 2021
Response via : Initial Calibration

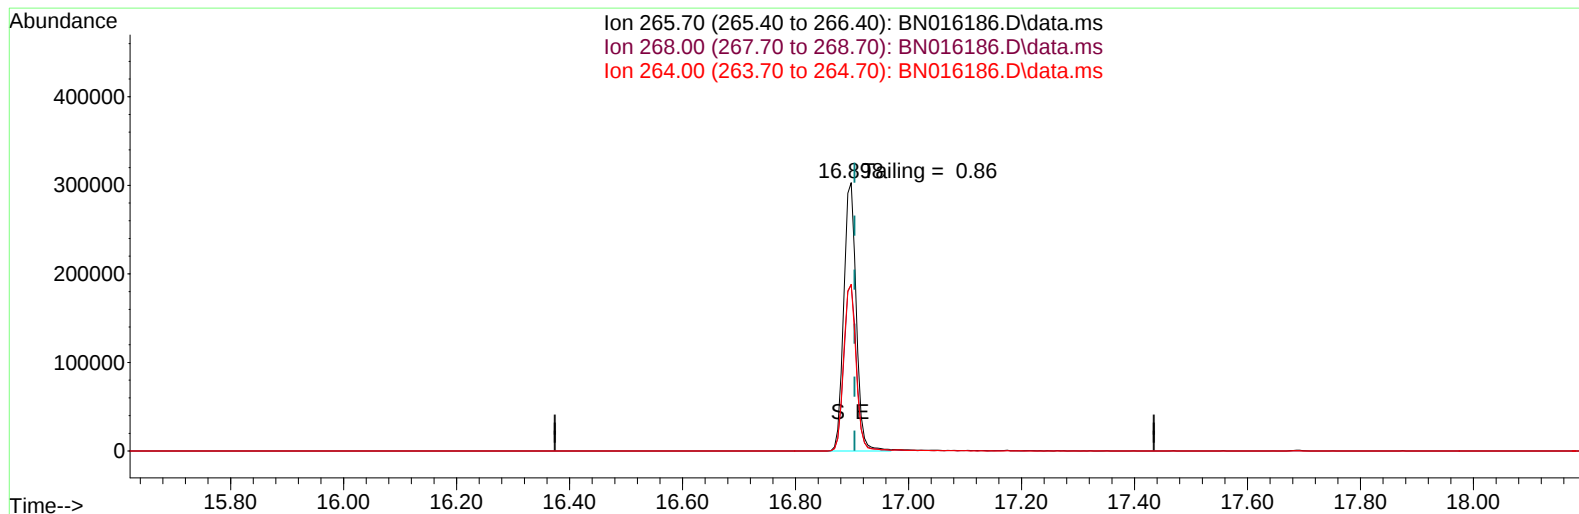

TIC: BN016186.D\data.ms

(70) Pentachlorophenol (C)




16.898min (-0.006) 27960.11 ng

response 468470

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.01
264.00	61.60	62.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090421\
Data File : BN016186.D
Acq On : 04 Sep 2021 10:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 02:24:08 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 17:12:56 2021
Response via : Initial Calibration

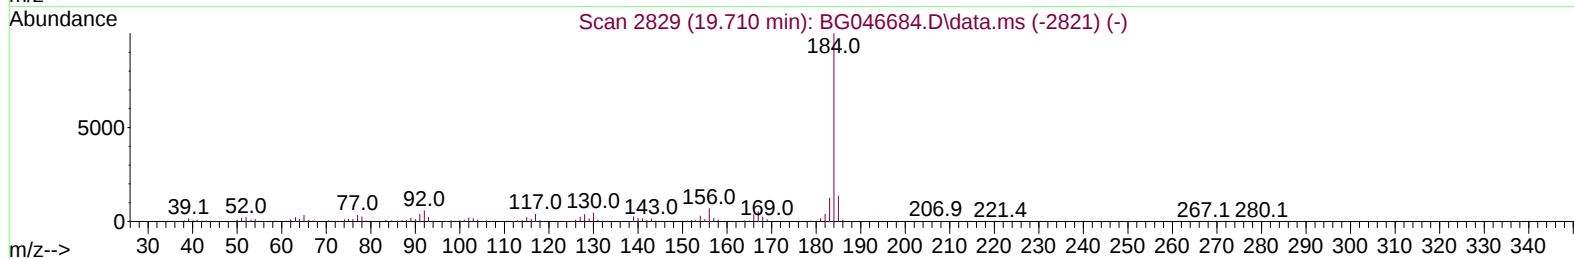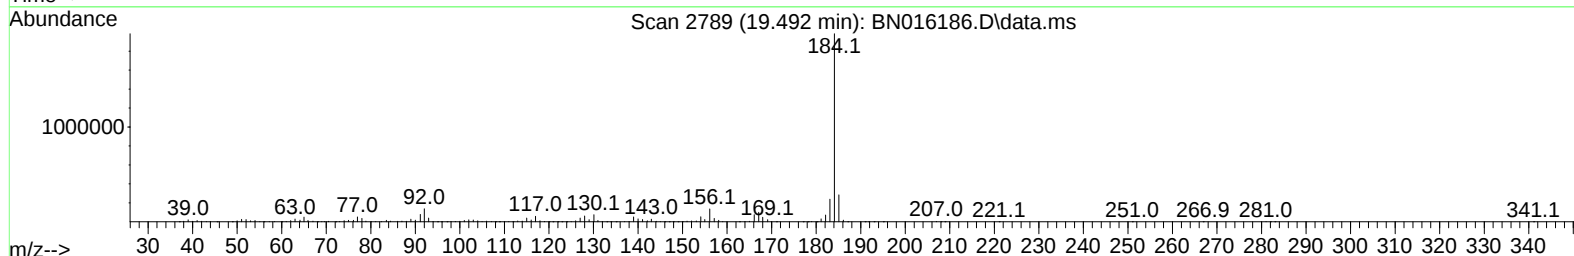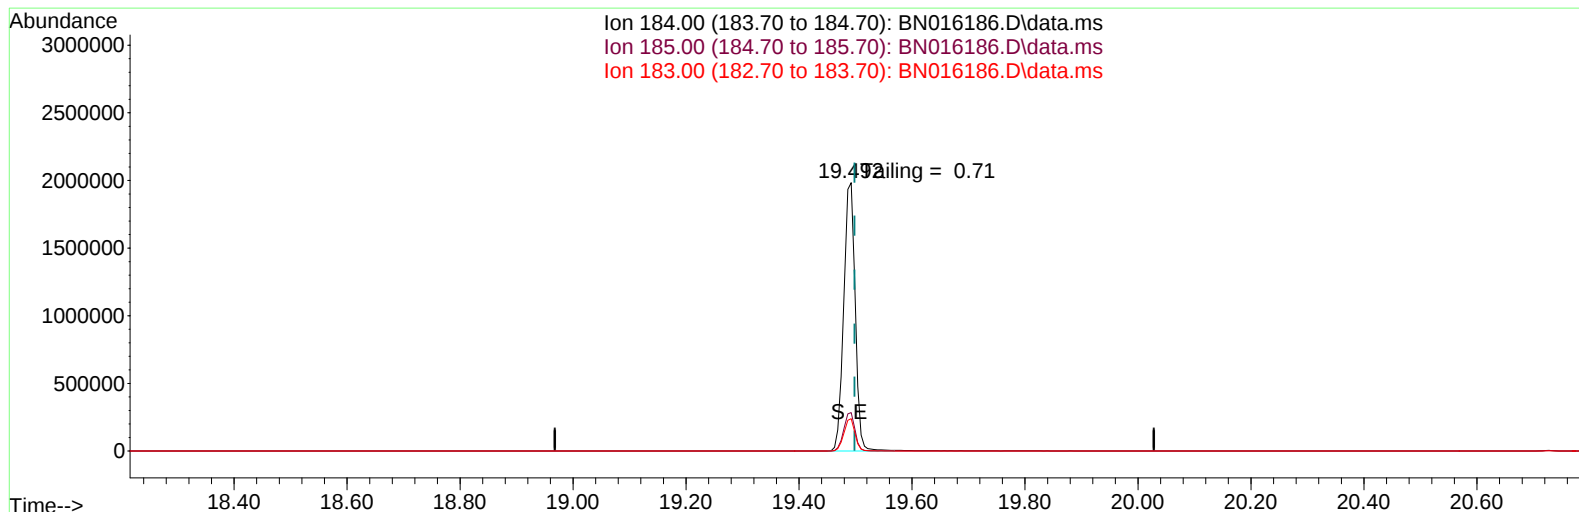

TIC: BN016186.D\data.ms

(77) Benzidine**19.492min (-0.006) 220530.10 ng****response 2800744**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.30
183.00	13.20	12.05
0.00	0.00	0.00