
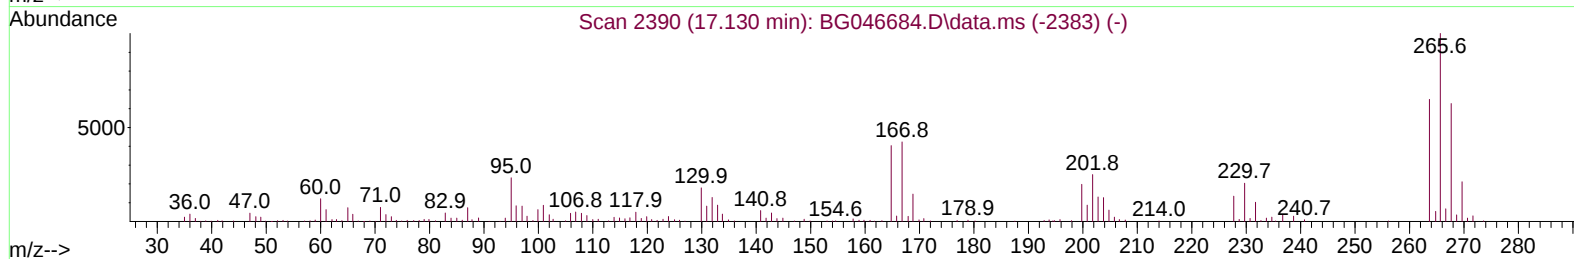
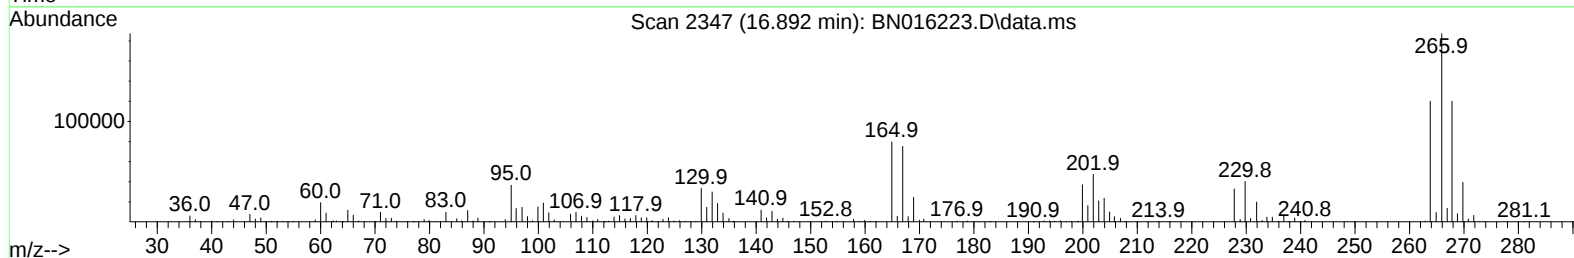


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090421\
Data File : BN016223.D
Acq On : 05 Sep 2021 11:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 36 Sample Multiplier: 1

Quant Time: Sep 06 07:37:40 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 17:12:56 2021
Response via : Initial Calibration

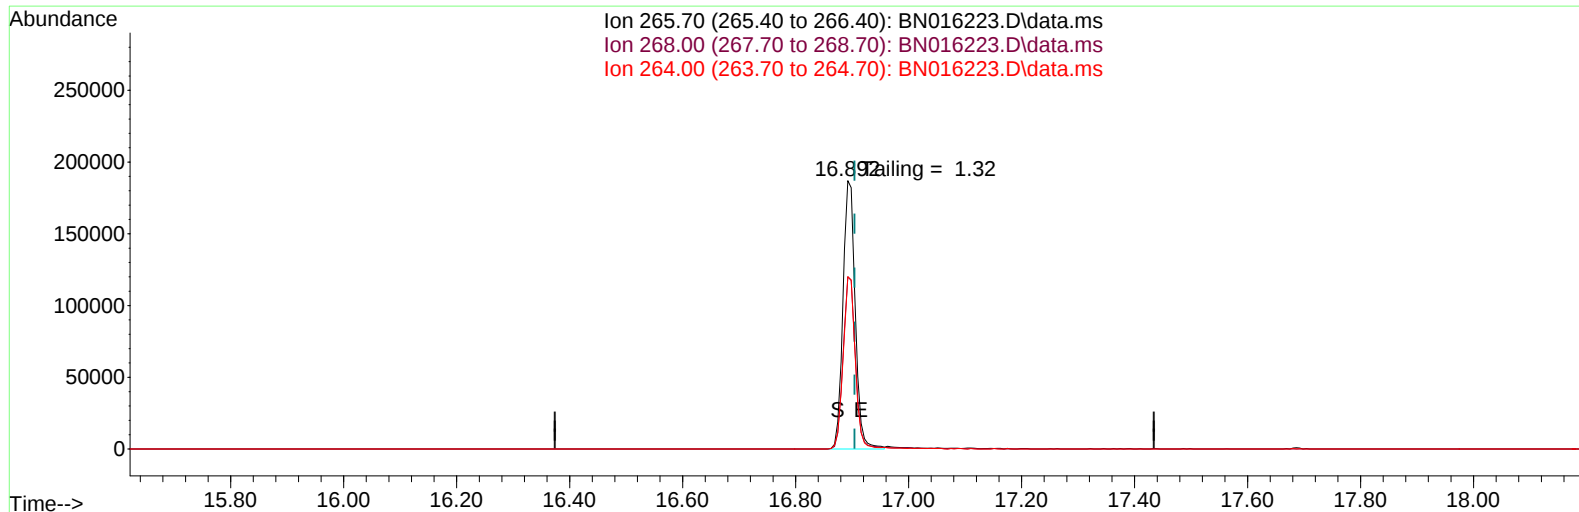

TIC: BN016223.D\data.ms

(70) Pentachlorophenol (C)




16.892min (-0.012) 19040.77 ng

response 280176

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.14
264.00	61.60	64.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090421\
 Data File : BN016223.D
 Acq On : 05 Sep 2021 11:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Quant Time: Sep 06 07:37:40 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 17:12:56 2021
 Response via : Initial Calibration

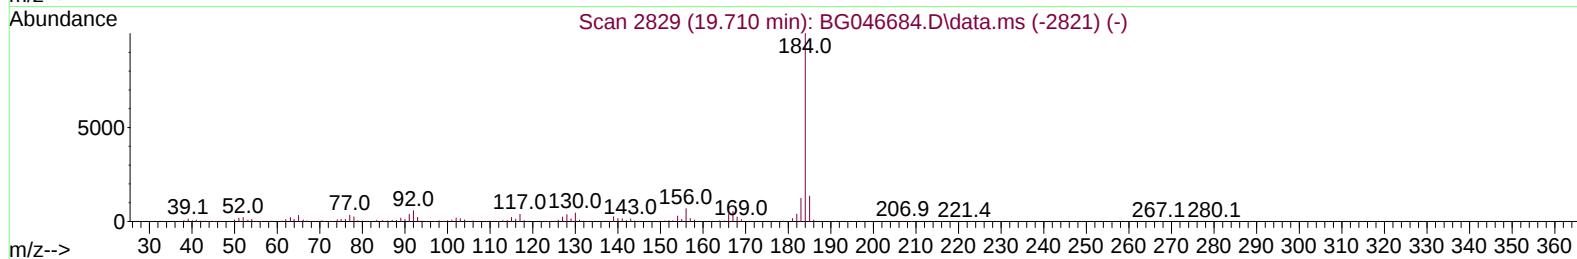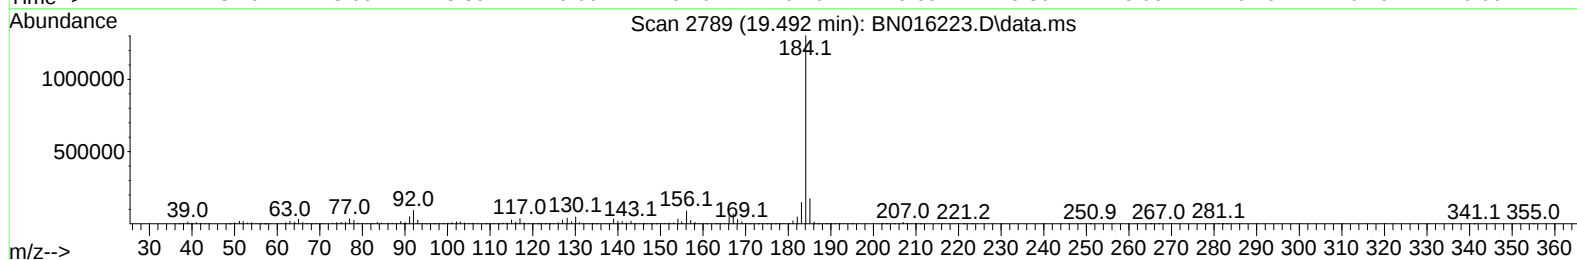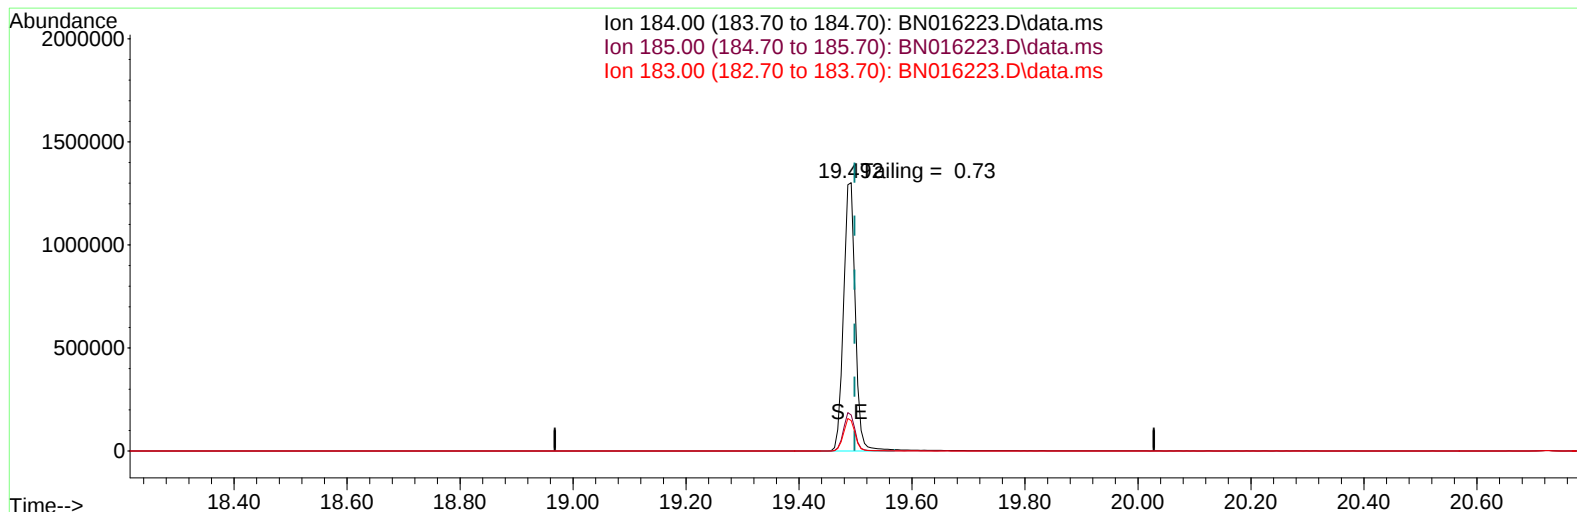

TIC: BN016223.D\data.ms

(77) Benzidine**19.492min (-0.006) 216185.09 ng****response 1885908**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.41
183.00	13.20	11.32
0.00	0.00	0.00