

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090421\
 Data File : BN016190.D
 Acq On : 04 Sep 2021 12:35
 Operator : CG/JU
 Sample : SSTDICC0.8
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

Quant Time: Sep 06 01:27:47 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN090421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 06 01:25:38 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.873	152	13144	0.400	ng	0.00
7) Naphthalene-d8	10.660	136	67399	0.400	ng	0.00
13) Acenaphthene-d10	14.497	164	39743	0.400	ng	0.00
19) Phenanthrene-d10	17.248	188	79796	0.400	ng	0.00
29) Chrysene-d12	21.429	240	83372	0.400	ng	0.00
35) Perylene-d12	23.826	264	83449	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.457	112	29356	0.933	ng	0.00
5) Phenol-d6	7.033	99	38024	0.866	ng	0.00
8) Nitrobenzene-d5	9.025	82	41786	0.943	ng	0.00
11) 2-Methylnaphthalene-d10	12.251	152	87338	0.859	ng	0.00
14) 2,4,6-Tribromophenol	15.994	330	13748	1.219	ng	0.00
15) 2-Fluorobiphenyl	13.126	172	115374	0.721	ng	0.00
27) Fluoranthene-d10	19.281	212	193022	0.858	ng	0.00
31) Terphenyl-d14	19.877	244	163000	0.797	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.373	88	3712	0.515	ng	# 70
3) n-Nitrosodimethylamine	3.742	42	8520	0.752	ng	99
6) bis(2-Chloroethyl)ether	7.301	93	28047	0.764	ng	100
9) Naphthalene	10.710	128	142275	0.803	ng	100
10) Hexachlorobutadiene	11.002	225	29240	0.743	ng	# 100
12) 2-Methylnaphthalene	12.327	142	97313	0.860	ng	99
16) Acenaphthylene	14.218	152	142821	0.977	ng	100
17) Acenaphthene	14.560	154	89037	0.796	ng	99
18) Fluorene	15.550	166	113476	0.848	ng	100
20) 4,6-Dinitro-2-methylph...	15.639	198	2392	0.450	ng	# 60
21) 4-Bromophenyl-phenylether	16.433	248	33228	0.829	ng	98
22) Hexachlorobenzene	16.555	284	39134	0.695	ng	99
23) Atrazine	16.701	200	33807	1.379	ng	99
24) Pentachlorophenol	16.895	266	7551	0.511	ng	98
25) Phenanthrene	17.285	178	176138	0.776	ng	100
26) Anthracene	17.382	178	169768	0.913	ng	100
28) Fluoranthene	19.306	202	212689	0.844	ng	100
30) Pyrene	19.673	202	216515	0.873	ng	100
32) Benzo(a)anthracene	21.418	228	222712	0.880	ng	100
33) Chrysene	21.471	228	220302	0.822	ng	100
34) Bis(2-ethylhexyl)phtha...	21.344	149	144192	2.136	ng	99
36) Indeno(1,2,3-cd)pyrene	26.301	276	192622	0.610	ng	100
37) Benzo(b)fluoranthene	23.097	252	227982	0.763	ng	98
38) Benzo(k)fluoranthene	23.145	252	210937	0.758	ng	98
39) Benzo(a)pyrene	23.720	252	202907	0.788	ng	99
40) Dibenzo(a,h)anthracene	26.322	278	161224	0.617	ng	97
41) Benzo(g,h,i)perylene	27.064	276	159988	0.593	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090421\
Data File : BN016190.D
Acq On : 04 Sep 2021 12:35
Operator : CG/JU
Sample : SSTDIC0.8
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Quant Time: Sep 06 01:27:47 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN090421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 06 01:25:38 2021
Response via : Initial Calibration




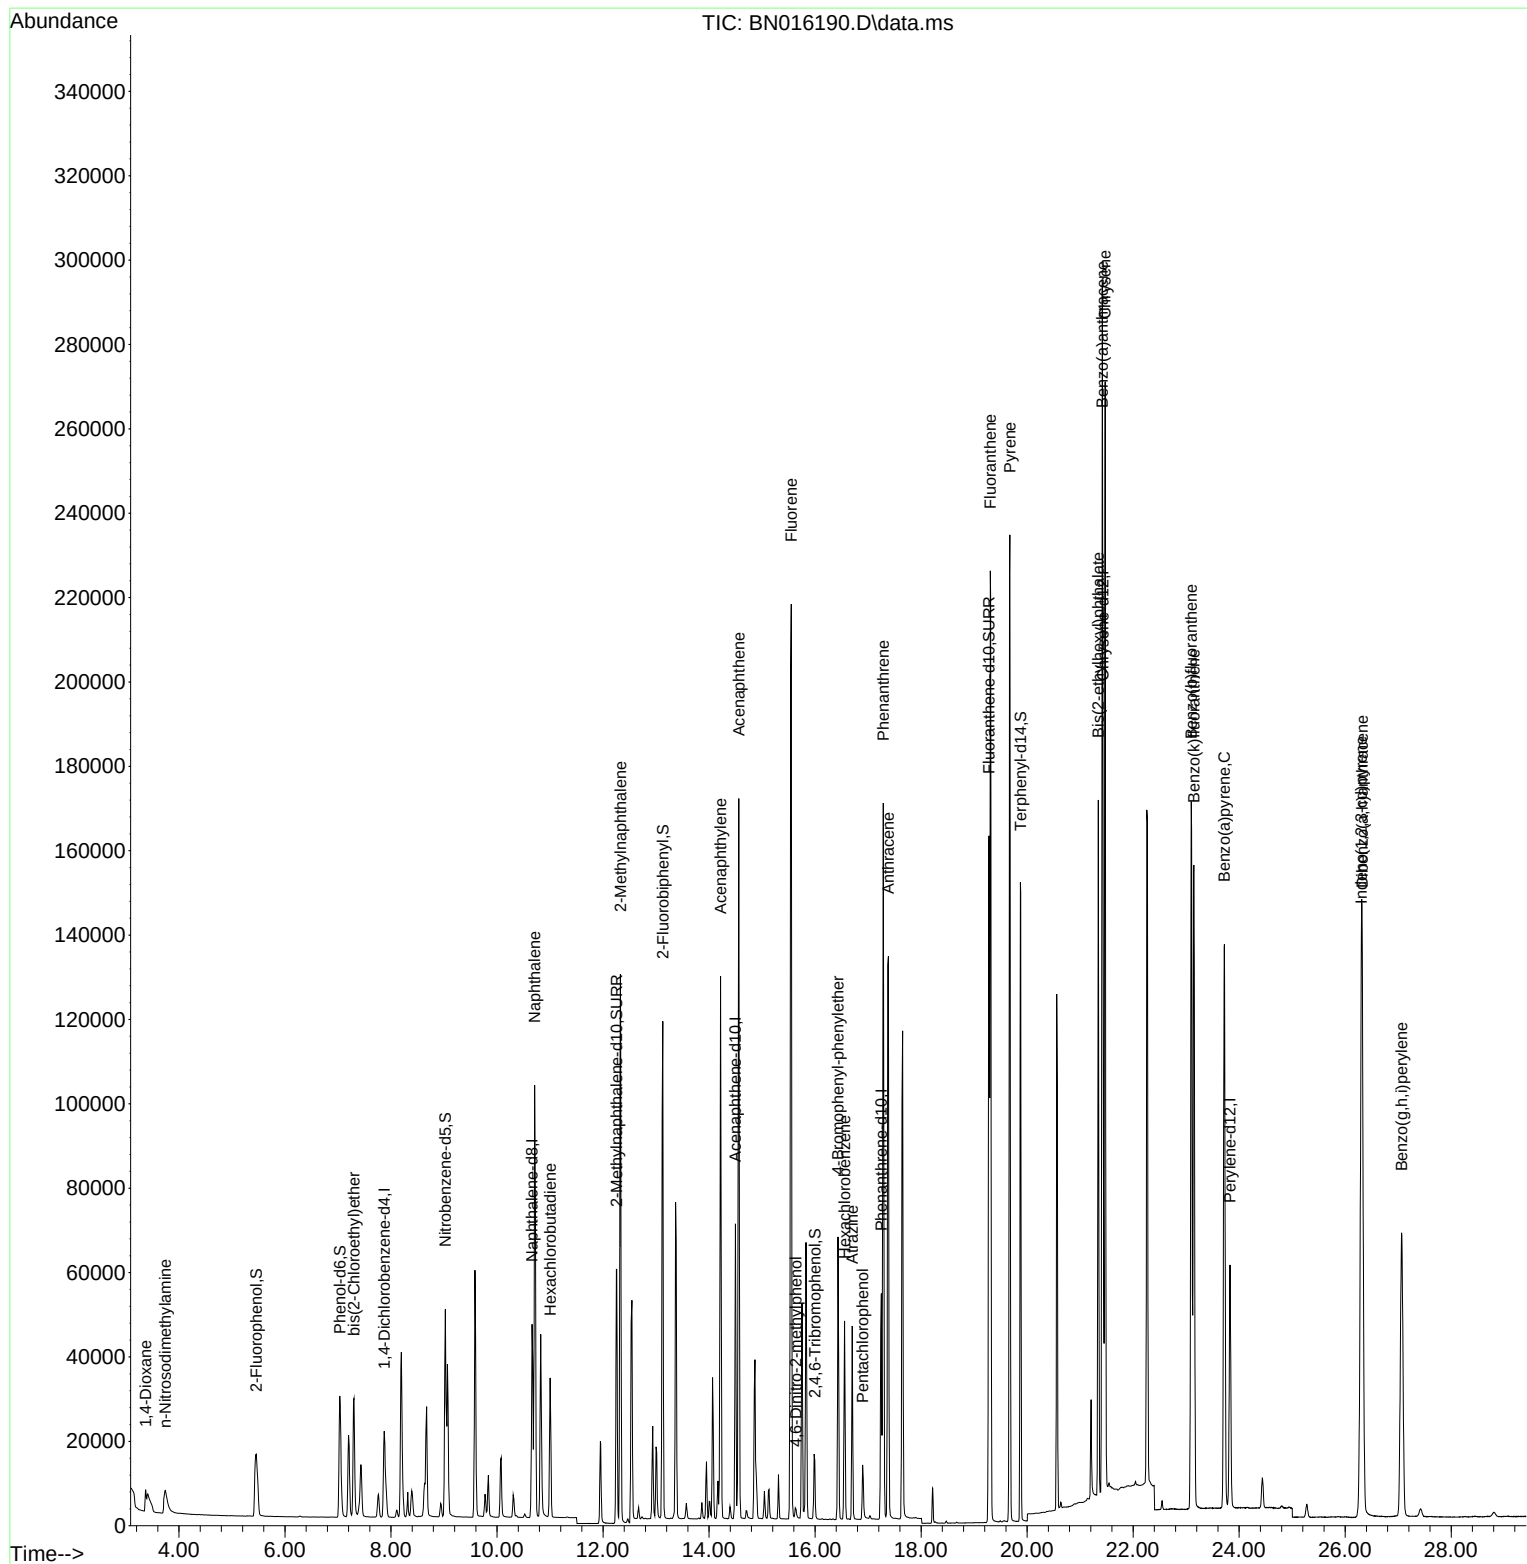


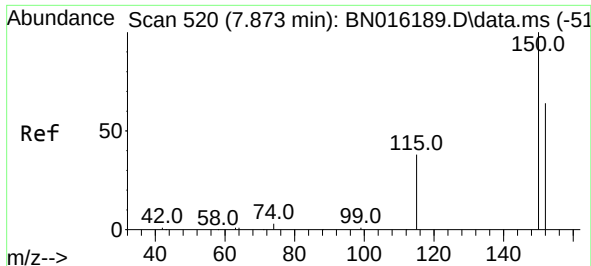

#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.873 min Scan# 520
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:152 Resp: 13144
Ion Ratio Lower Upper
152 100
150 155.4 125.3 187.9
115 60.9 48.4 72.6

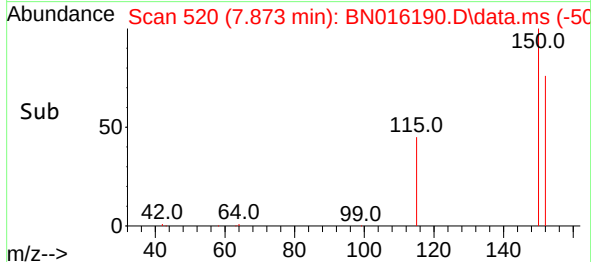

#2
1,4-Dioxane
Concen: 0.515 ng
RT: 3.373 min Scan# 32
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35

Tgt Ion: 88 Resp: 3712
Ion Ratio Lower Upper
88 100
43 40.1 77.0 115.4#
58 89.0 70.8 106.2


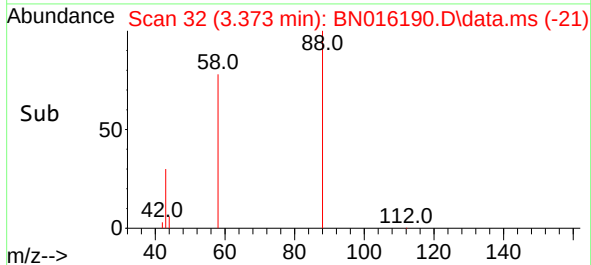

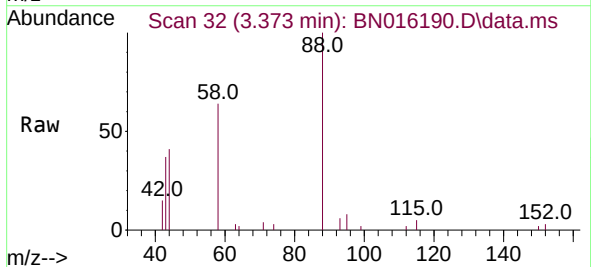


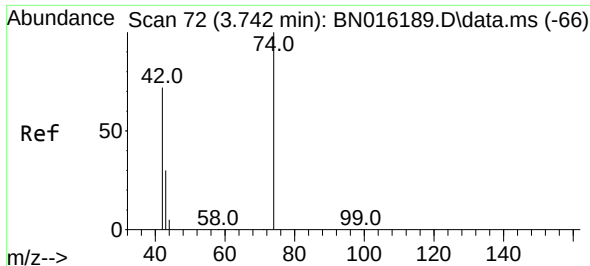

#3
n-Nitrosodimethylamine
Concen: 0.752 ng
RT: 3.742 min Scan# 72
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion: 42 Resp: 8520
Ion Ratio Lower Upper
42 100
74 141.0 112.2 168.4
44 6.9 5.0 7.4

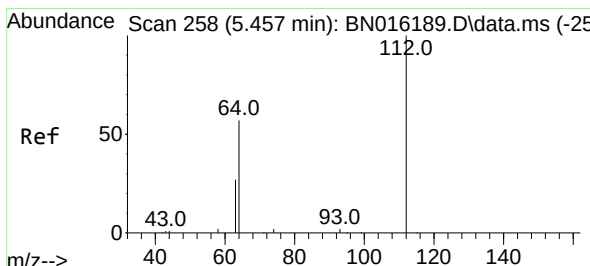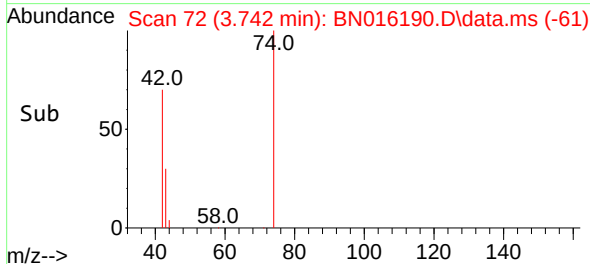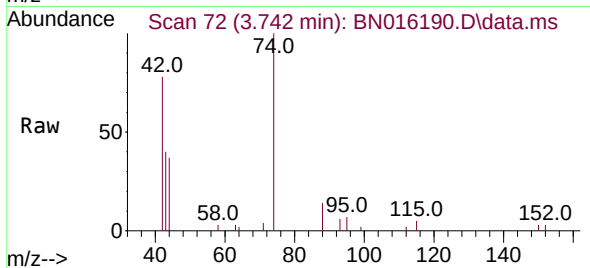

#4
2-Fluorophenol
Concen: 0.933 ng
RT: 5.457 min Scan# 258
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35

Tgt Ion: 112 Resp: 29356
Ion Ratio Lower Upper
112 100
64 59.6 46.8 70.2
63 29.0 22.7 34.1


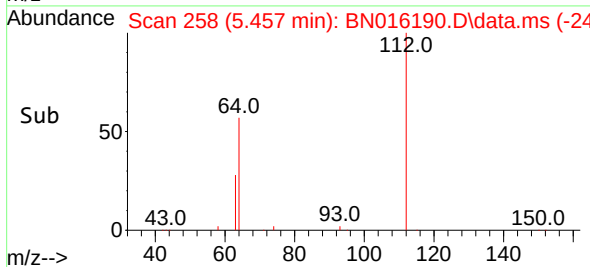

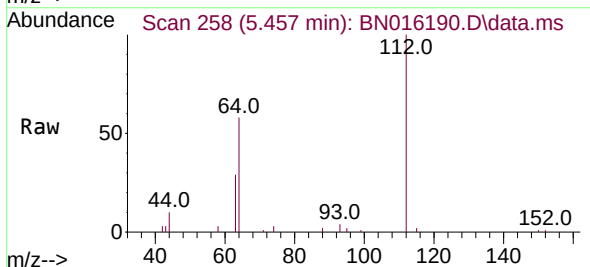


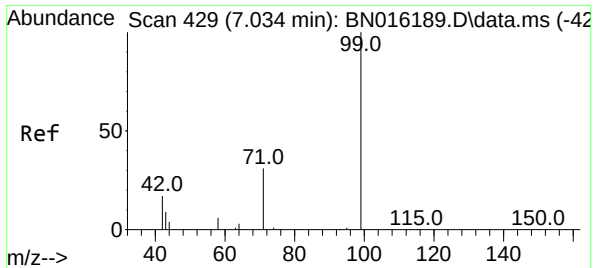

#5
Phenol-d6
Concen: 0.866 ng
RT: 7.033 min Scan# 429
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35




Instrument :
BNA_N
ClientSampled :
SSTDICC0.8


Tgt Ion:	99	Resp:	38024
Ion	Ratio	Lower	Upper
99	100		
42	17.0	13.8	20.6
71	30.2	24.3	36.5

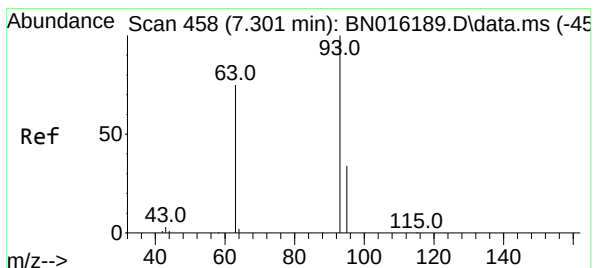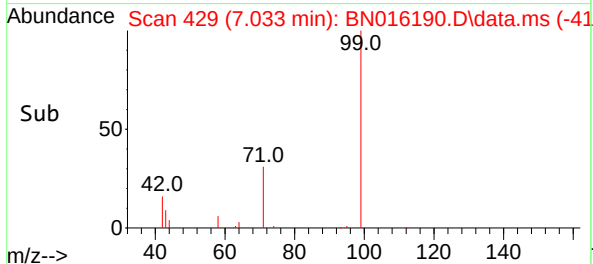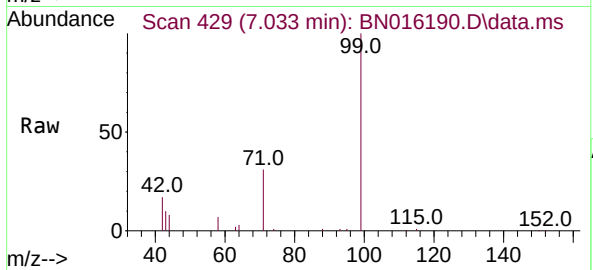

#6
bis(2-Chloroethyl)ether
Concen: 0.764 ng
RT: 7.301 min Scan# 458
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35

Tgt Ion:	93	Resp:	28047
Ion	Ratio	Lower	Upper
93	100		
63	78.3	62.8	94.2
95	33.1	27.0	40.4


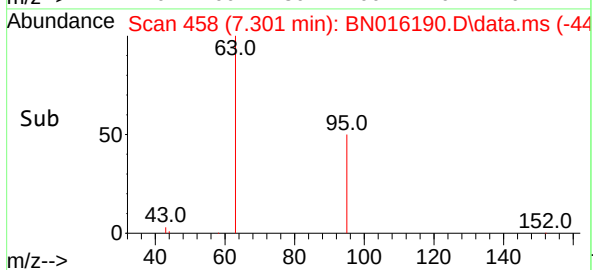

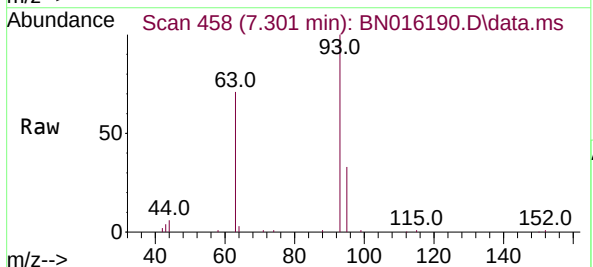


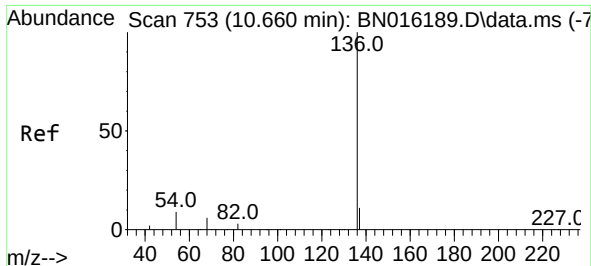

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.660 min Scan# 753
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:	136	Resp:	67399
Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.9	13.3
54	8.9	7.2	10.8
68	6.5	5.2	7.8

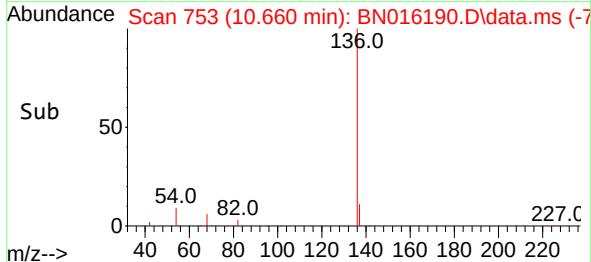

#8
Nitrobenzene-d5
Concen: 0.943 ng
RT: 9.025 min Scan# 624
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35

Tgt Ion:	82	Resp:	41786
Ion	Ratio	Lower	Upper
82	100		
128	49.3	39.3	58.9
54	48.7	40.2	60.4


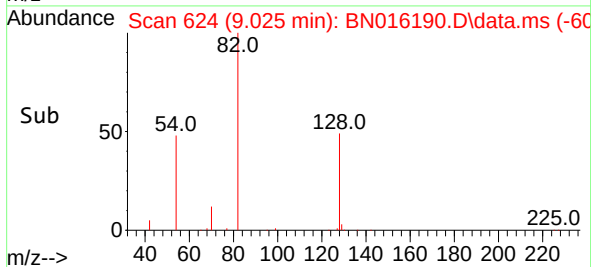

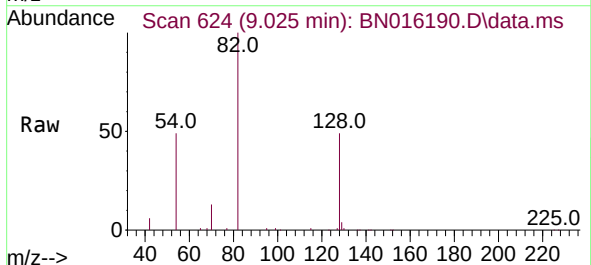


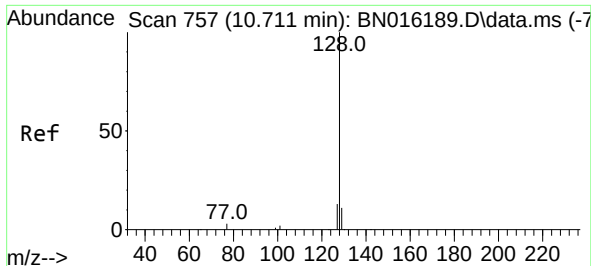

#9
Naphthalene
Concen: 0.803 ng
RT: 10.710 min Scan# 757
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:128 Resp: 142275
Ion Ratio Lower Upper
128 100
129 11.0 8.9 13.3
127 13.0 10.4 15.6

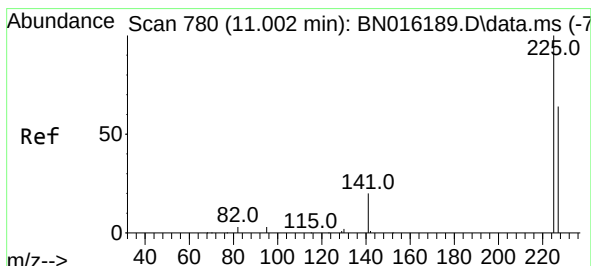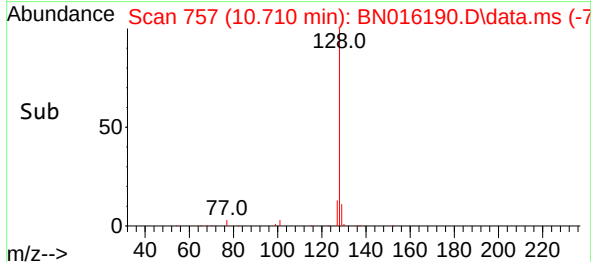

#10
Hexachlorobutadiene
Concen: 0.743 ng
RT: 11.002 min Scan# 780
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35

Tgt Ion:225 Resp: 29240
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.2 51.2 76.8


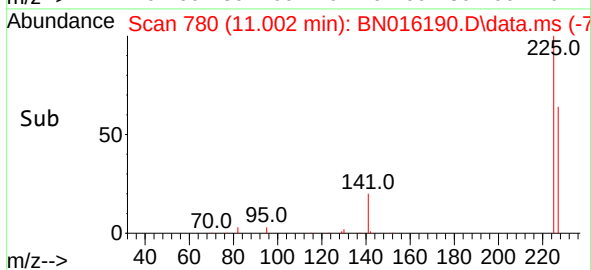

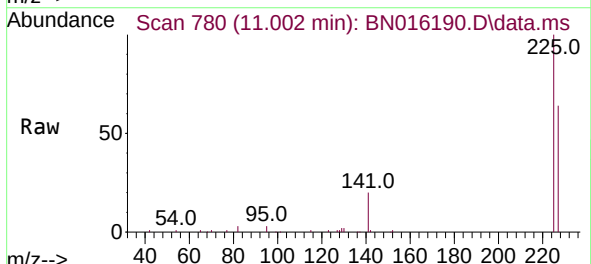


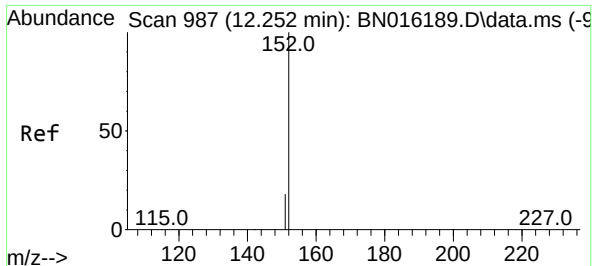

#11
2-Methylnaphthalene-d10
Concen: 0.859 ng
RT: 12.251 min Scan# 987
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:152 Resp: 87338
Ion Ratio Lower Upper
152 100
151 20.2 16.2 24.2

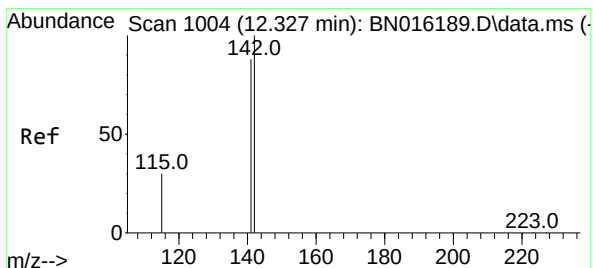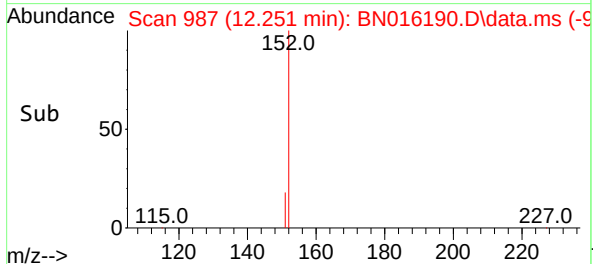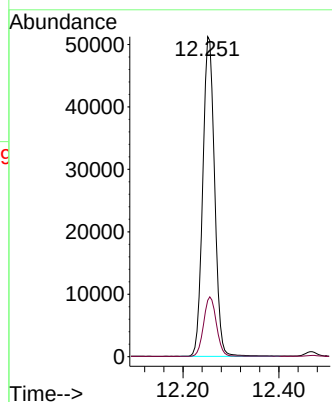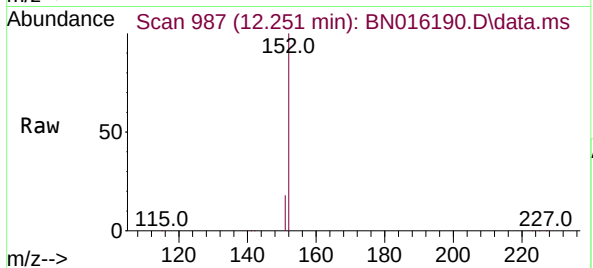

#12
2-Methylnaphthalene
Concen: 0.860 ng
RT: 12.327 min Scan# 1004
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35

Tgt Ion:142 Resp: 97313
Ion Ratio Lower Upper
142 100
141 86.5 70.4 105.6
115 30.0 24.4 36.6


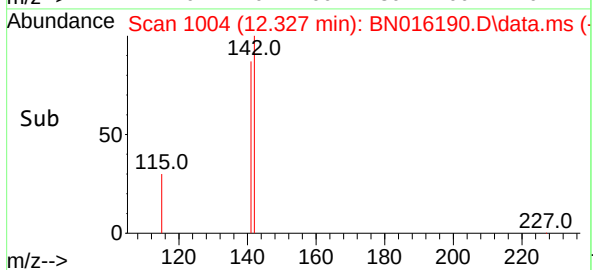
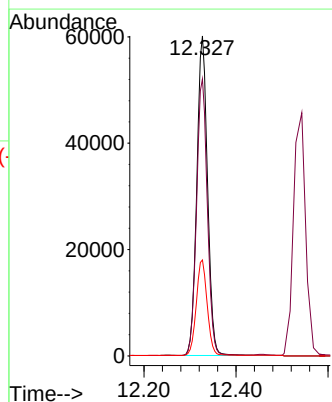
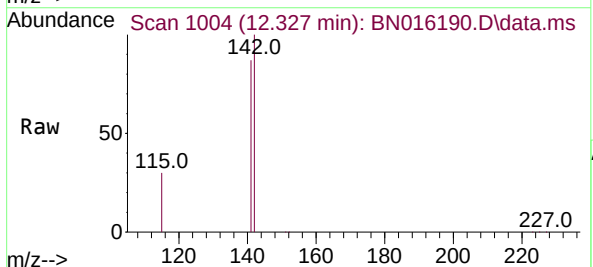




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.497 min Scan# 1201
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:164 Resp: 39743
Ion Ratio Lower Upper
164 100
162 100.4 79.8 119.6
160 43.5 34.2 51.4

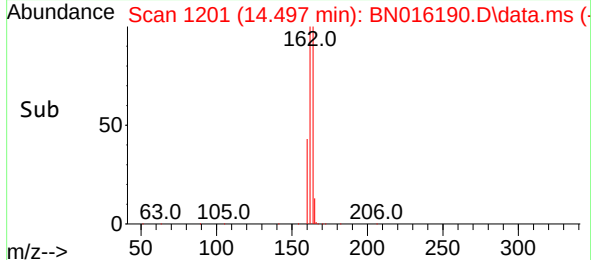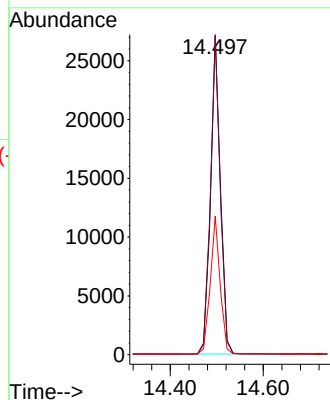

#14
2,4,6-Tribromophenol
Concen: 1.219 ng
RT: 15.994 min Scan# 1319
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35

Tgt Ion:330 Resp: 13748
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 31.6 25.4 38.2


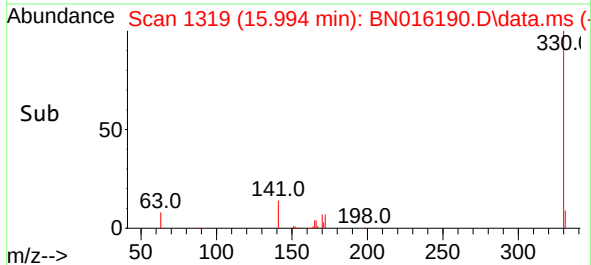
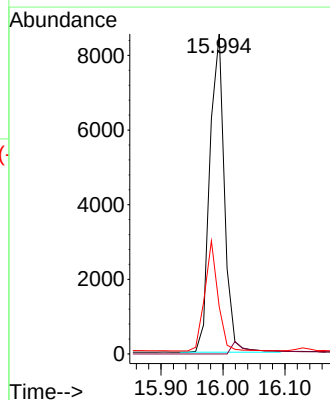
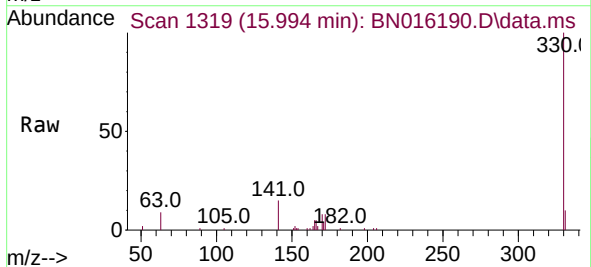


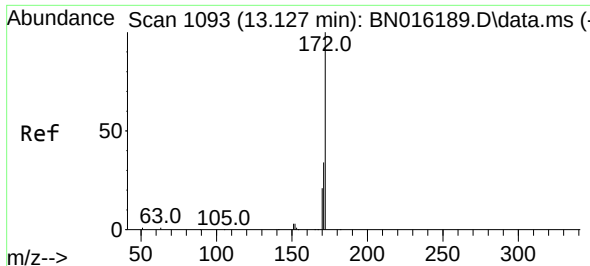

#15
2-Fluorobiphenyl
Concen: 0.721 ng
RT: 13.126 min Scan# 1093
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:172 Resp: 115374
Ion Ratio Lower Upper
172 100
171 33.5 26.9 40.3
170 21.3 17.1 25.7

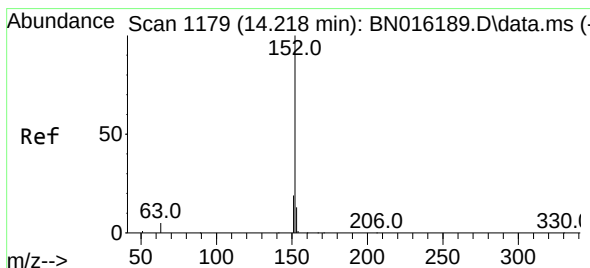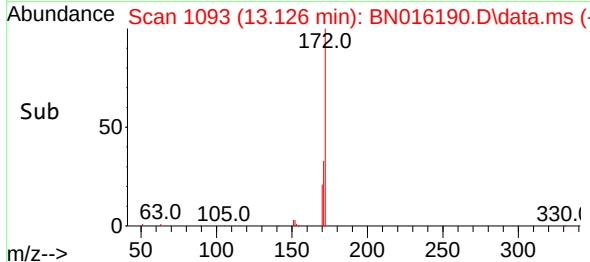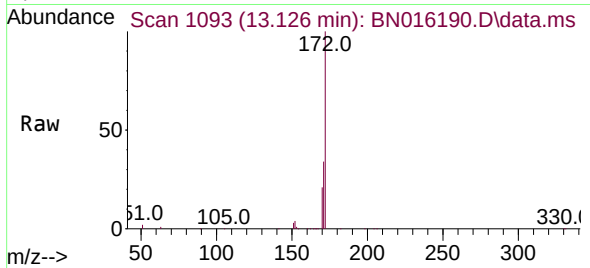

#16
Acenaphthylene
Concen: 0.977 ng
RT: 14.218 min Scan# 1179
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35

Tgt Ion:152 Resp: 142821
Ion Ratio Lower Upper
152 100
151 19.1 15.3 22.9
153 13.0 10.4 15.6


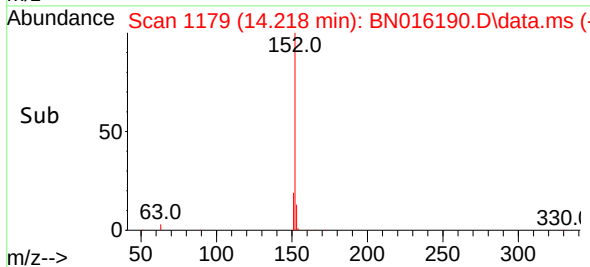

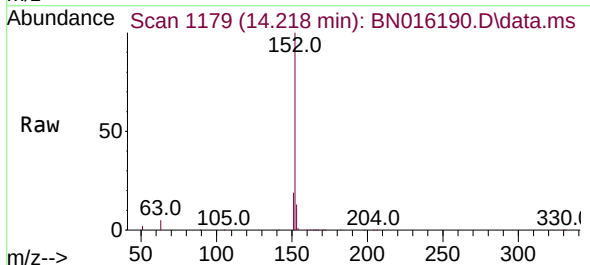




#17
Acenaphthene
Concen: 0.796 ng
RT: 14.560 min Scan# 1206
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:154 Resp: 89037
Ion Ratio Lower Upper
154 100
153 110.7 89.1 133.7
152 51.6 41.2 61.8

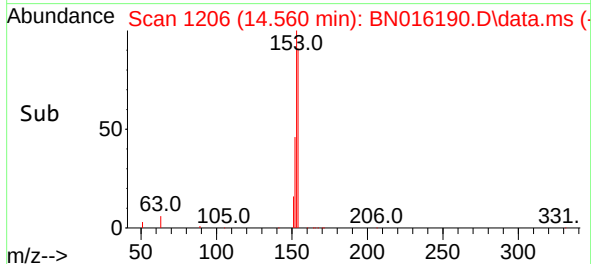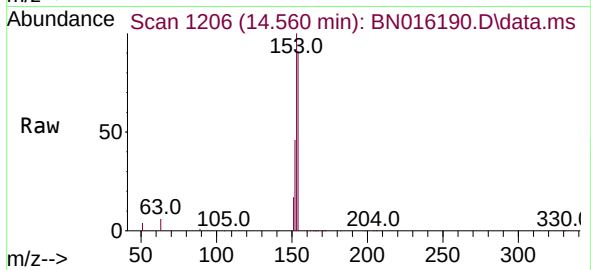

#18
Fluorene
Concen: 0.848 ng
RT: 15.550 min Scan# 1284
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35

Tgt Ion:166 Resp: 113476
Ion Ratio Lower Upper
166 100
165 96.1 77.0 115.6
167 13.5 10.9 16.3


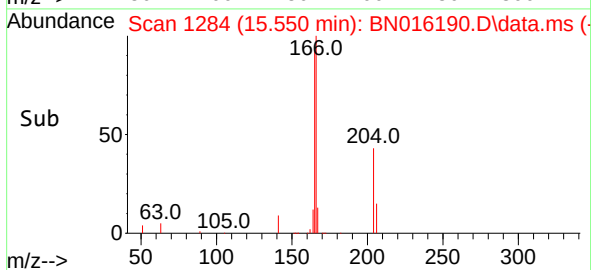

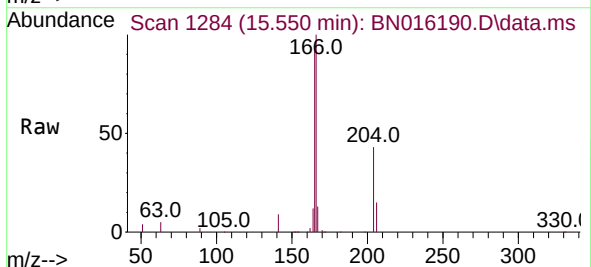


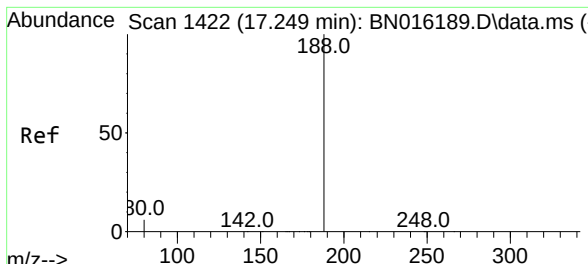

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.248 min Scan# 1422
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:188	Resp:	79796
Ion Ratio	Lower	Upper
188	100	
94	0.0	0.0
80	6.1	5.0
		7.6

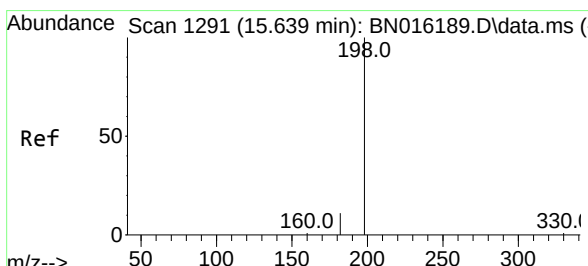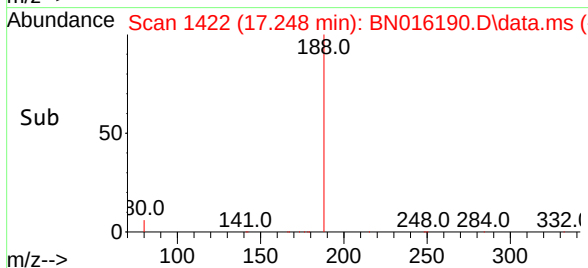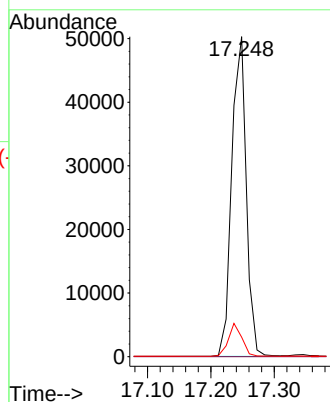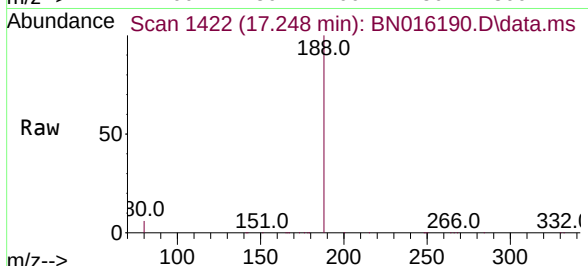

#20
4,6-Dinitro-2-methylphenol
Concen: 0.450 ng
RT: 15.639 min Scan# 1291
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35

Tgt Ion:198	Resp:	2392
Ion Ratio	Lower	Upper
198	100	
182	12.6	28.8
77	0.0	0.0
		43.2#


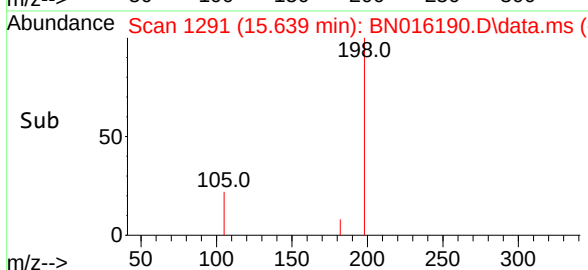
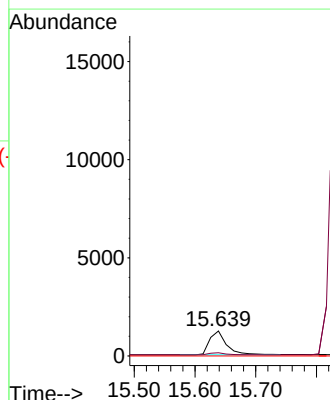
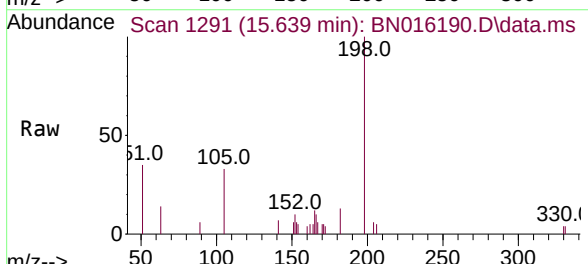


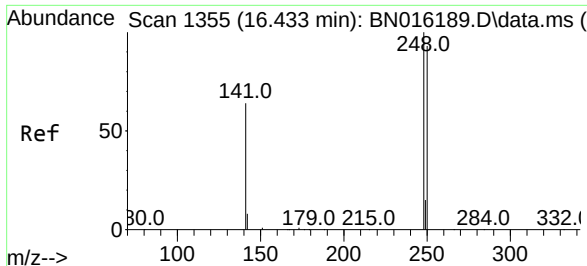

#21
4-Bromophenyl-phenylether
Concen: 0.829 ng
RT: 16.433 min Scan# 1355
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:248 Resp: 33228
Ion Ratio Lower Upper
248 100
250 95.1 74.6 112.0
141 65.5 51.6 77.4

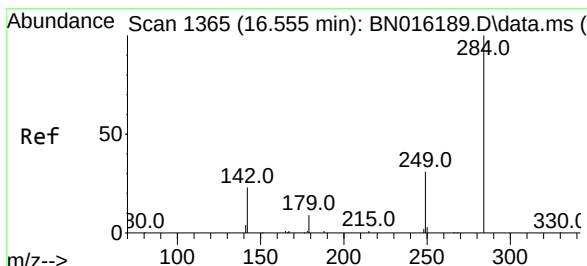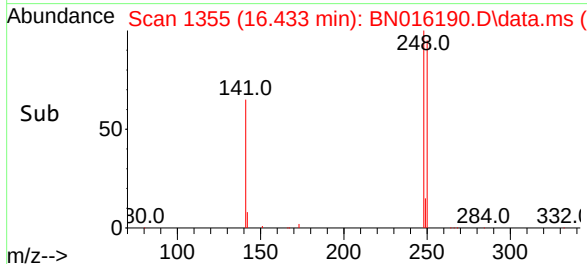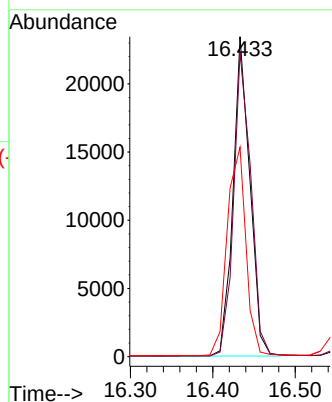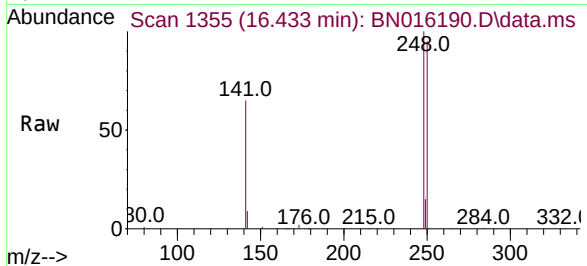

#22
Hexachlorobenzene
Concen: 0.695 ng
RT: 16.555 min Scan# 1365
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35

Tgt Ion:284 Resp: 39134
Ion Ratio Lower Upper
284 100
142 28.6 22.7 34.1
249 30.8 24.3 36.5


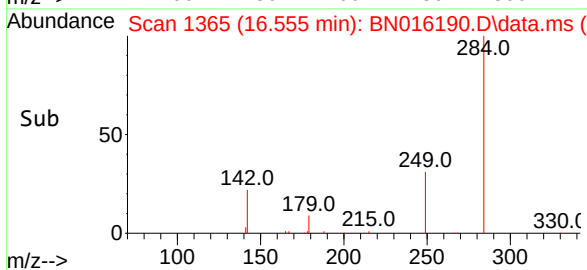

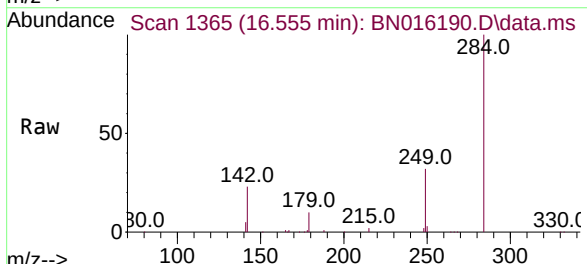


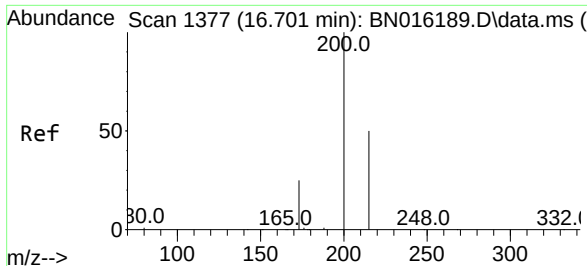

#23
Atrazine
Concen: 1.379 ng
RT: 16.701 min Scan# 1377
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:200 Resp: 33807
Ion Ratio Lower Upper
200 100
173 26.3 20.6 31.0
215 50.8 40.5 60.7

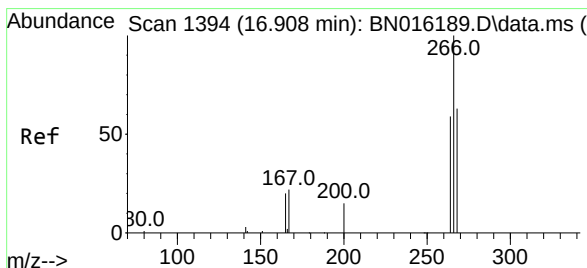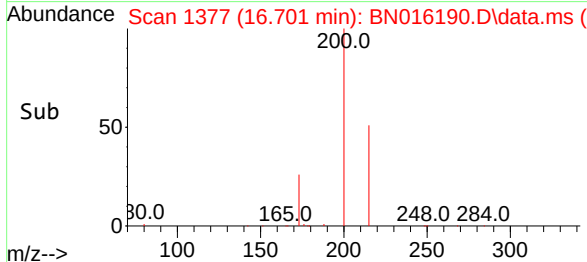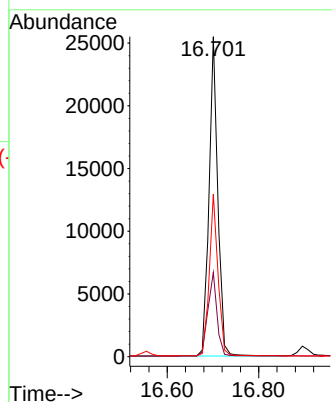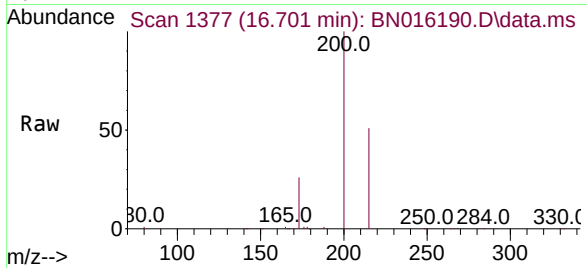

#24
Pentachlorophenol
Concen: 0.511 ng
RT: 16.895 min Scan# 1393
Delta R.T. -0.012 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35

Tgt Ion:266 Resp: 7551
Ion Ratio Lower Upper
266 100
264 62.5 50.4 75.6
268 64.2 49.6 74.4


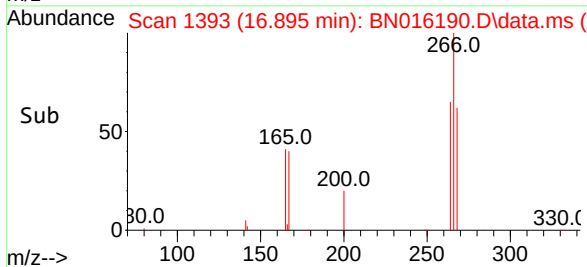

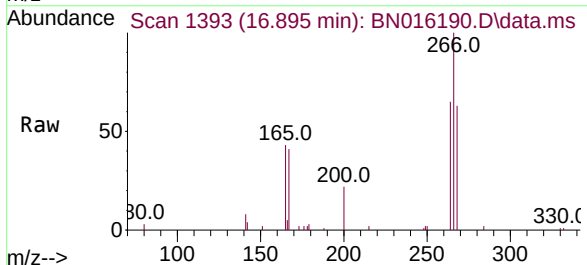


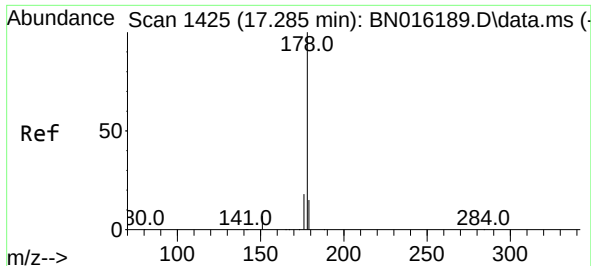

#25
Phenanthrene
Concen: 0.776 ng
RT: 17.285 min Scan# 1425
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:178 Resp: 176138
Ion Ratio Lower Upper
178 100
176 18.0 14.5 21.7
179 15.5 12.3 18.5

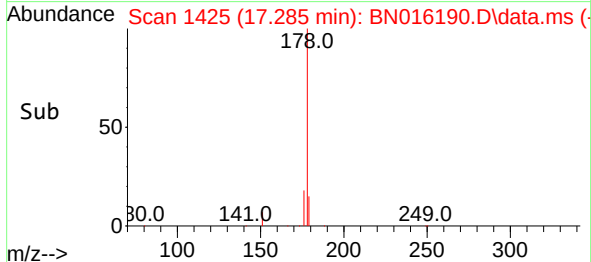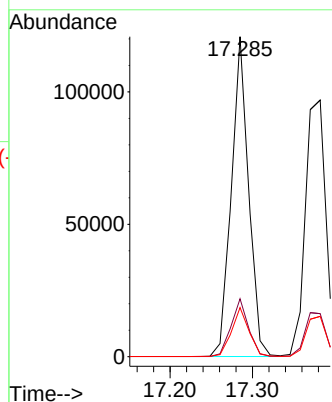

#26
Anthracene
Concen: 0.913 ng
RT: 17.382 min Scan# 1433
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35

Tgt Ion:178 Resp: 169768
Ion Ratio Lower Upper
178 100
176 17.3 13.8 20.8
179 15.4 12.4 18.6


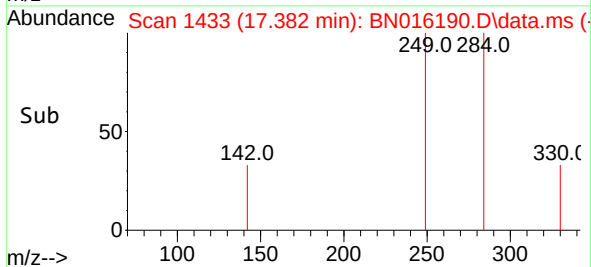

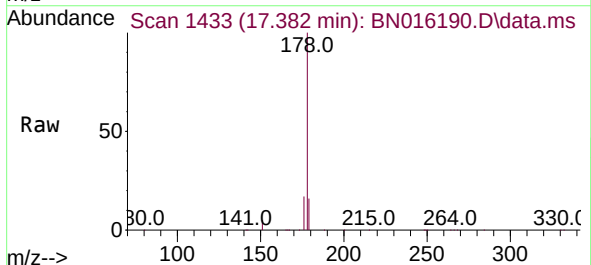


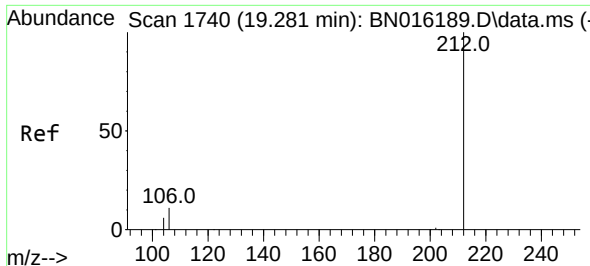

#27
Fluoranthene-d10
Concen: 0.858 ng
RT: 19.281 min Scan# 1740
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:212 Resp: 193022
Ion Ratio Lower Upper
212 100
106 12.2 9.7 14.5
104 6.8 5.4 8.0

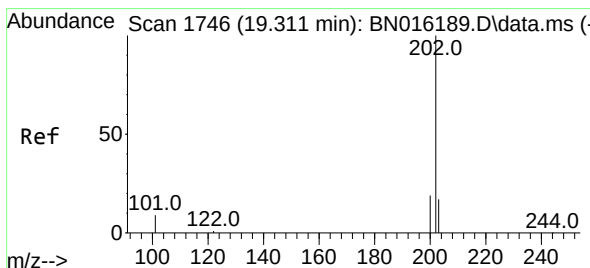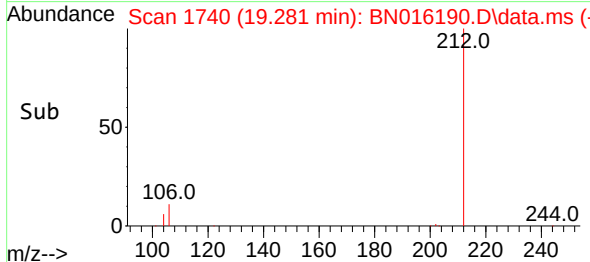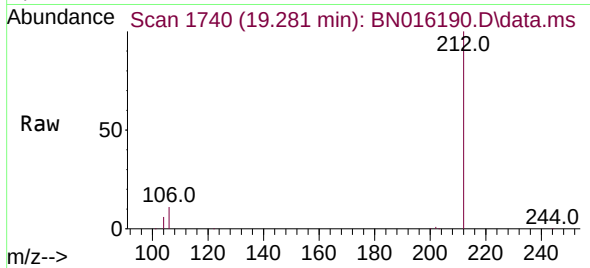

#28
Fluoranthene
Concen: 0.844 ng
RT: 19.306 min Scan# 1745
Delta R.T. -0.005 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35

Tgt Ion:202 Resp: 212689
Ion Ratio Lower Upper
202 100
101 10.5 8.4 12.6
203 17.4 13.8 20.8


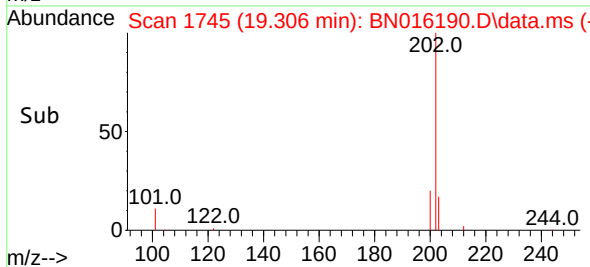

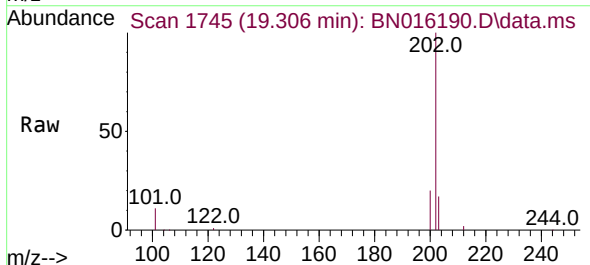


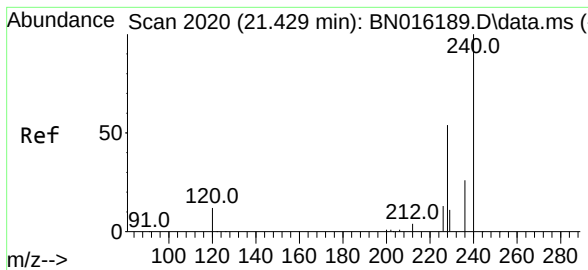

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.429 min Scan# 2020
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:	240	Resp:	83372
Ion Ratio	Lower	Upper	
240	100		
120	12.9	10.0	15.0
236	26.1	20.9	31.3

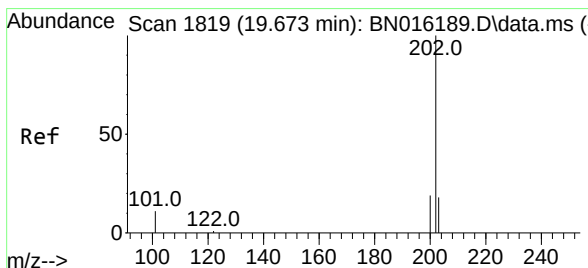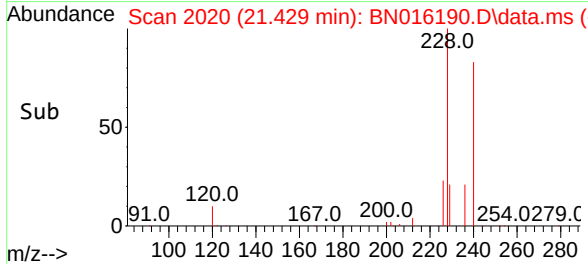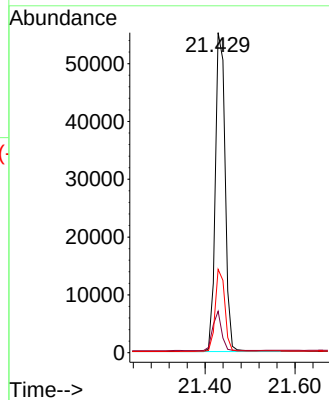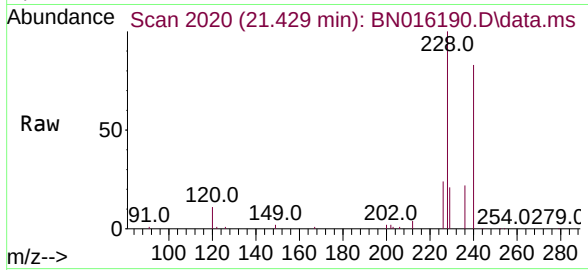

#30
Pyrene
Concen: 0.873 ng
RT: 19.673 min Scan# 1819
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35

Tgt Ion:	202	Resp:	216515
Ion Ratio	Lower	Upper	
202	100		
200	19.7	15.8	23.8
203	17.6	14.1	21.1


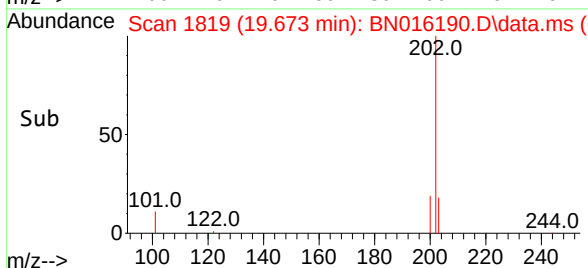
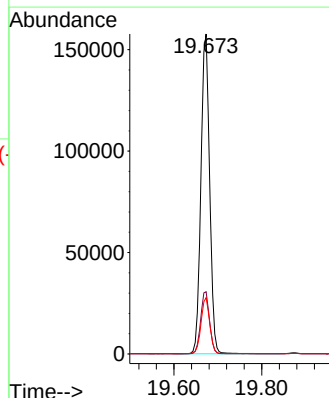
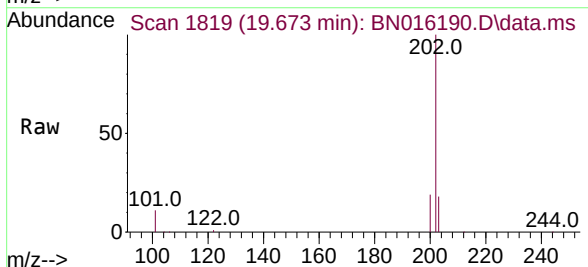


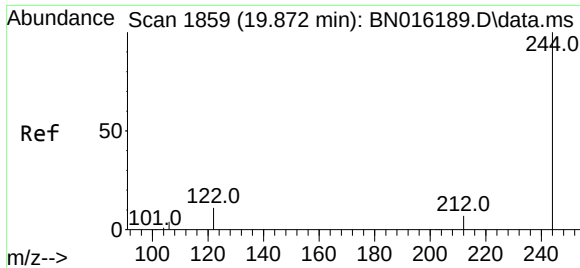

#31
 Terphenyl-d14
 Concen: 0.797 ng
 RT: 19.877 min Scan# 1860
 Delta R.T. 0.005 min
 Lab File: BN016190.D
 Acq: 04 Sep 2021 12:35




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8


Tgt Ion:244	Resp:	163000
Ion Ratio	Lower	Upper
244	100	
212	6.6	5.5 8.3
122	9.6	9.0 13.4

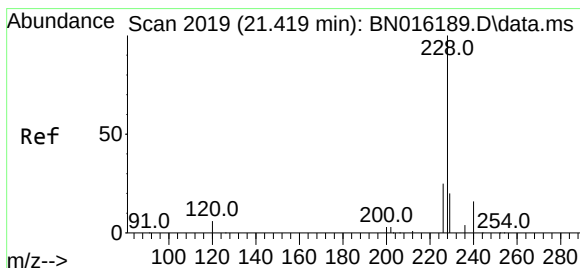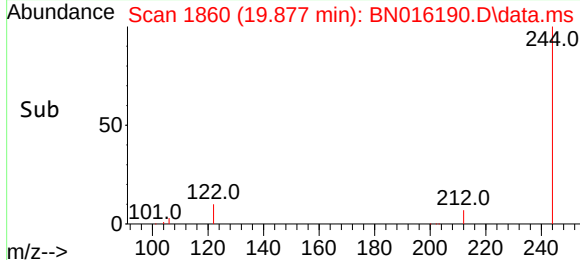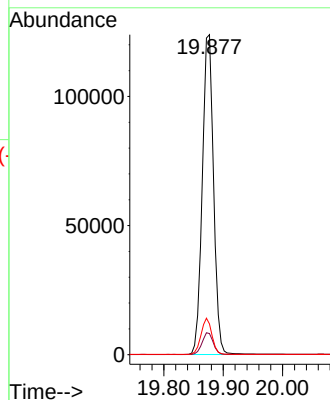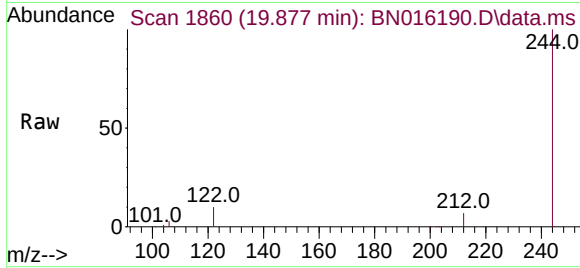

#32
 Benzo(a)anthracene
 Concen: 0.880 ng
 RT: 21.418 min Scan# 2019
 Delta R.T. -0.000 min
 Lab File: BN016190.D
 Acq: 04 Sep 2021 12:35

Tgt Ion:228	Resp:	222712
Ion Ratio	Lower	Upper
228	100	
226	25.6	20.5 30.7
229	20.0	16.2 24.4


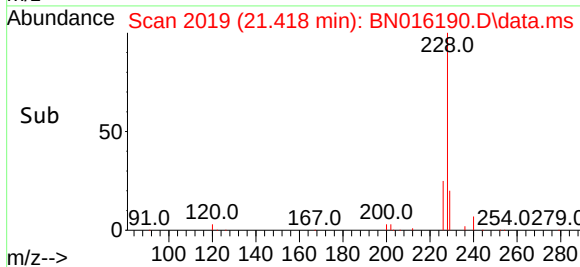
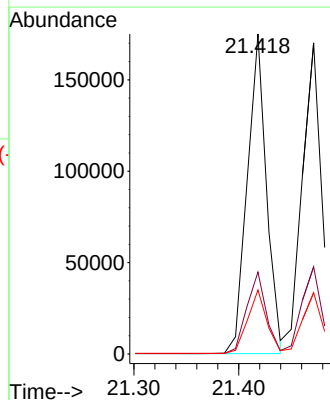
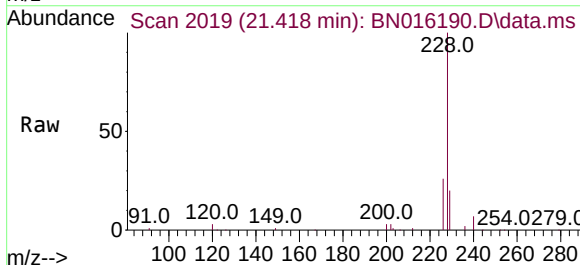


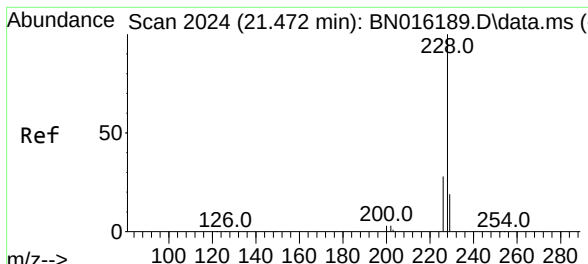

#33
Chrysene
Concen: 0.822 ng
RT: 21.471 min Scan# 2024
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:	228	Resp:	220302
Ion Ratio	Lower	Upper	
228	100		
226	28.0	22.5	33.7
229	19.7	16.0	24.0

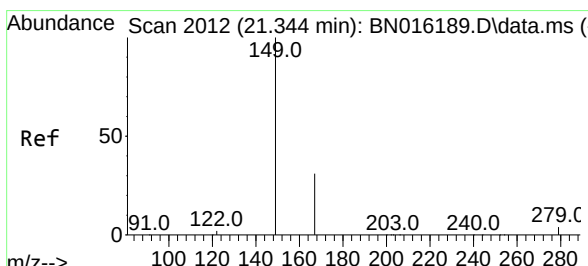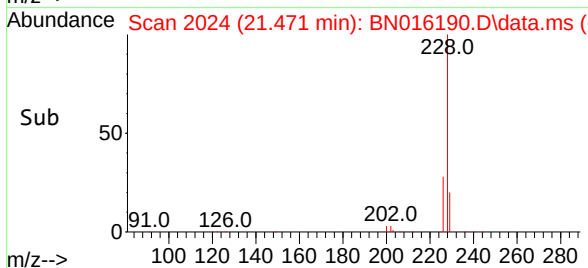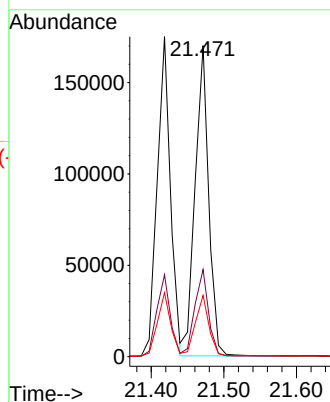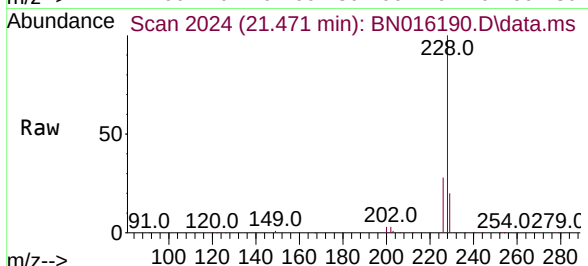

#34
Bis(2-ethylhexyl)phthalate
Concen: 2.136 ng
RT: 21.344 min Scan# 2012
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35


Tgt Ion:	149	Resp:	144192
Ion Ratio	Lower	Upper	
149	100		
167	29.9	24.2	36.4
279	5.0	4.0	6.0

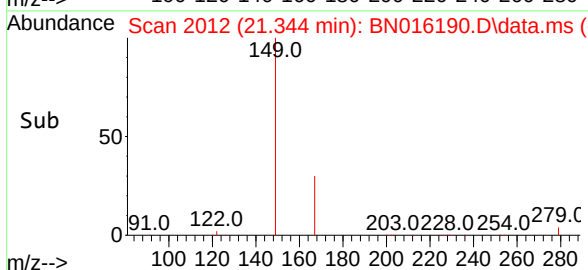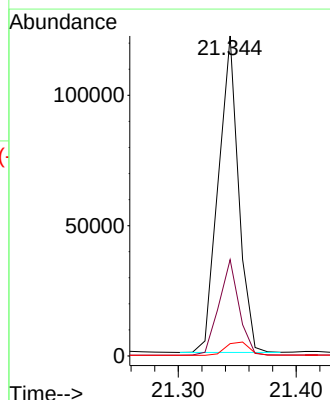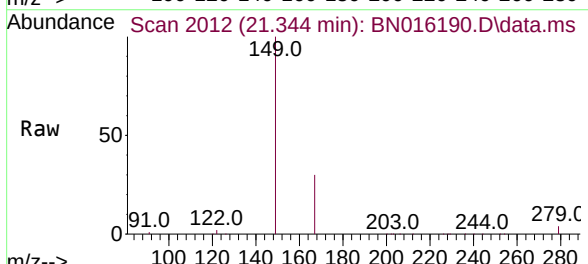



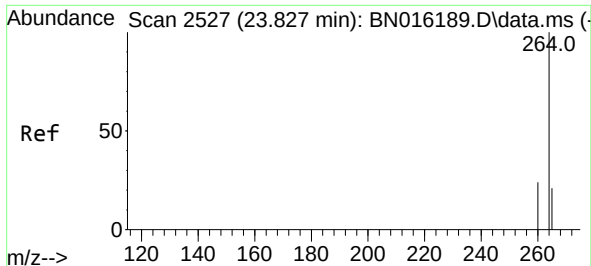


#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.826 min Scan# 2527
 Delta R.T. -0.000 min
 Lab File: BN016190.D
 Acq: 04 Sep 2021 12:35

Instrument :
 BNA_N
 ClientSampled :
 SSTDICC0.8







Tgt Ion:264	Resp:	83449
Ion Ratio	Lower	Upper
264	100	
260	24.1	19.5 29.3
265	24.9	20.2 30.2

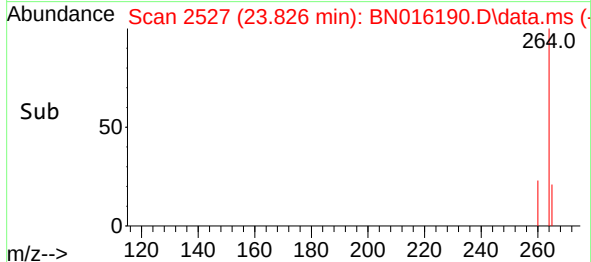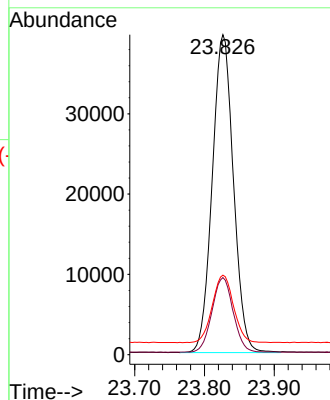

#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.610 ng
 RT: 26.301 min Scan# 3250
 Delta R.T. -0.004 min
 Lab File: BN016190.D
 Acq: 04 Sep 2021 12:35

Tgt Ion:276	Resp:	192622
Ion Ratio	Lower	Upper
276	100	
138	24.5	19.5 29.3
277	25.2	20.2 30.4


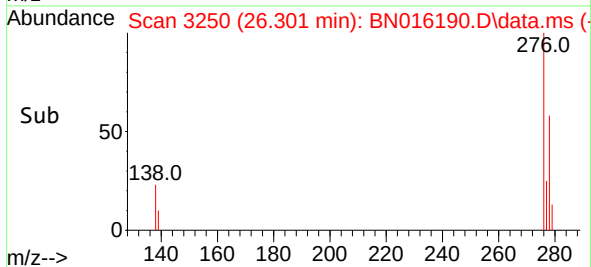
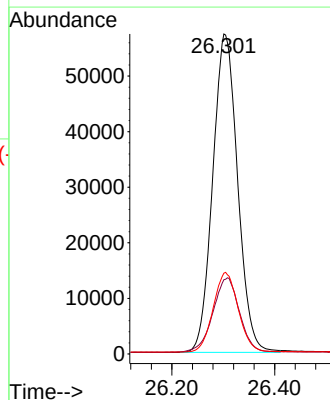
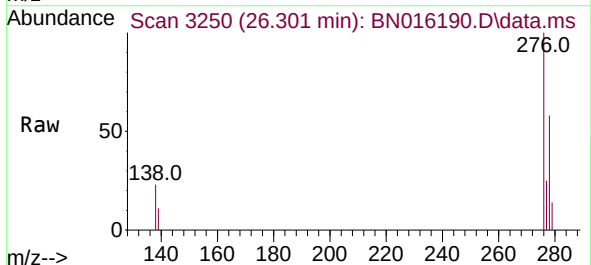


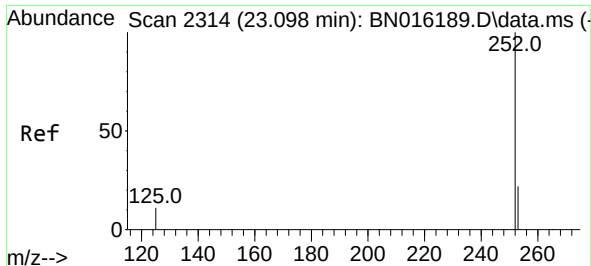

#37
Benzo(b)fluoranthene
Concen: 0.763 ng
RT: 23.097 min Scan# 2314
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:252 Resp: 227982
Ion Ratio Lower Upper
252 100
253 22.6 18.6 27.8
125 12.0 10.5 15.7

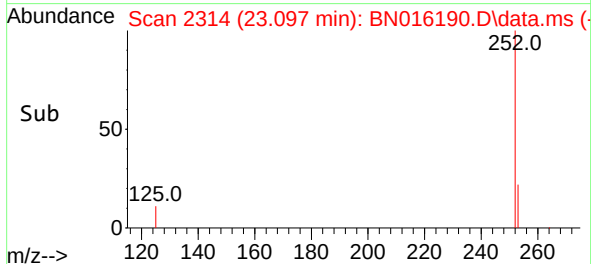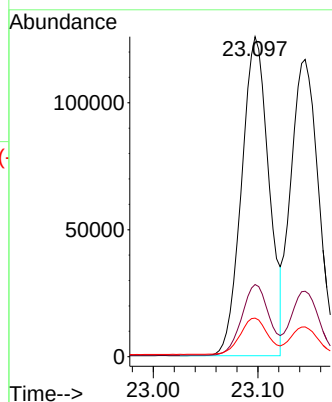

#38
Benzo(k)fluoranthene
Concen: 0.758 ng
RT: 23.145 min Scan# 2328
Delta R.T. 0.003 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35

Tgt Ion:252 Resp: 210937
Ion Ratio Lower Upper
252 100
253 22.0 18.2 27.2
125 10.0 9.1 13.7


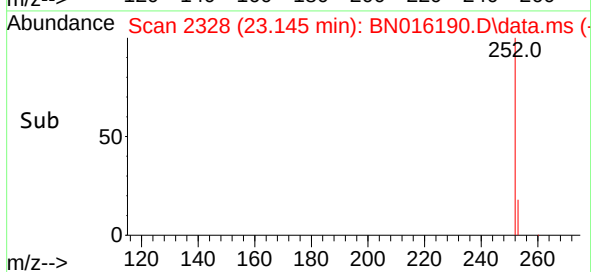
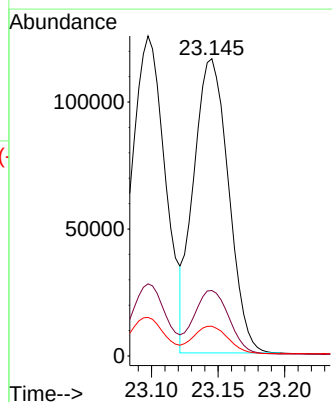
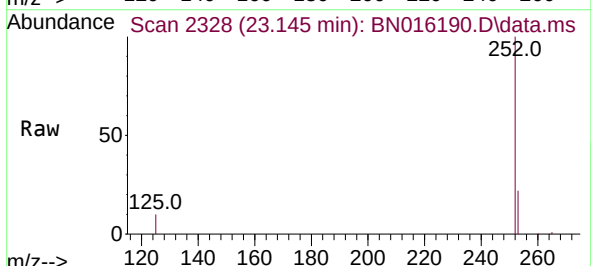


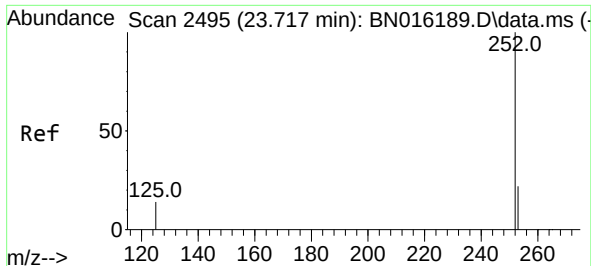

#39
Benzo(a)pyrene
Concen: 0.788 ng
RT: 23.720 min Scan# 2496
Delta R.T. 0.003 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:252 Resp: 202907
Ion Ratio Lower Upper
252 100
253 23.2 19.0 28.4
125 15.8 12.6 19.0

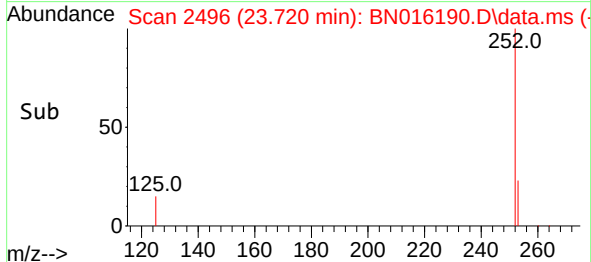

#40
Dibenzo(a,h)anthracene
Concen: 0.617 ng
RT: 26.322 min Scan# 3256
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35

Tgt Ion:278 Resp: 161224
Ion Ratio Lower Upper
278 100
139 15.9 14.0 21.0
279 24.1 20.2 30.2

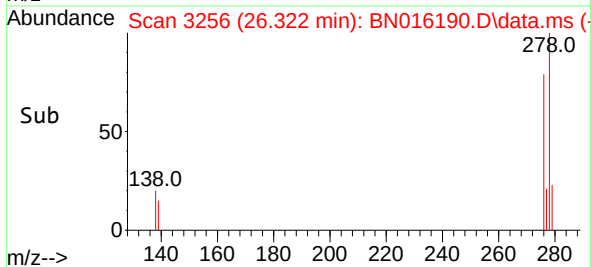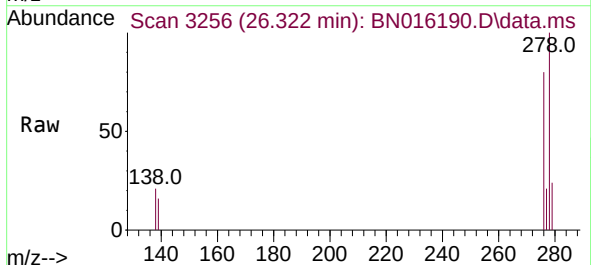

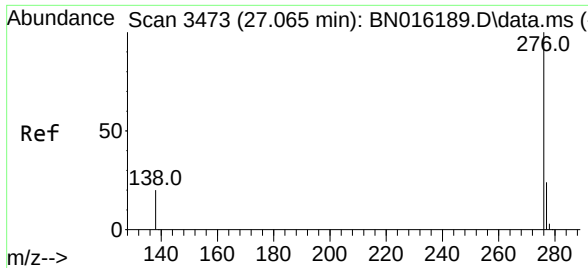

#41
Benzo(g,h,i)perylene
Concen: 0.593 ng
RT: 27.064 min Scan# 3473
Delta R.T. -0.000 min
Lab File: BN016190.D
Acq: 04 Sep 2021 12:35

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

Tgt Ion:276 Resp: 159988
Ion Ratio Lower Upper
276 100
277 24.5 20.3 30.5
138 20.9 17.5 26.3

