
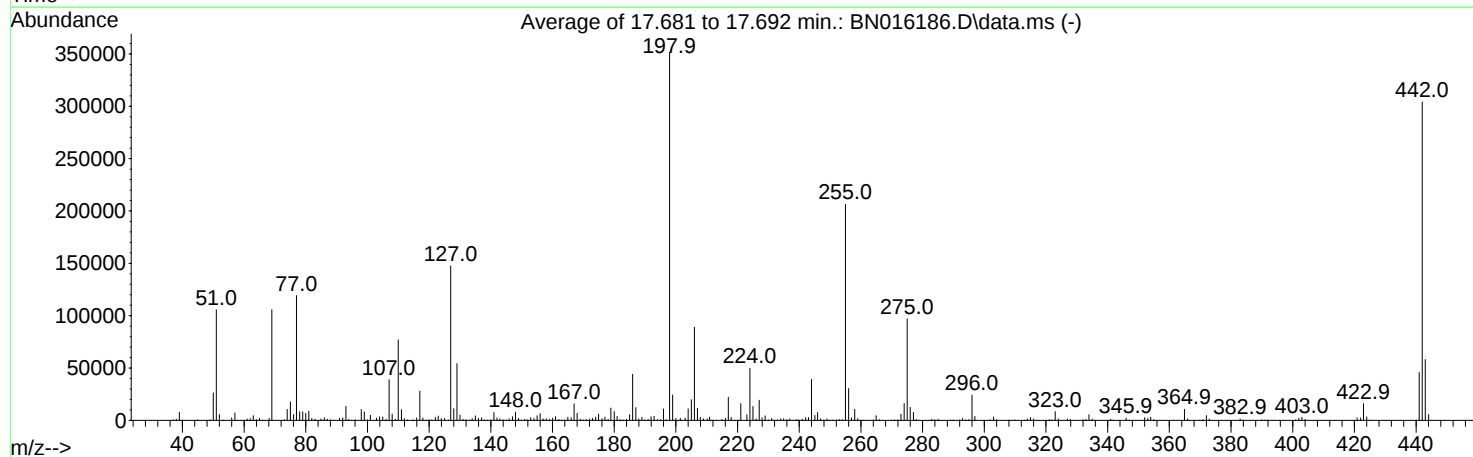


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090421\
 Data File : BN016186.D
 Acq On : 04 Sep 2021 10:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN090421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 06 02:08:58 2021

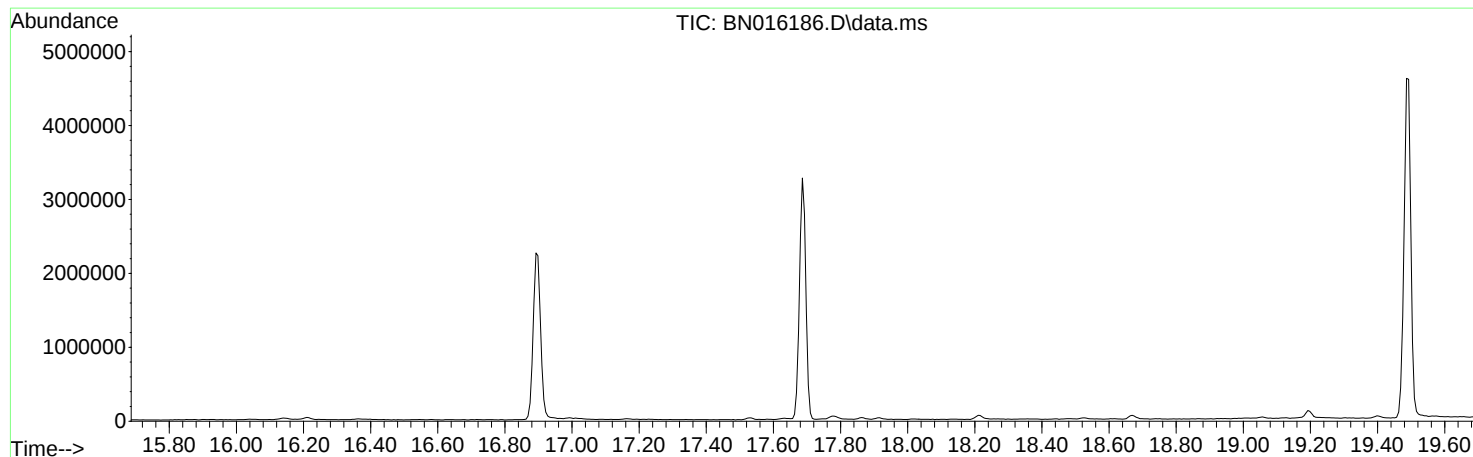

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.1	105626	PASS
68	69	0.00	2	1.8	1938	PASS
69	198	0.00	100	30.1	105830	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.0	147435	PASS
197	198	0.00	2	0.2	671	PASS
198	198	100	100	100.0	351403	PASS
199	198	5	9	6.9	24152	PASS
275	198	10	60	27.6	97072	PASS
365	198	1	100	3.0	10580	PASS
441	198	0.01	100	13.0	45773	PASS
442	442	50	100	100.0	304171	PASS
443	442	15	24	19.1	58021	PASS

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/4/2021	BNA_N	<u>BN016186.D</u>
Compound Name	Response	Retention Time
DDT	1350073	20.727
DDD	8699	20.339
DDE	2235	19.781
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10934	1361007	0.80

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090421\
 Data File : BN016186.D
 Acq On : 04 Sep 2021 10:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 06 02:24:08 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 17:12:56 2021
 Response via : Initial Calibration

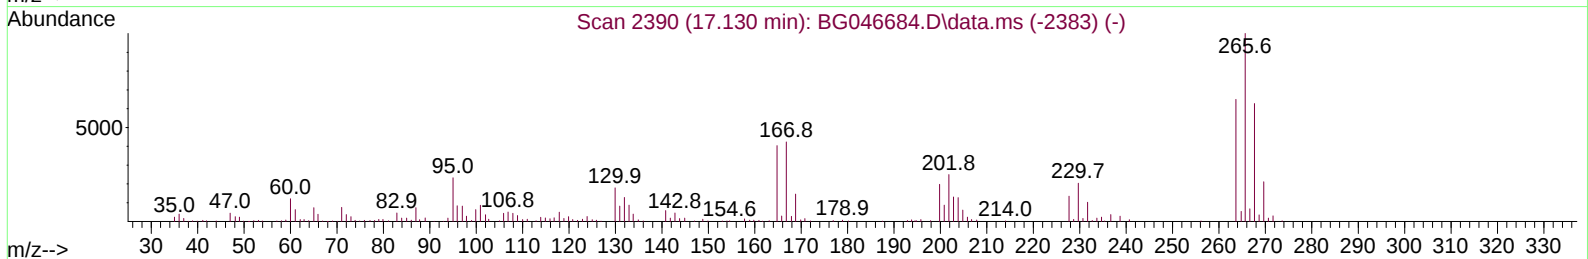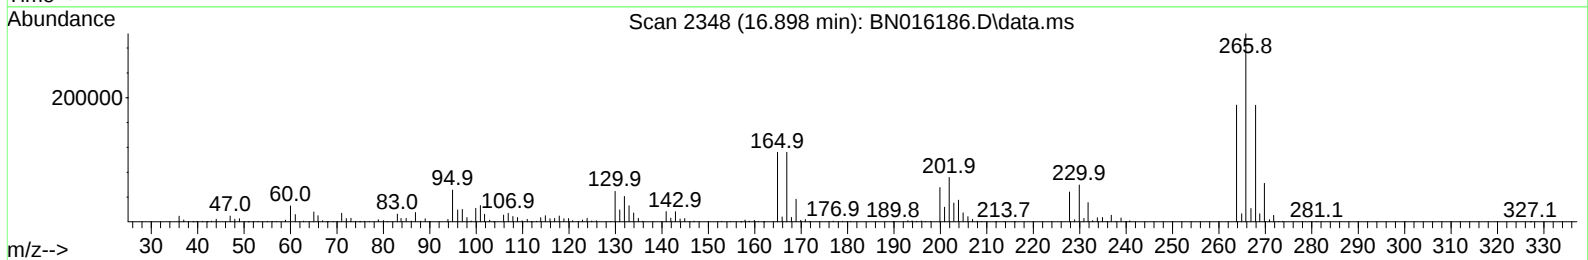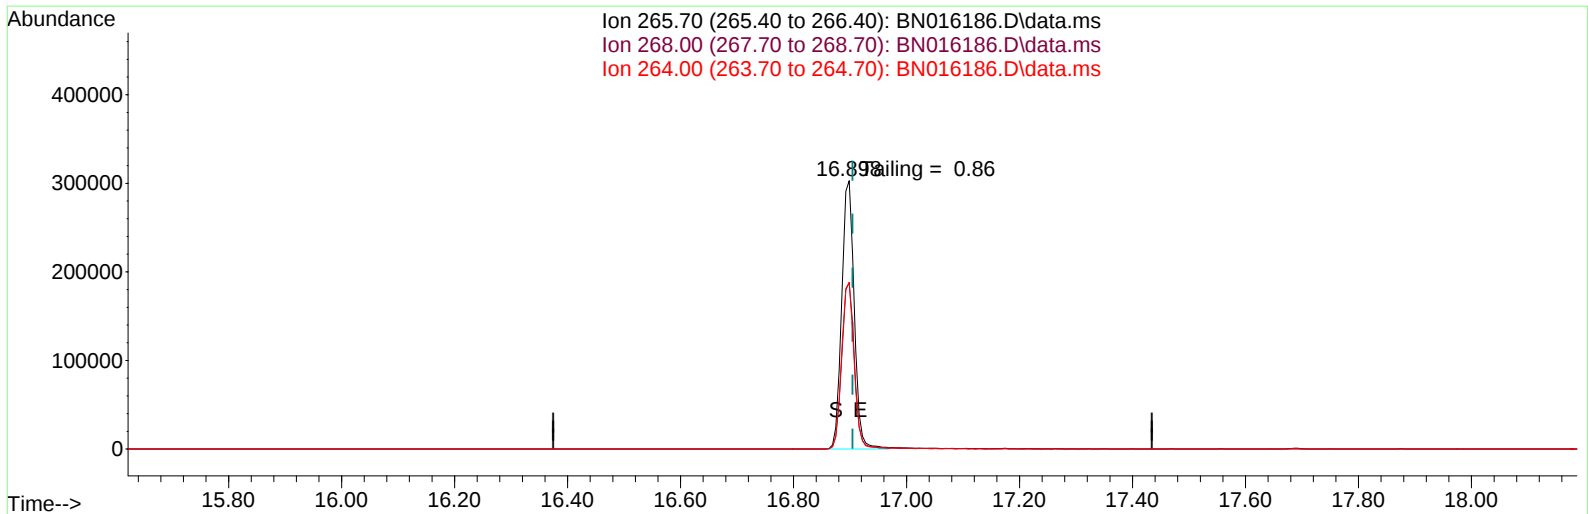

TIC: BN016186.D\data.ms

(70) Pentachlorophenol (C)

16.898min (-0.006) 27960.11 ng




response 468470

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.01
264.00	61.60	62.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090421\
Data File : BN016186.D
Acq On : 04 Sep 2021 10:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 06 02:24:08 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 17:12:56 2021
Response via : Initial Calibration

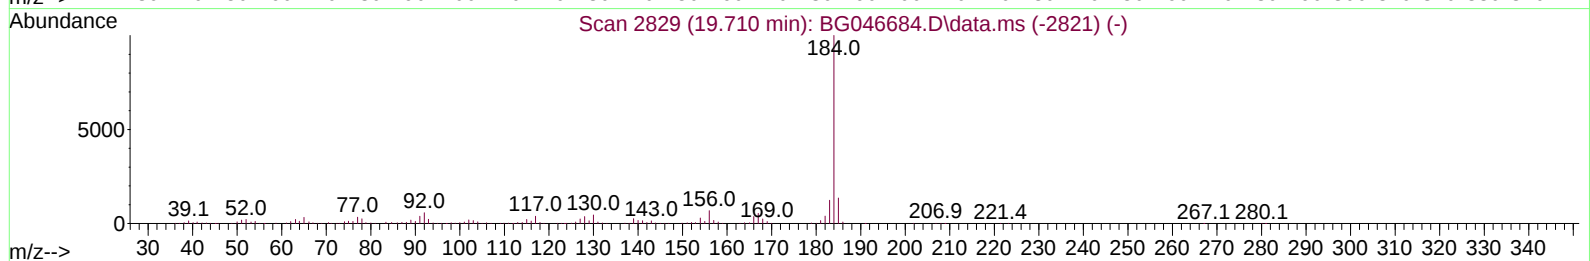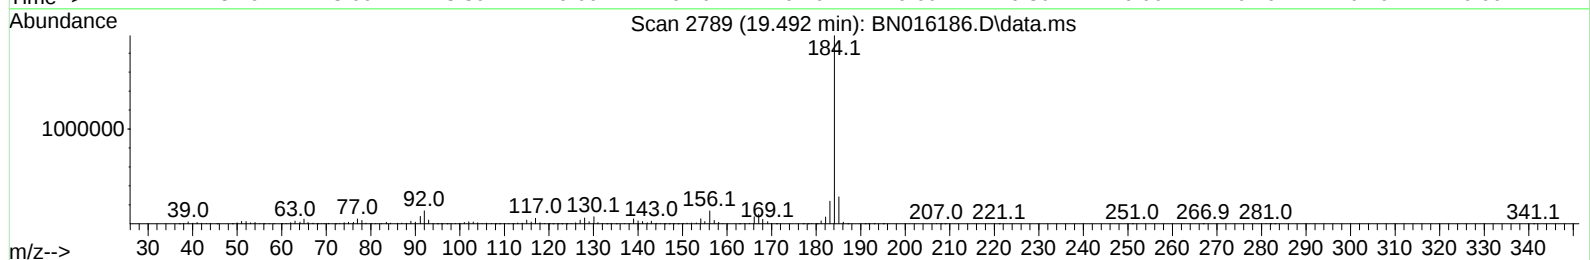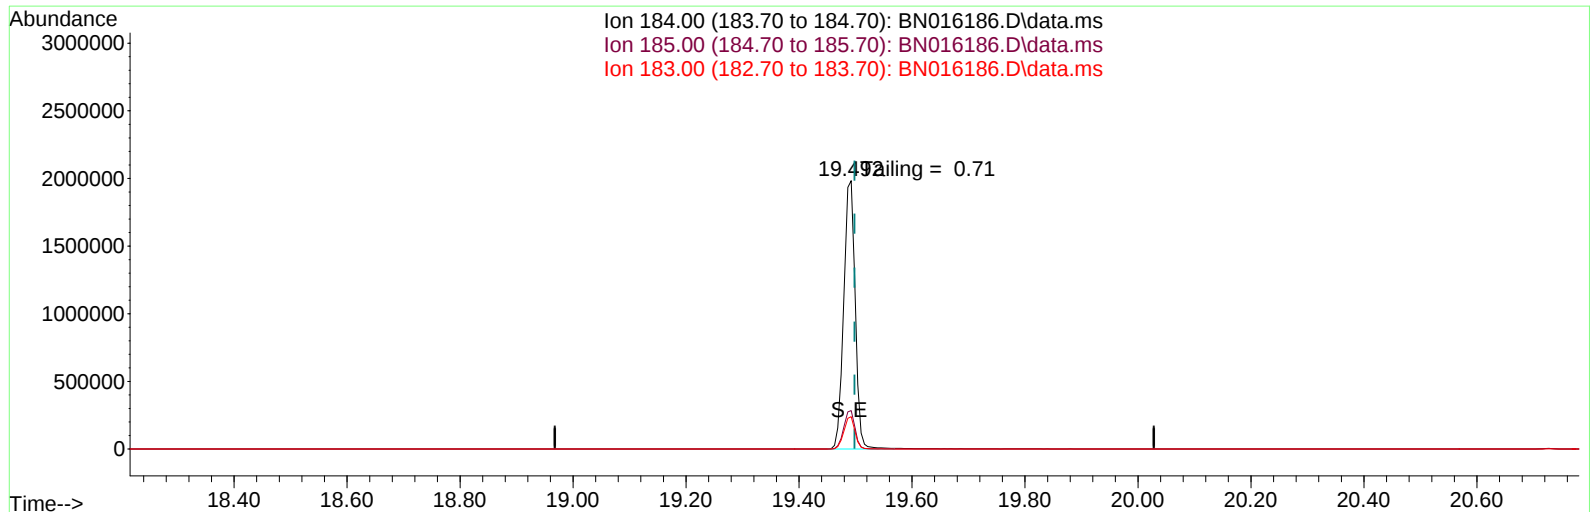

TIC: BN016186.D\data.ms

(77) Benzidine

19.492min (-0.006) 220530.10 ng

response 2800744

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.30
183.00	13.20	12.05
0.00	0.00	0.00