
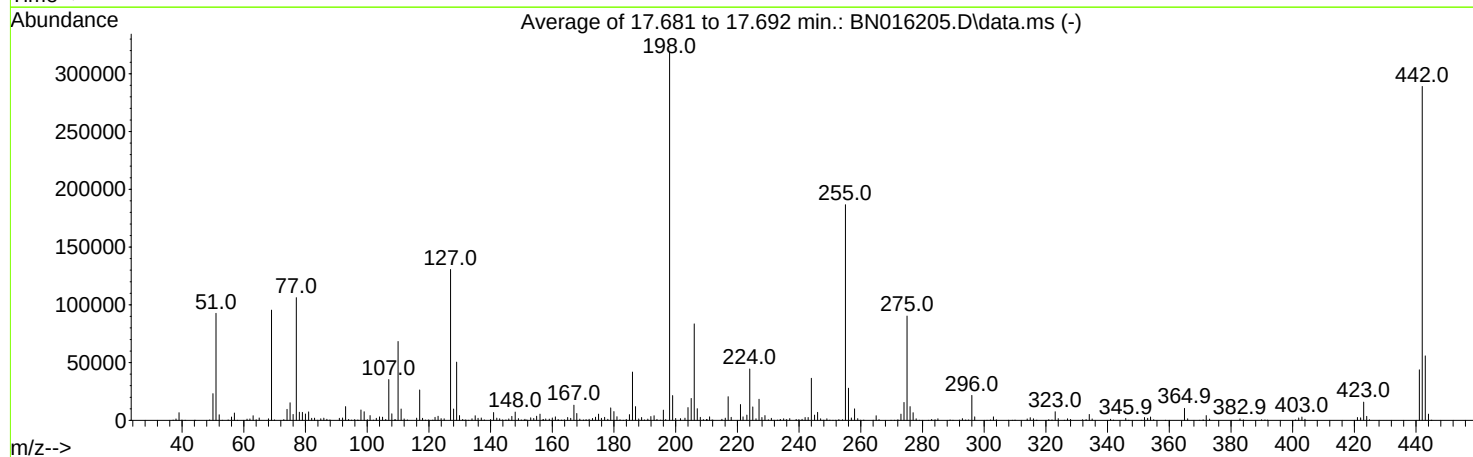


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090421\
 Data File : BN016205.D
 Acq On : 04 Sep 2021 22:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN090421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 06 02:08:58 2021

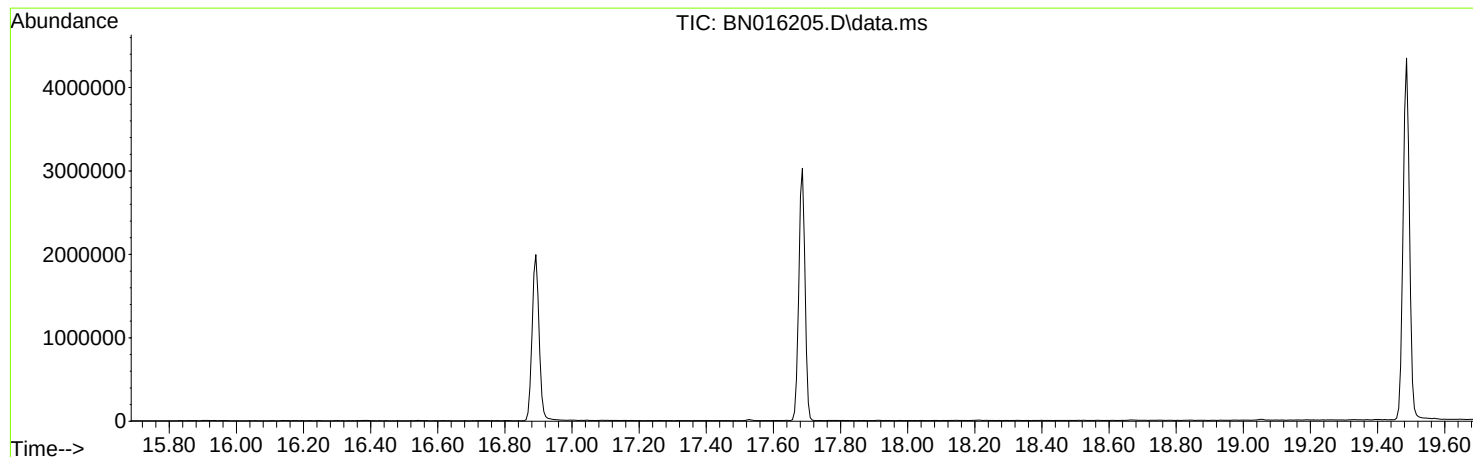

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.1	92611	PASS
68	69	0.00	2	1.5	1398	PASS
69	198	0.00	100	30.0	95443	PASS
70	69	0.00	2	0.5	439	PASS
127	198	10	80	41.0	130576	PASS
197	198	0.00	2	0.2	676	PASS
198	198	100	100	100.0	318400	PASS
199	198	5	9	6.7	21416	PASS
275	198	10	60	28.3	90240	PASS
365	198	1	100	3.3	10454	PASS
441	198	0.01	100	13.7	43717	PASS
442	442	50	100	100.0	289003	PASS
443	442	15	24	19.3	55827	PASS

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/4/2021	BNA_N	<u>BN016205.D</u>
Compound Name	Response	Retention Time
DDT	1217631	20.722
DDD	10613	20.286
DDE	121	19.775
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10734	1228365	0.87

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090421\
 Data File : BN016205.D
 Acq On : 04 Sep 2021 22:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 06 07:23:19 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 17:12:56 2021
 Response via : Initial Calibration

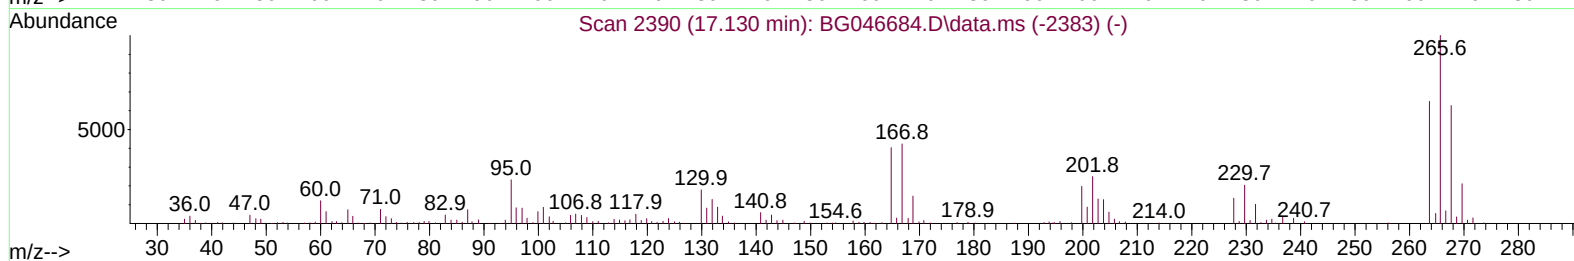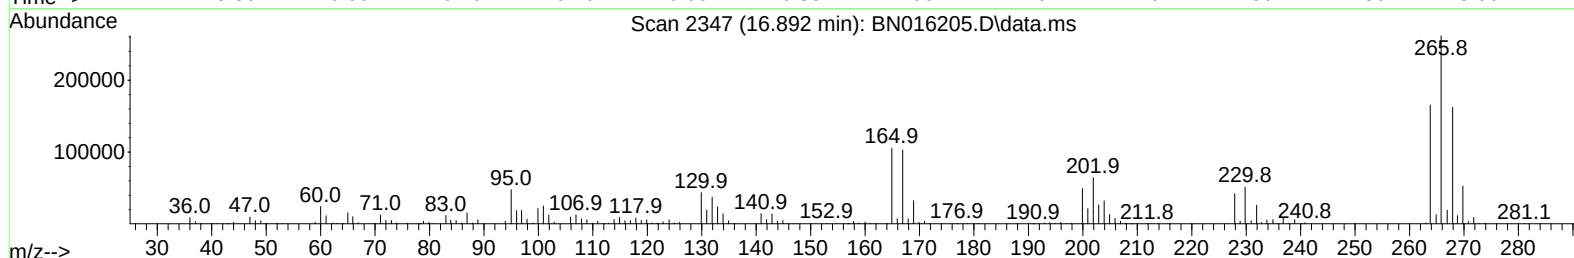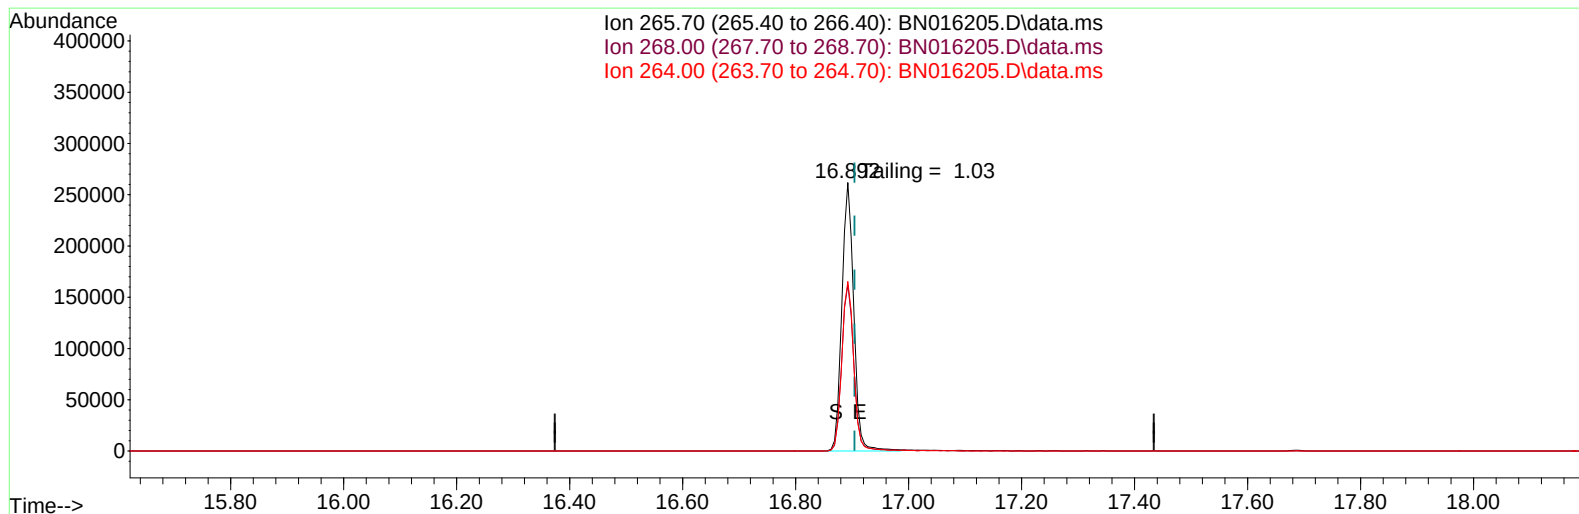

TIC: BN016205.D\data.ms

(70) Pentachlorophenol (C)

16.892min (-0.012) 27162.00 ng




response 383689

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.97
264.00	61.60	63.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090421\
 Data File : BN016205.D
 Acq On : 04 Sep 2021 22:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 06 07:23:19 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 17:12:56 2021
 Response via : Initial Calibration

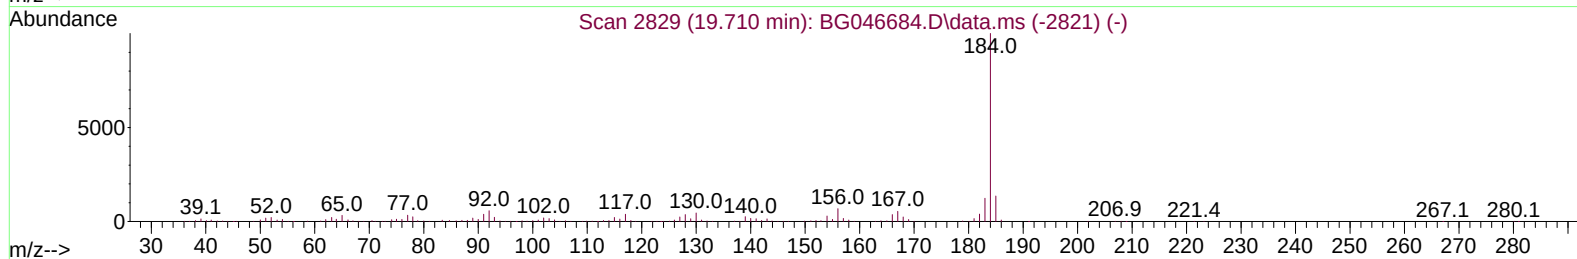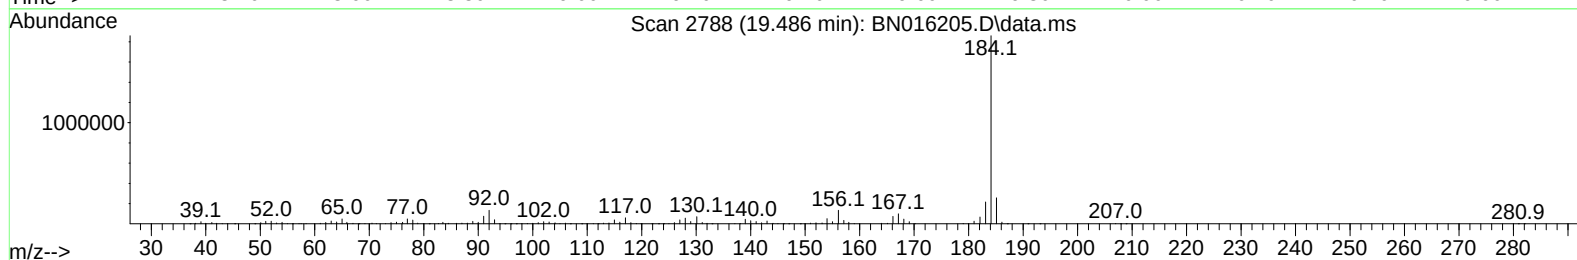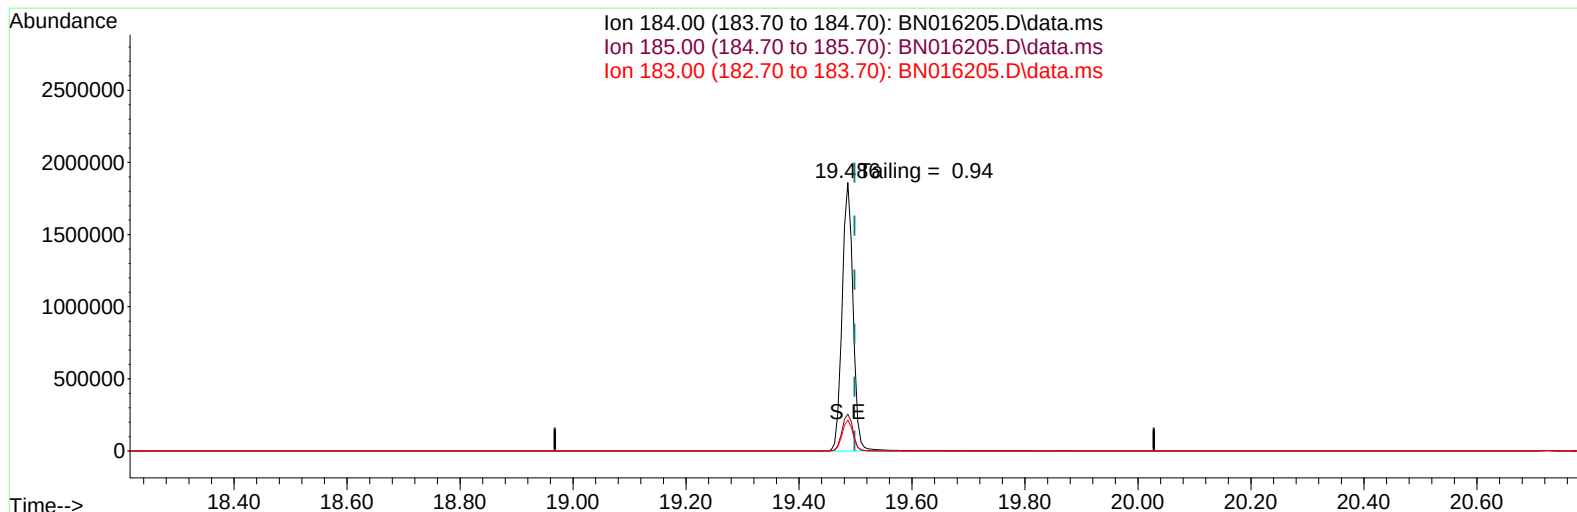

TIC: BN016205.D\data.ms

(77) Benzidine

19.486min (-0.012) 0.00 ng

response 2487909

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.77
183.00	13.20	11.60
0.00	0.00	0.00