
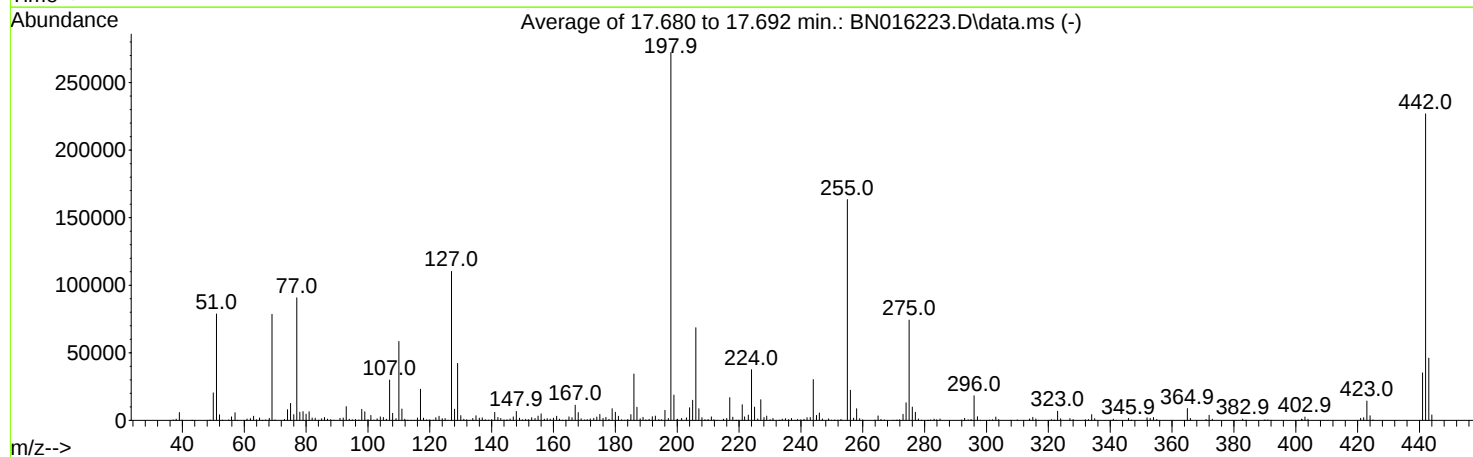


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090421\
 Data File : BN016223.D
 Acq On : 05 Sep 2021 11:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN090421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 06 02:08:58 2021

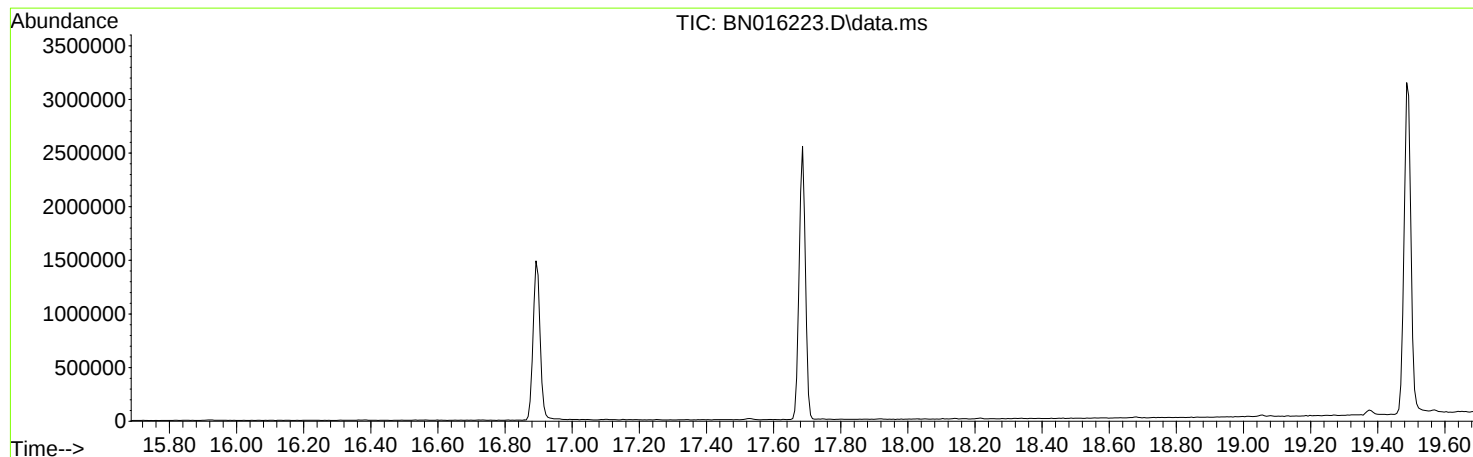

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.9	78797	PASS
68	69	0.00	2	2.0	1532	PASS
69	198	0.00	100	28.8	78467	PASS
70	69	0.00	2	0.5	413	PASS
127	198	10	80	40.5	110264	PASS
197	198	0.00	2	0.5	1403	PASS
198	198	100	100	100.0	272256	PASS
199	198	5	9	6.9	18671	PASS
275	198	10	60	27.3	74269	PASS
365	198	1	100	3.2	8768	PASS
441	198	0.01	100	12.9	35147	PASS
442	442	50	100	100.0	226944	PASS
443	442	15	24	20.3	46104	PASS

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/4/2021	BNA_N	<u>BN016223.D</u>
Compound Name	Response	Retention Time
DDT	932919	20.727
DDD	69520	20.286
DDE	6881	19.775
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
76401	1009320	7.57

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090421\
 Data File : BN016223.D
 Acq On : 05 Sep 2021 11:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 06 07:37:40 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 17:12:56 2021
 Response via : Initial Calibration

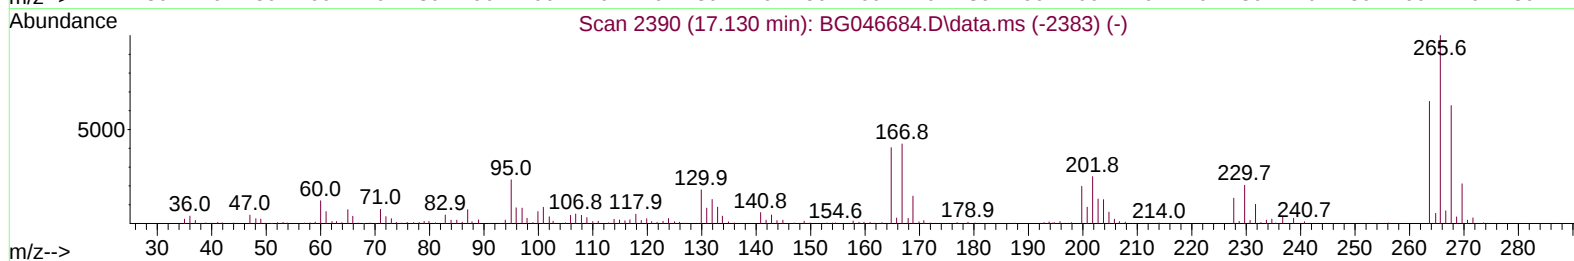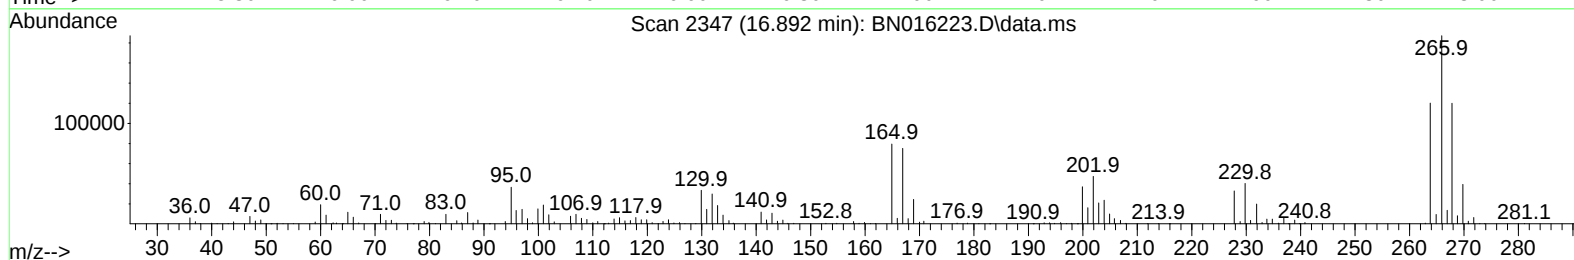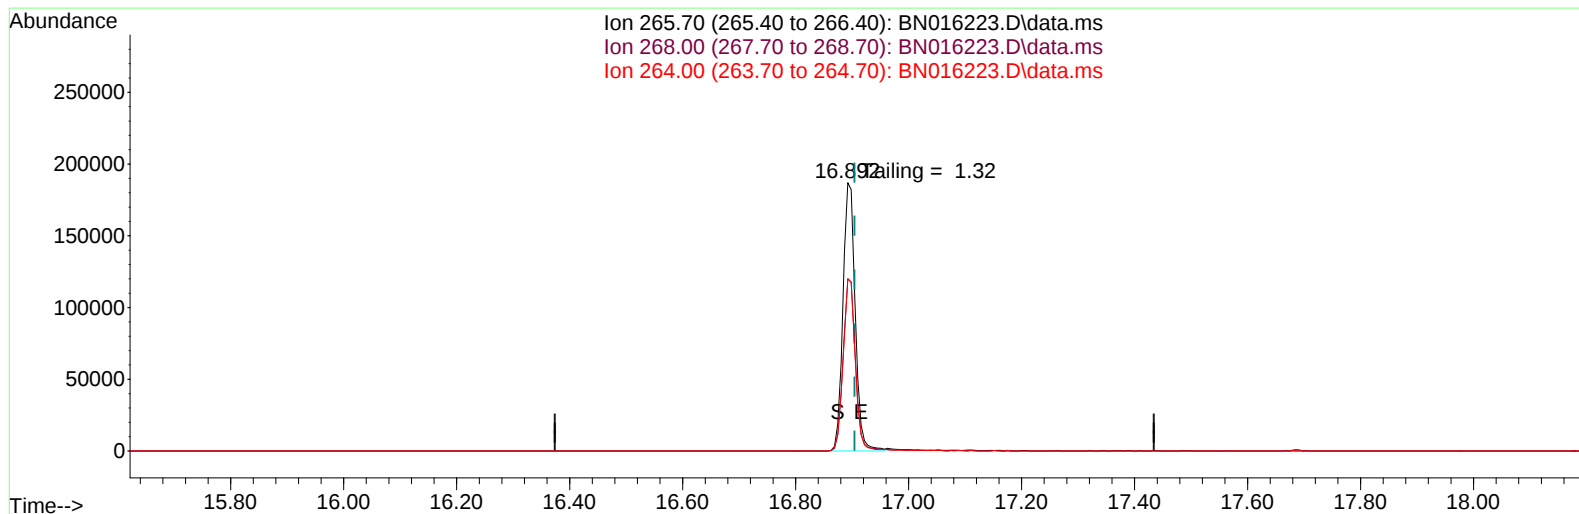

TIC: BN016223.D\data.ms

(70) Pentachlorophenol (C)

16.892min (-0.012) 19040.77 ng




response 280176

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.14
264.00	61.60	64.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090421\
Data File : BN016223.D
Acq On : 05 Sep 2021 11:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 06 07:37:40 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 17:12:56 2021
Response via : Initial Calibration

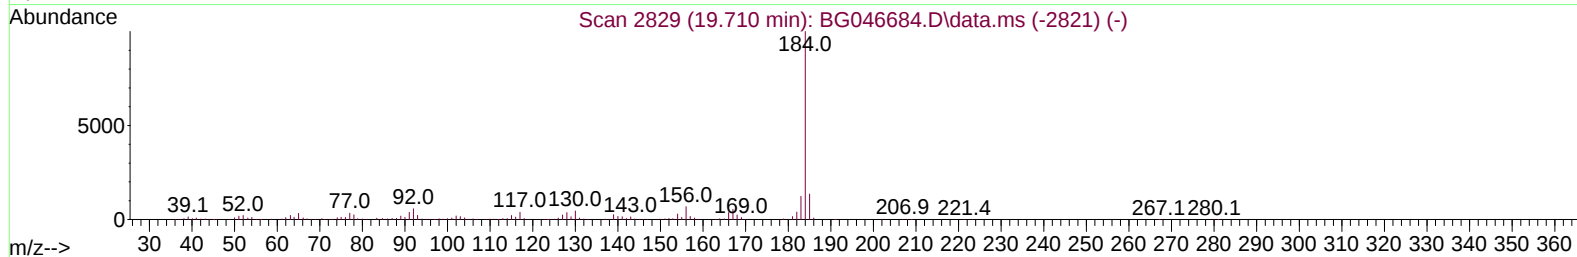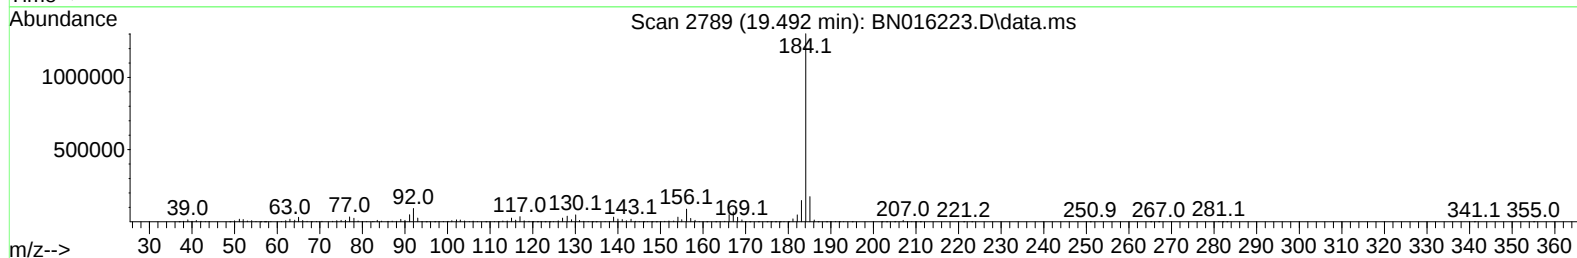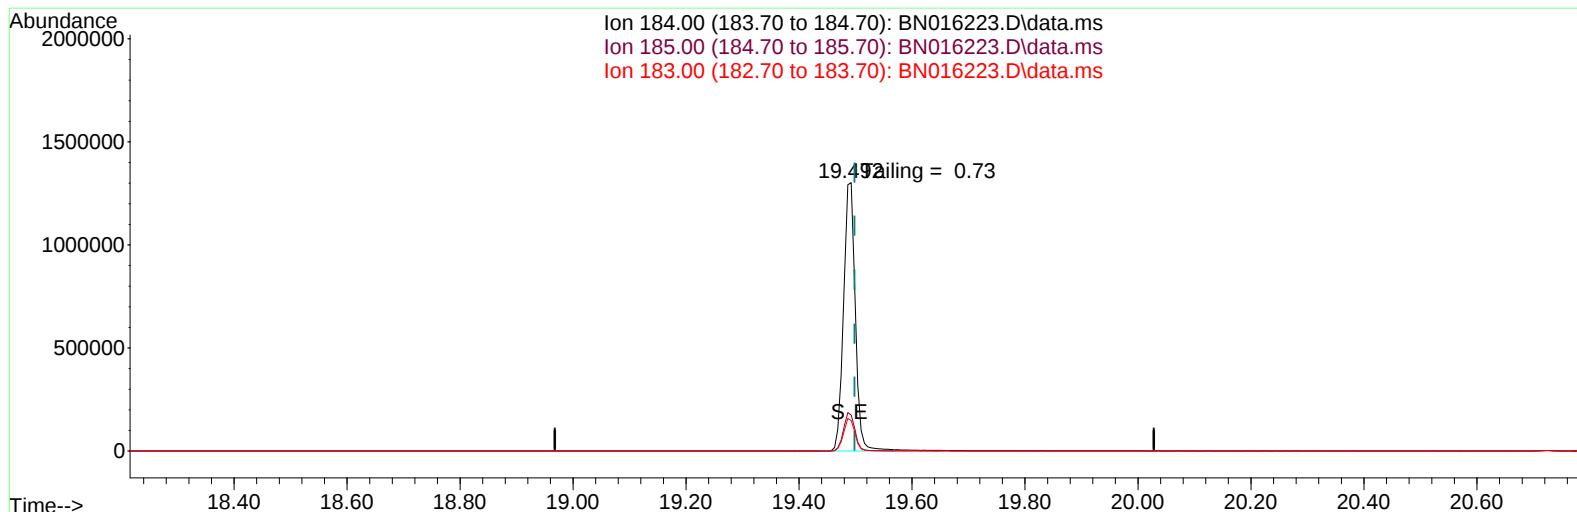

TIC: BN016223.D\data.ms

(77) Benzidine

19.492min (-0.006) 216185.09 ng

response 1885908

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.41
183.00	13.20	11.32
0.00	0.00	0.00