
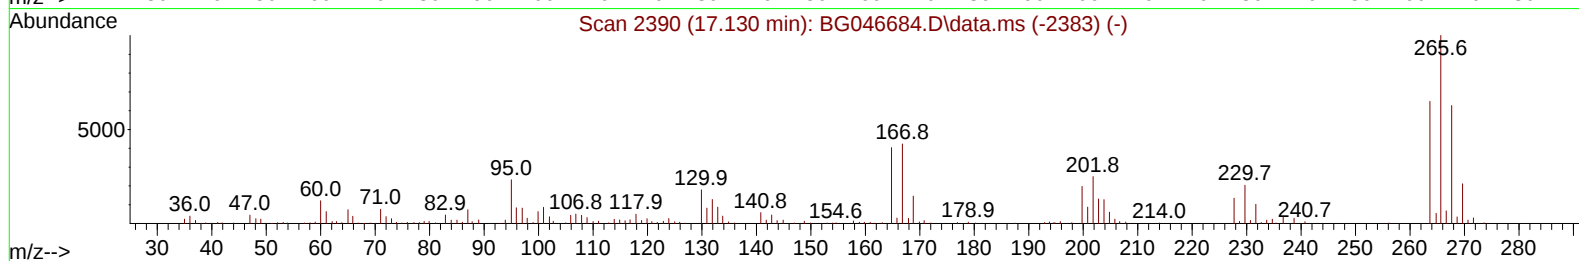
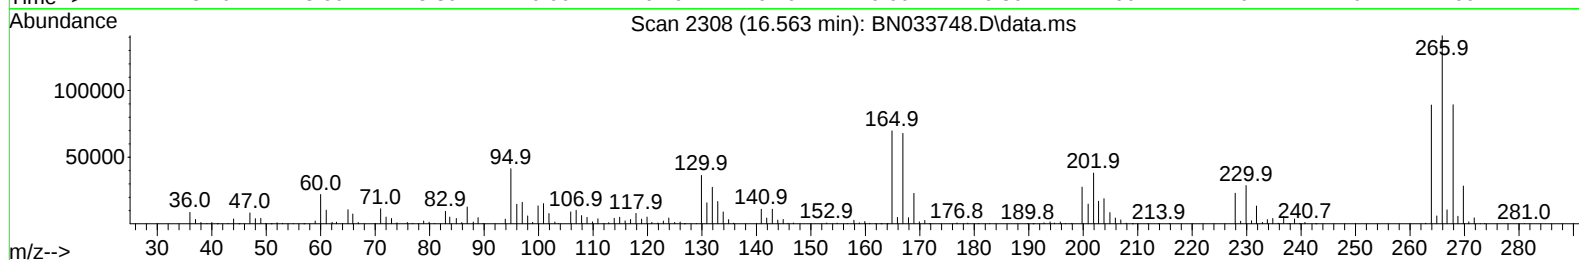


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090424\
Data File : BN033748.D
Acq On : 04 Sep 2024 10:22
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 18:53:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 04:54:27 2024
Response via : Initial Calibration

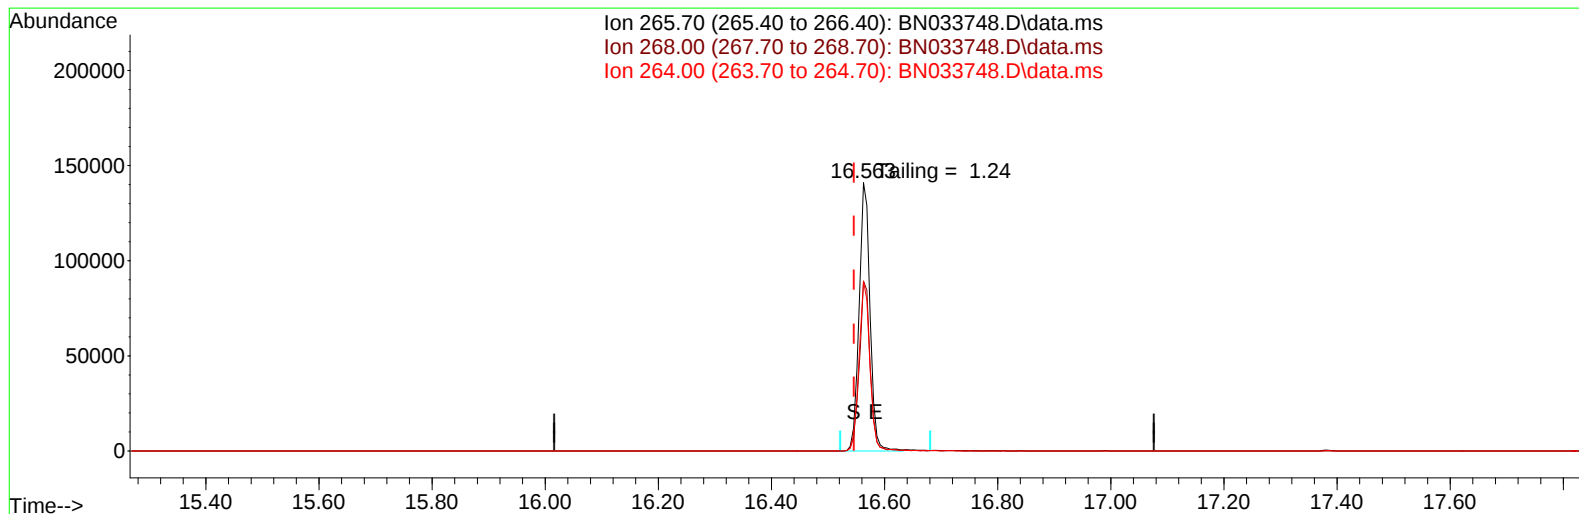

TIC: BN033748.D\data.ms

(70) Pentachlorophenol (C)




16.563min (+ 0.017) 22675.23 ng

response 190228

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.37
264.00	61.60	63.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090424\
Data File : BN033748.D
Acq On : 04 Sep 2024 10:22
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 18:53:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 04:54:27 2024
Response via : Initial Calibration

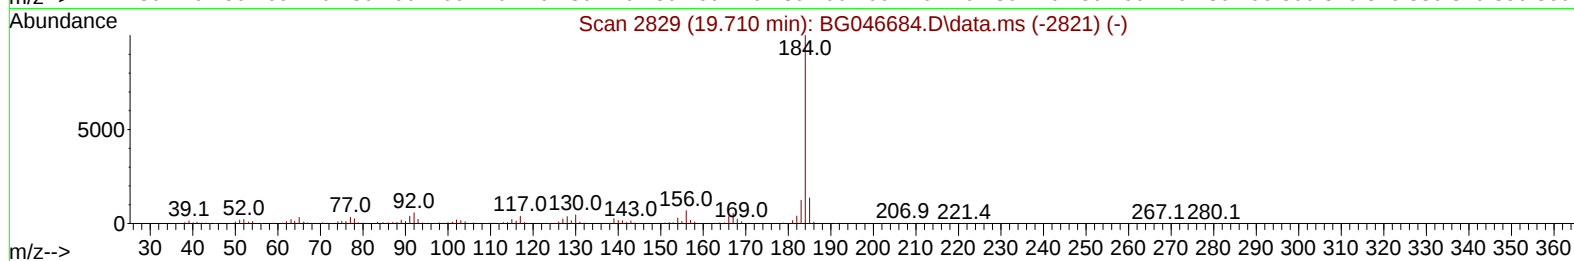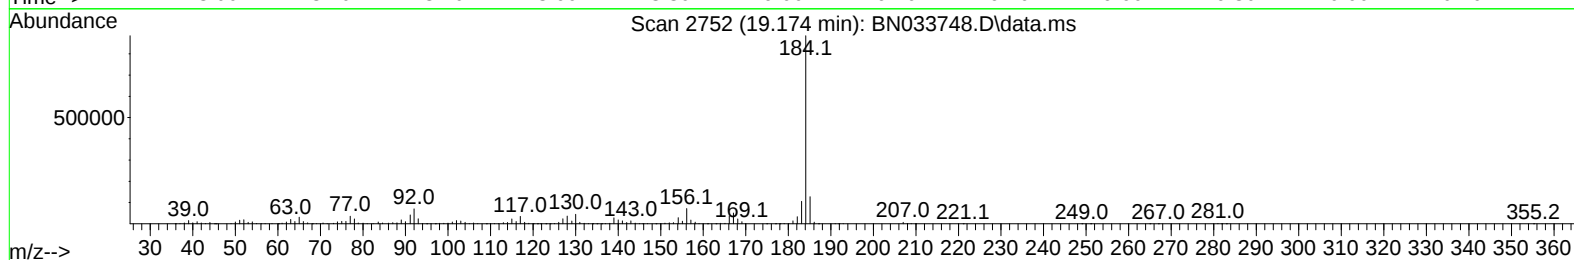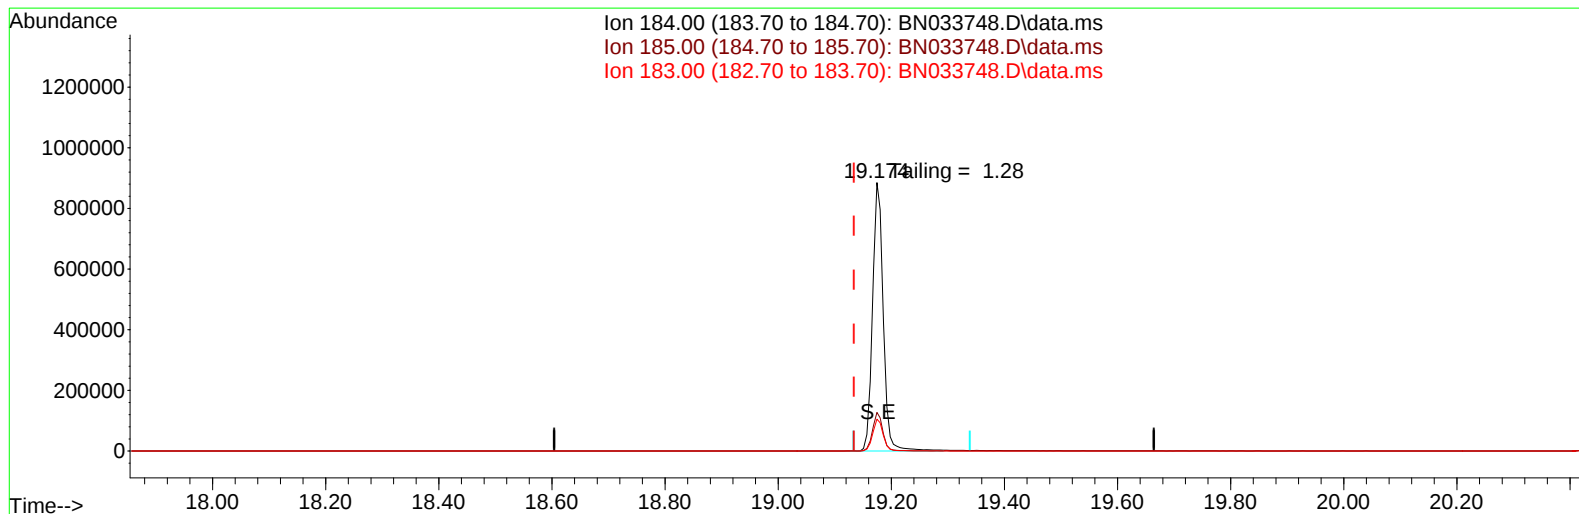

TIC: BN033748.D\data.ms

(77) Benzidine**19.174min (+ 0.040) 0.00 ng****response 1173747**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.39
183.00	13.20	11.89
0.00	0.00	0.00