

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090424\
 Data File : BN033753.D
 Acq On : 04 Sep 2024 15:18
 Operator : MA/JU
 Sample : SSTDICC0.8
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

Quant Time: Sep 04 18:05:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN090424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 04 18:03:07 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.516	152	5370	0.400	ng	0.00
7) Naphthalene-d8	10.272	136	13830	0.400	ng	0.00
13) Acenaphthene-d10	14.157	164	6461	0.400	ng	0.00
19) Phenanthrene-d10	16.905	188	12747	0.400	ng	0.00
29) Chrysene-d12	21.112	240	9954	0.400	ng	0.00
35) Perylene-d12	23.271	264	10135	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.154	112	13812	0.840	ng	0.00
5) Phenol-d6	6.707	99	16156	0.830	ng	0.00
8) Nitrobenzene-d5	8.649	82	9908	0.841	ng	0.00
11) 2-Methylnaphthalene-d10	11.873	152	16548	0.846	ng	0.00
14) 2,4,6-Tribromophenol	15.651	330	2603	0.798	ng	0.00
15) 2-Fluorobiphenyl	12.767	172	22791	0.846	ng	0.00
27) Fluoranthene-d10	18.947	212	25848	0.822	ng	0.00
31) Terphenyl-d14	19.560	244	17597	0.829	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.168	88	5257	0.860	ng	98
3) n-Nitrosodimethylamine	3.457	42	6294	0.877	ng	97
6) bis(2-Chloroethyl)ether	6.960	93	12615	0.859	ng	100
9) Naphthalene	10.325	128	31359	0.849	ng	100
10) Hexachlorobutadiene	10.624	225	6564	0.854	ng	# 100
12) 2-Methylnaphthalene	11.945	142	19201	0.848	ng	99
16) Acenaphthylene	13.868	152	23166	0.830	ng	100
17) Acenaphthene	14.210	154	16201	0.846	ng	100
18) Fluorene	15.204	166	19783	0.838	ng	99
20) 4,6-Dinitro-2-methylph...	15.290	198	1540	0.765	ng	# 66
21) 4-Bromophenyl-phenylether	16.110	248	6102	0.826	ng	98
22) Hexachlorobenzene	16.209	284	7009	0.828	ng	99
23) Atrazine	16.396	200	4843	0.821	ng	97
24) Pentachlorophenol	16.557	266	2773	0.801	ng	99
25) Phenanthrene	16.942	178	29123	0.829	ng	100
26) Anthracene	17.041	178	24820	0.813	ng	100
28) Fluoranthene	18.980	202	32608	0.828	ng	100
30) Pyrene	19.342	202	32920	0.821	ng	100
32) Benzo(a)anthracene	21.104	228	29462	0.829	ng	100
33) Chrysene	21.148	228	29279	0.833	ng	99
34) Bis(2-ethylhexyl)phtha...	21.059	149	15443	0.797	ng	100
36) Indeno(1,2,3-cd)pyrene	25.399	276	35682	0.852	ng	99
37) Benzo(b)fluoranthene	22.633	252	31381	0.843	ng	# 92
38) Benzo(k)fluoranthene	22.674	252	30462	0.839	ng	# 92
39) Benzo(a)pyrene	23.177	252	25911	0.832	ng	# 90
40) Dibenzo(a,h)anthracene	25.414	278	28634	0.853	ng	95
41) Benzo(g,h,i)perylene	26.048	276	31066	0.853	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090424\
Data File : BN033753.D
Acq On : 04 Sep 2024 15:18
Operator : MA/JU
Sample : SSTDICC0.8
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Quant Time: Sep 04 18:05:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 18:03:07 2024
Response via : Initial Calibration

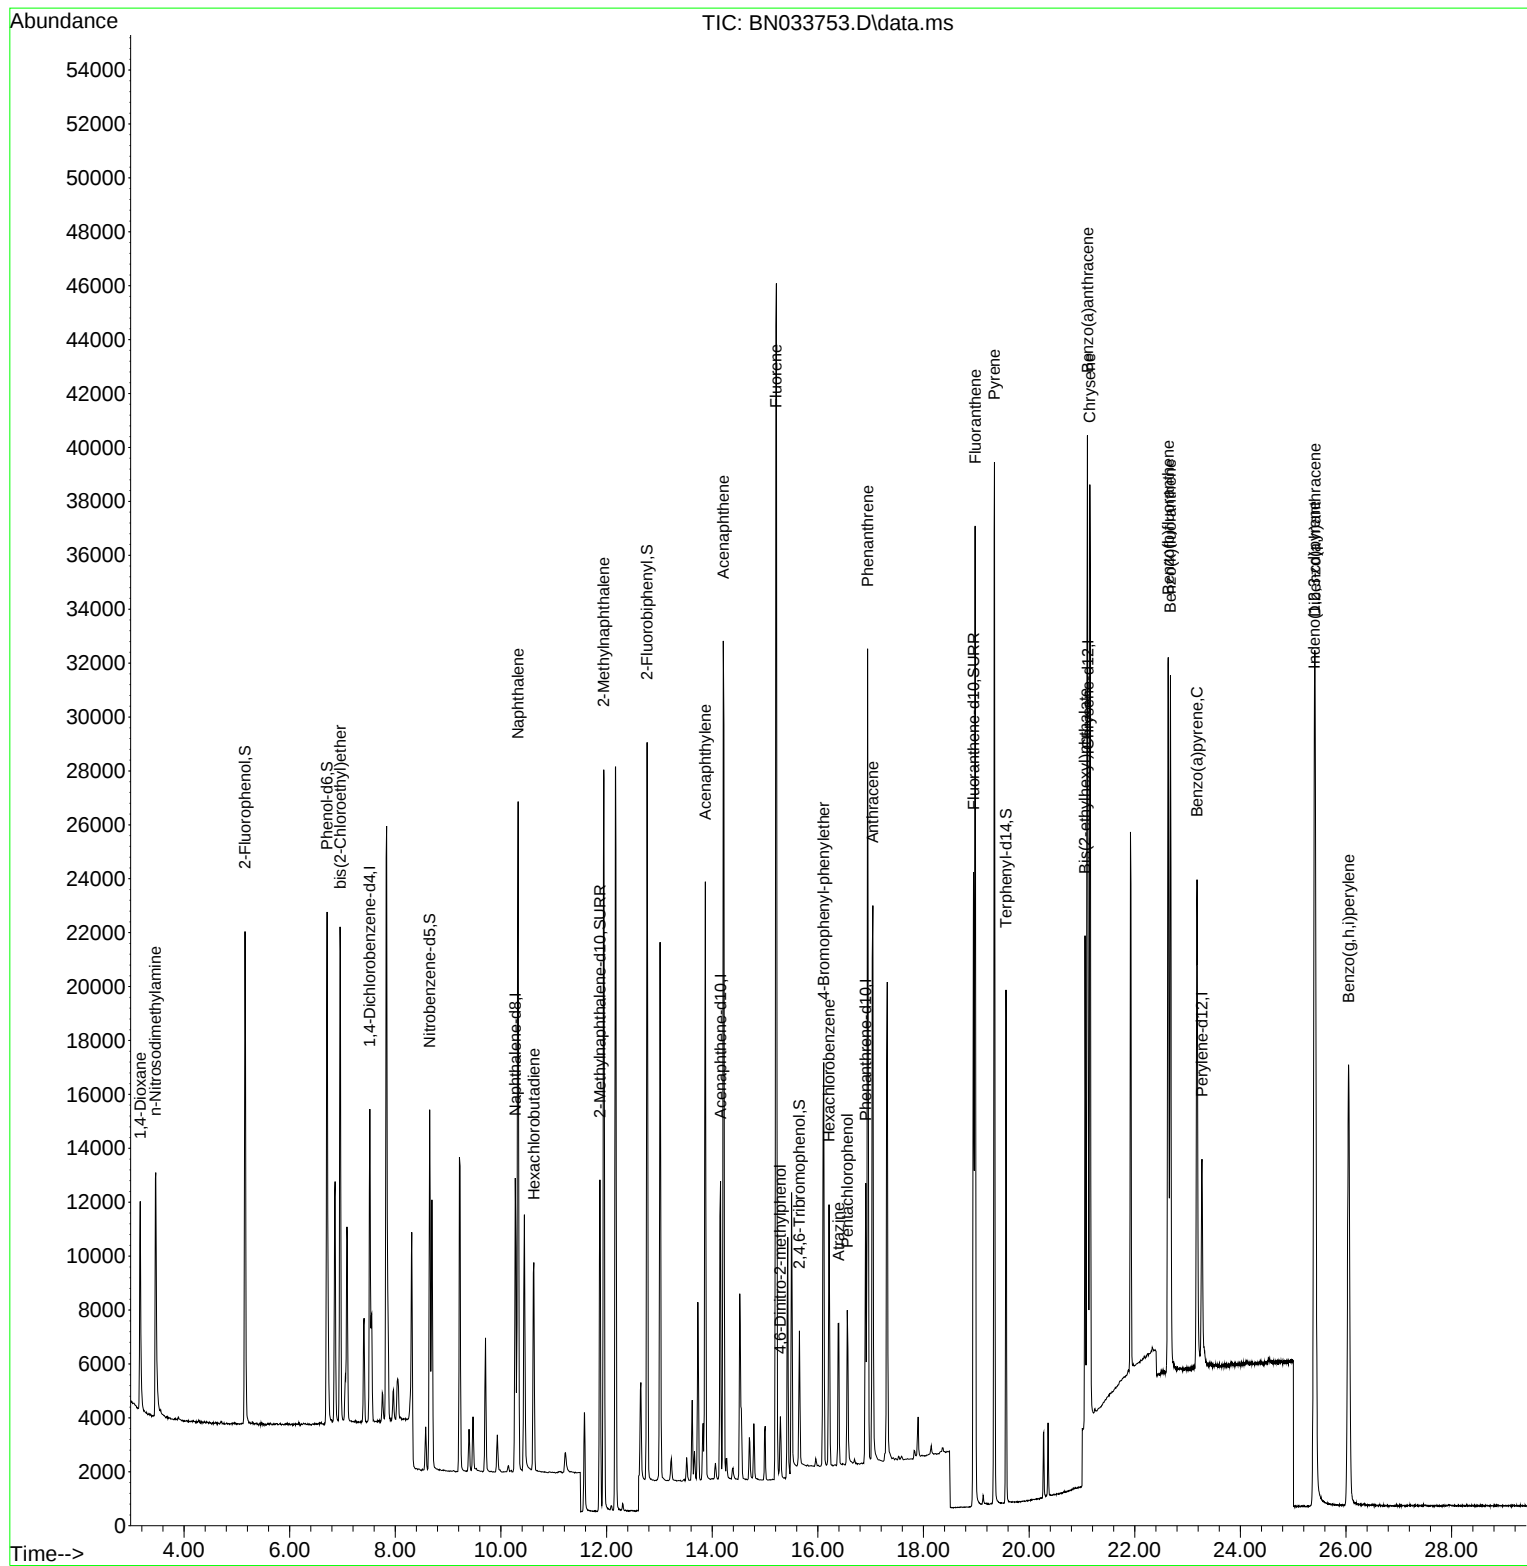





#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.516 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN033753.D
 Acq: 04 Sep 2024 15:18


Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8





Tgt Ion:152 Resp: 5370
 Ion Ratio Lower Upper
 152 100
 150 155.3 123.3 184.9
 115 64.7 51.0 76.4

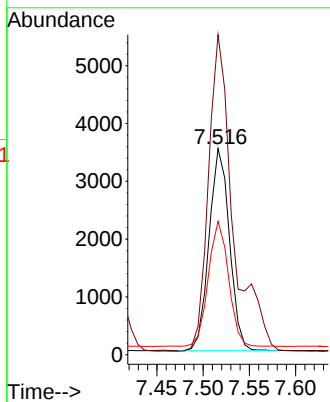

#2
 1,4-Dioxane
 Concen: 0.860 ng
 RT: 3.168 min Scan# 26
 Delta R.T. -0.000 min
 Lab File: BN033753.D
 Acq: 04 Sep 2024 15:18



Tgt Ion: 88 Resp: 5257
 Ion Ratio Lower Upper
 88 100
 43 33.0 29.0 43.4
 58 79.4 64.1 96.1



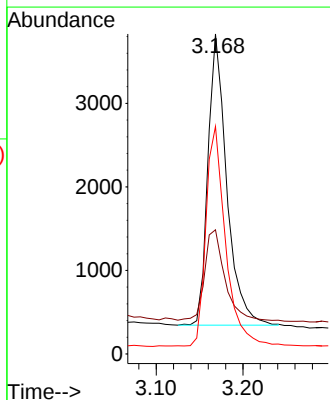





#3
 n-Nitrosodimethylamine
 Concen: 0.877 ng
 RT: 3.457 min Scan# 61
 Delta R.T. -0.007 min
 Lab File: BN033753.D
 Acq: 04 Sep 2024 15:18




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

Tgt Ion:	42	Resp:	6294
Ion	Ratio	Lower	Upper
42	100		
74	113.5	93.5	140.3
44	9.2	7.4	11.0

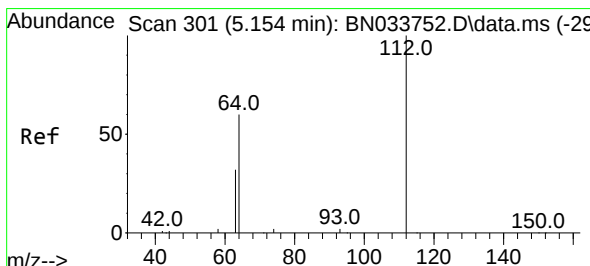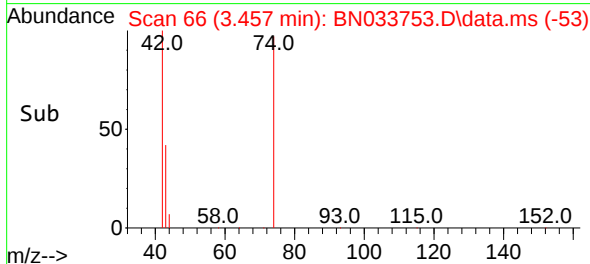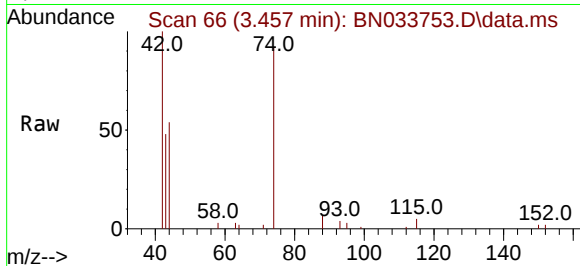

#4
 2-Fluorophenol
 Concen: 0.840 ng
 RT: 5.154 min Scan# 301
 Delta R.T. -0.000 min
 Lab File: BN033753.D
 Acq: 04 Sep 2024 15:18

Tgt Ion:	112	Resp:	13812
Ion	Ratio	Lower	Upper
112	100		
64	60.3	47.6	71.4
63	32.4	25.9	38.9

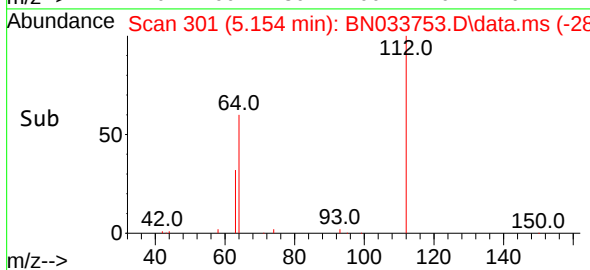

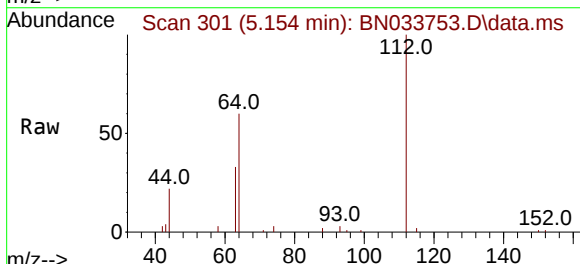




#5
Phenol-d6
Concen: 0.830 ng
RT: 6.707 min Scan# 516
Delta R.T. -0.000 min
Lab File: BN033753.D
Acq: 04 Sep 2024 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion: 99 Resp: 16156
Ion Ratio Lower Upper
99 100
42 22.1 18.0 27.0
71 35.7 28.7 43.1

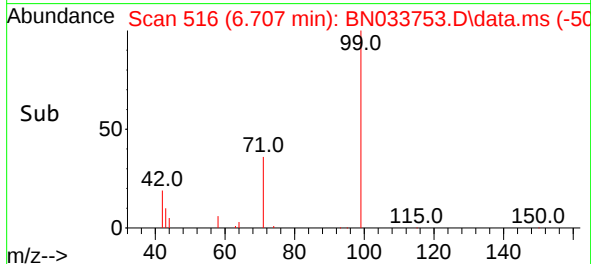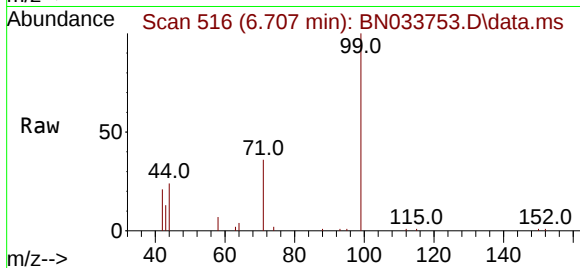

#6
bis(2-Chloroethyl)ether
Concen: 0.859 ng
RT: 6.960 min Scan# 551
Delta R.T. -0.000 min
Lab File: BN033753.D
Acq: 04 Sep 2024 15:18

Tgt Ion: 93 Resp: 12615
Ion Ratio Lower Upper
93 100
63 80.3 64.4 96.6
95 32.8 26.5 39.7




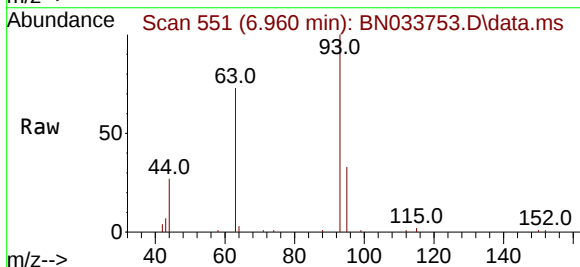




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.272 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN033753.D
Acq: 04 Sep 2024 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:	136	Resp:	13830
Ion	Ratio	Lower	Upper
136	100		
137	11.3	9.0	13.4
54	9.9	8.1	12.1
68	7.0	5.8	8.8

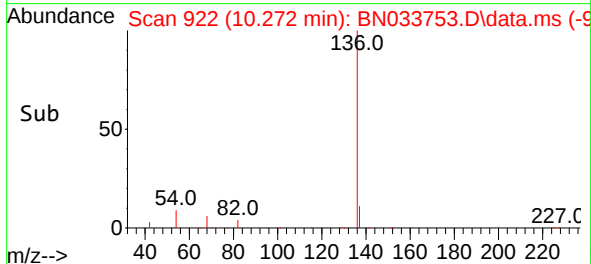

#8
Nitrobenzene-d5
Concen: 0.841 ng
RT: 8.649 min Scan# 770
Delta R.T. -0.000 min
Lab File: BN033753.D
Acq: 04 Sep 2024 15:18

Tgt Ion:	82	Resp:	9908
Ion	Ratio	Lower	Upper
82	100		
128	38.2	31.3	46.9
54	57.6	46.9	70.3





#9

Naphthalene

Concen: 0.849 ng

RT: 10.325 min Scan# 91

Delta R.T. -0.000 min

Lab File: BN033753.D

Acq: 04 Sep 2024 15:18

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:128 Resp: 31359

Ion Ratio Lower Upper

128 100

129 11.2 8.9 13.3

127 13.2 10.8 16.2

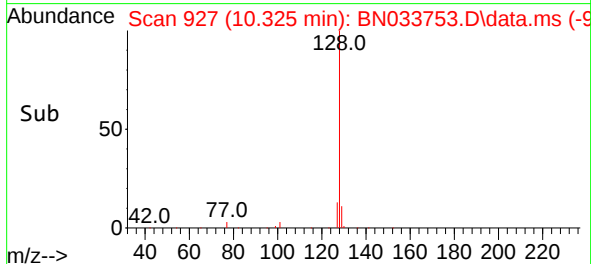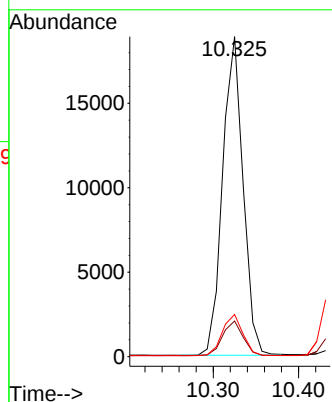

#10

Hexachlorobutadiene

Concen: 0.854 ng

RT: 10.624 min Scan# 955

Delta R.T. -0.000 min

Lab File: BN033753.D

Acq: 04 Sep 2024 15:18




Tgt Ion:225 Resp: 6564


Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 64.2 51.2 76.8


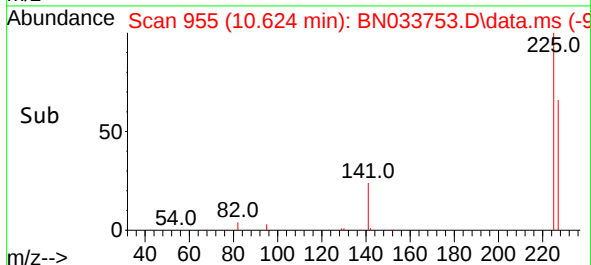




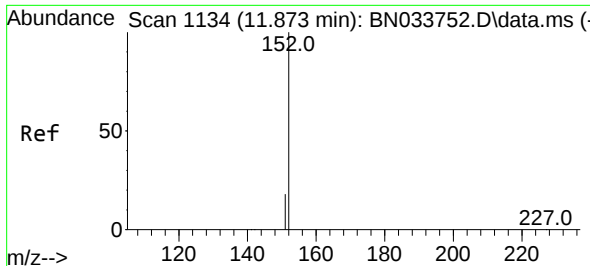

#11
2-Methylnaphthalene-d10
Concen: 0.846 ng
RT: 11.873 min Scan# 1134
Delta R.T. -0.000 min
Lab File: BN033753.D
Acq: 04 Sep 2024 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:152 Resp: 16548
Ion Ratio Lower Upper
152 100
151 20.8 16.7 25.1

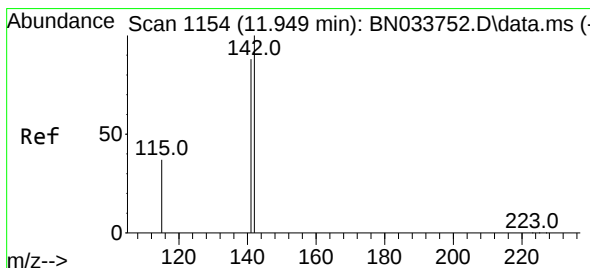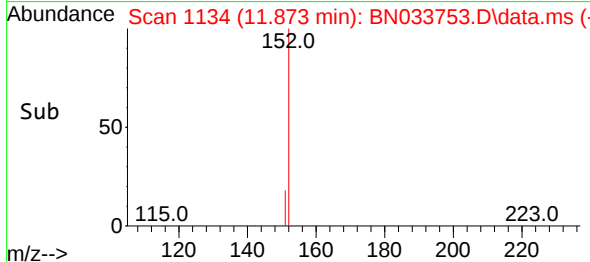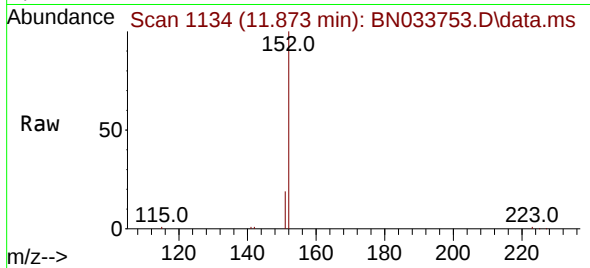

#12
2-Methylnaphthalene
Concen: 0.848 ng
RT: 11.945 min Scan# 1153
Delta R.T. -0.004 min
Lab File: BN033753.D
Acq: 04 Sep 2024 15:18

Tgt Ion:142 Resp: 19201
Ion Ratio Lower Upper
142 100
141 89.8 70.9 106.3
115 38.9 31.0 46.4


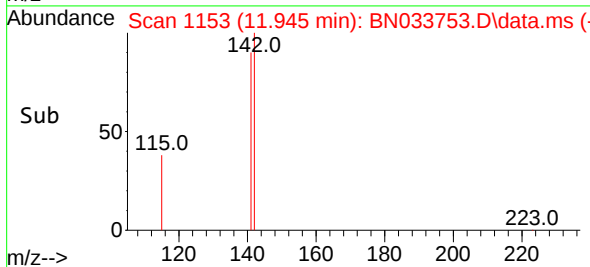

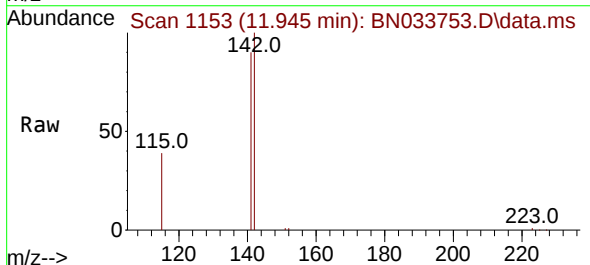




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.157 min Scan# 1473
Delta R.T. -0.000 min
Lab File: BN033753.D
Acq: 04 Sep 2024 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Tgt Ion:164 Resp: 6461
Ion Ratio Lower Upper
164 100
162 103.1 82.0 123.0
160 49.4 39.1 58.7

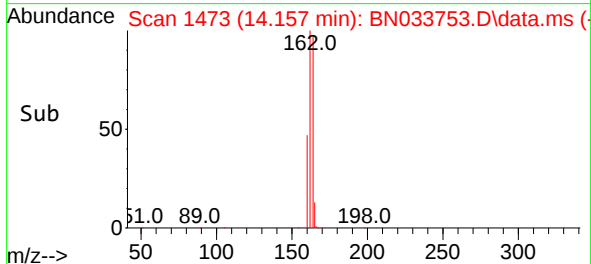

#14
2,4,6-Tribromophenol
Concen: 0.798 ng
RT: 15.651 min Scan# 1611
Delta R.T. -0.000 min
Lab File: BN033753.D
Acq: 04 Sep 2024 15:18

Tgt Ion:330 Resp: 2603
Ion Ratio Lower Upper
330 100
332 96.9 74.2 111.4
141 44.3 33.9 50.9








#15
2-Fluorobiphenyl
Concen: 0.846 ng
RT: 12.767 min Scan# 1343
Delta R.T. -0.000 min
Lab File: BN033753.D
Acq: 04 Sep 2024 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:	172	Resp:	22791
Ion Ratio	Lower	Upper	
172	100		
171	35.6	28.8	43.2
170	24.6	19.7	29.5

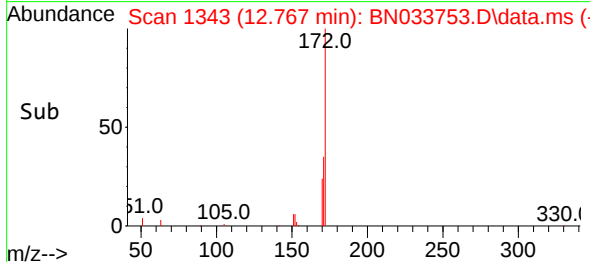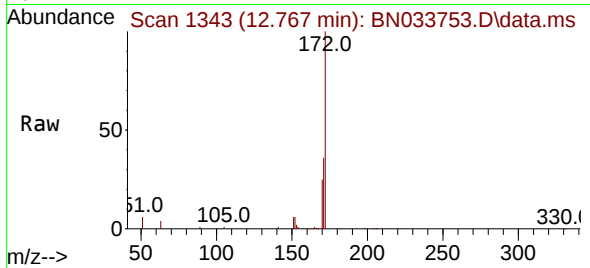

#16
Acenaphthylene
Concen: 0.830 ng
RT: 13.868 min Scan# 1446
Delta R.T. -0.000 min
Lab File: BN033753.D
Acq: 04 Sep 2024 15:18

Tgt Ion:	152	Resp:	23166
Ion Ratio	Lower	Upper	
152	100		
151	19.5	15.6	23.4
153	13.1	10.3	15.5

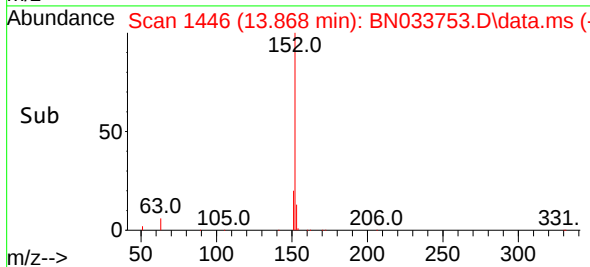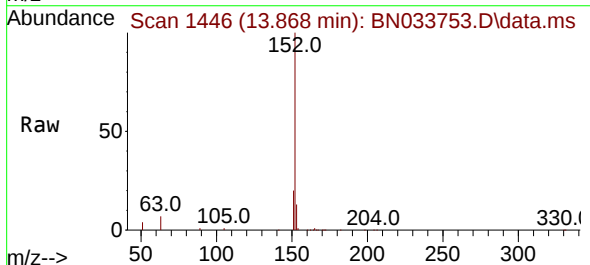

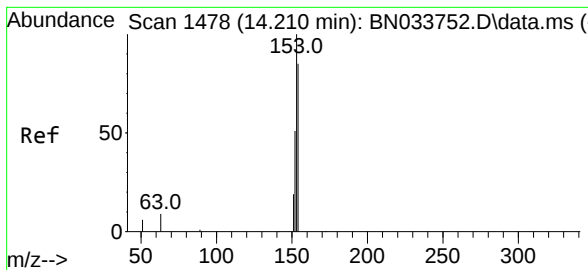

#17

Acenaphthene

Concen: 0.846 ng

RT: 14.210 min Scan# 1478

Delta R.T. -0.000 min

Lab File: BN033753.D

Acq: 04 Sep 2024 15:18

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:154 Resp: 16201

Ion Ratio Lower Upper

154 100

153 114.2 91.4 137.2

152 57.4 45.8 68.6

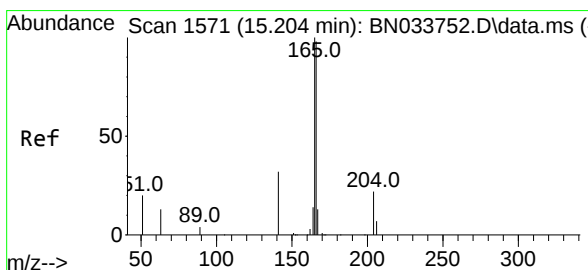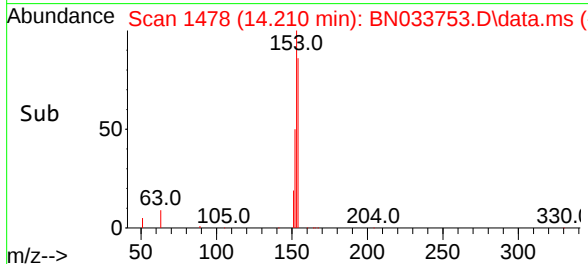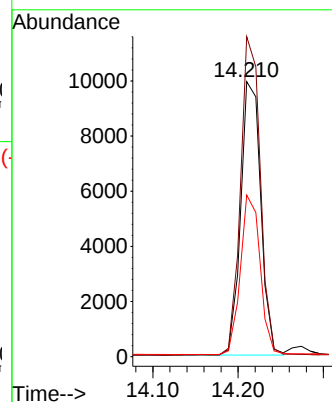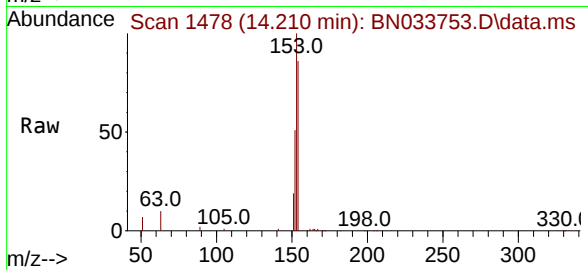

#18

Fluorene

Concen: 0.838 ng

RT: 15.204 min Scan# 1571

Delta R.T. -0.000 min

Lab File: BN033753.D

Acq: 04 Sep 2024 15:18




Tgt Ion:166 Resp: 19783


Ion Ratio Lower Upper

166 100

165 99.3 78.8 118.2

167 13.4 10.6 16.0

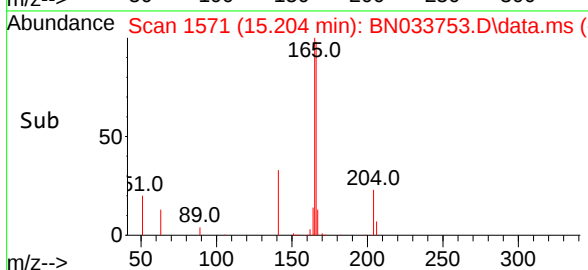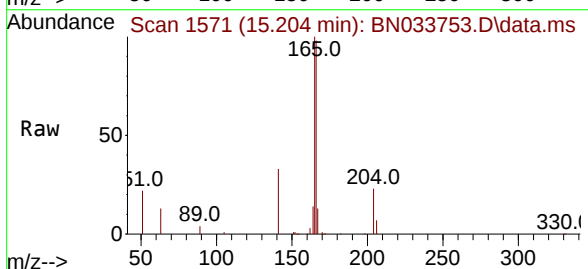



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.905 min Scan# 1712

Delta R.T. -0.000 min

Lab File: BN033753.D

Acq: 04 Sep 2024 15:18

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:188 Resp: 12747

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 9.6 7.9 11.9

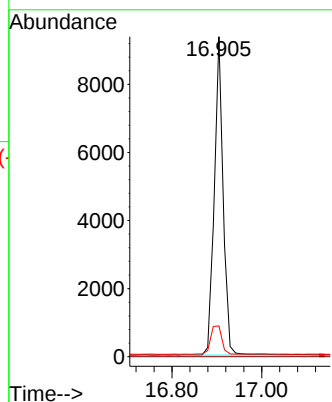

#20

4,6-Dinitro-2-methylphenol

Concen: 0.765 ng

RT: 15.290 min Scan# 1579

Delta R.T. -0.000 min

Lab File: BN033753.D

Acq: 04 Sep 2024 15:18




Tgt Ion:198 Resp: 1540


Ion Ratio Lower Upper

198 100

51 70.3 92.8 139.2#

105 55.8 59.4 89.0#



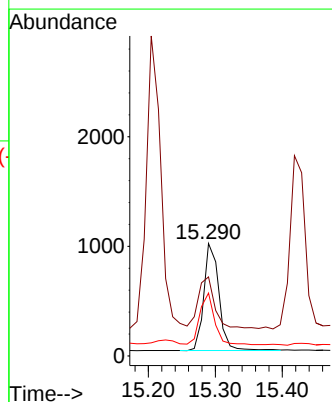



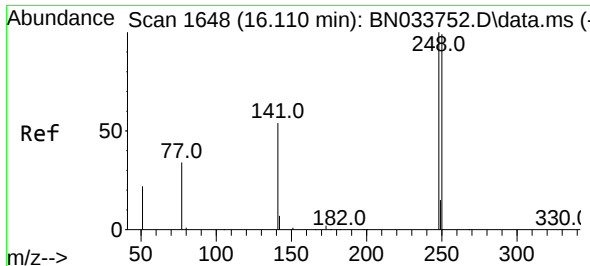

#21
4-Bromophenyl-phenylether
Concen: 0.826 ng
RT: 16.110 min Scan# 1648
Delta R.T. -0.000 min
Lab File: BN033753.D
Acq: 04 Sep 2024 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:248 Resp: 6102
Ion Ratio Lower Upper
248 100
250 99.0 79.5 119.3
141 52.7 44.9 67.3

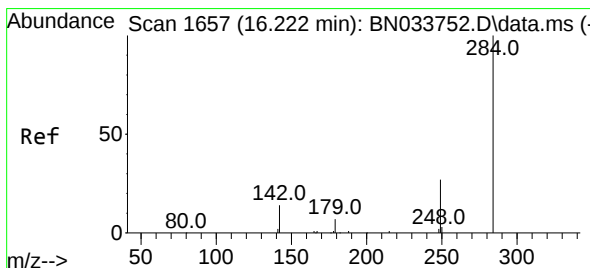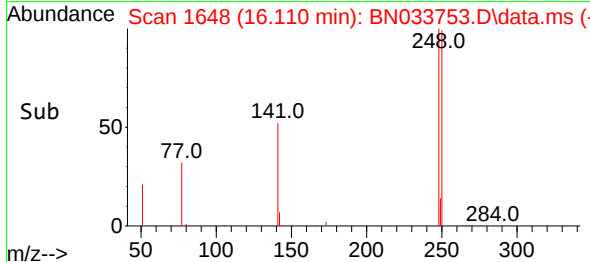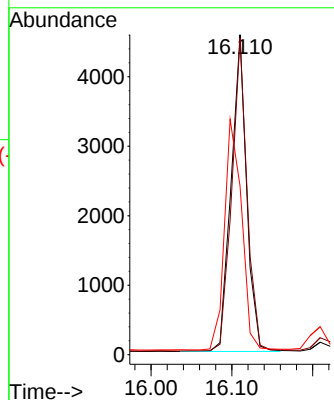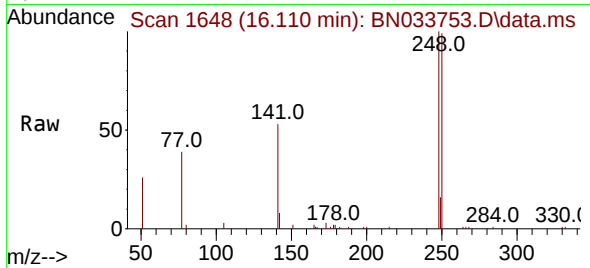

#22
Hexachlorobenzene
Concen: 0.828 ng
RT: 16.209 min Scan# 1656
Delta R.T. -0.012 min
Lab File: BN033753.D
Acq: 04 Sep 2024 15:18

Tgt Ion:284 Resp: 7009
Ion Ratio Lower Upper
284 100
142 42.0 32.8 49.2
249 33.1 26.2 39.2


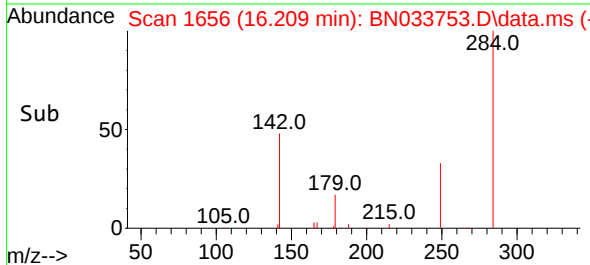
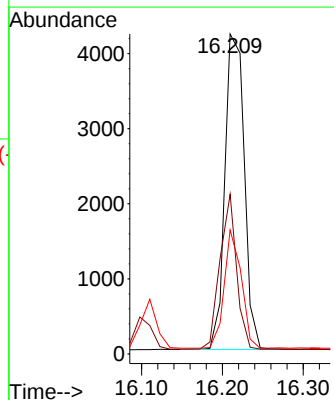
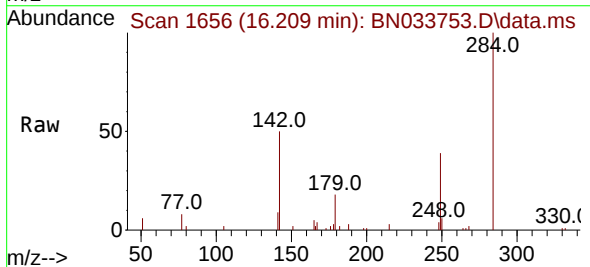


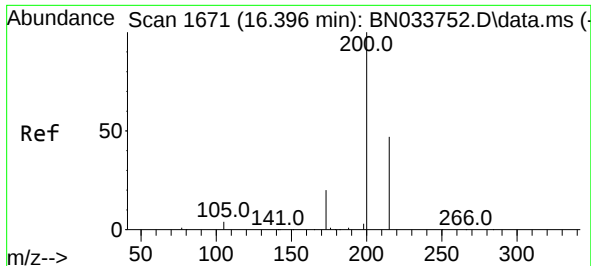

#23
Atrazine
Concen: 0.821 ng
RT: 16.396 min Scan# 1671
Delta R.T. -0.000 min
Lab File: BN033753.D
Acq: 04 Sep 2024 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:200 Resp: 4843
Ion Ratio Lower Upper
200 100
173 21.4 18.2 27.4
215 47.0 39.0 58.4

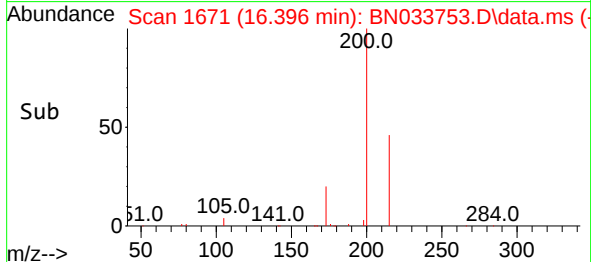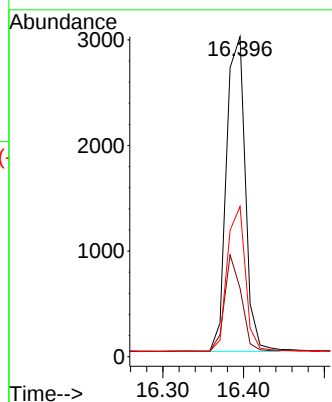

#24
Pentachlorophenol
Concen: 0.801 ng
RT: 16.557 min Scan# 1684
Delta R.T. -0.012 min
Lab File: BN033753.D
Acq: 04 Sep 2024 15:18

Tgt Ion:266 Resp: 2773
Ion Ratio Lower Upper
266 100
264 63.0 49.6 74.4
268 64.3 52.2 78.4

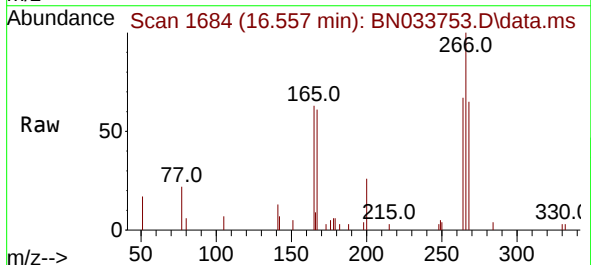



#25

Phenanthrene

Concen: 0.829 ng

RT: 16.942 min Scan# 1715

Delta R.T. -0.000 min

Lab File: BN033753.D

Acq: 04 Sep 2024 15:18

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:178 Resp: 29123

Ion Ratio Lower Upper

178 100

176 19.1 15.4 23.0

179 15.3 12.2 18.4

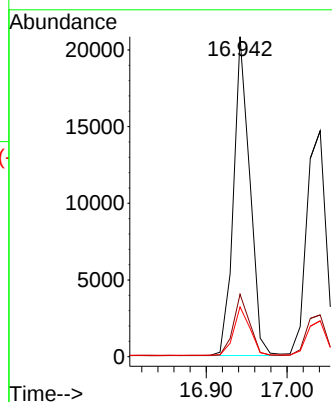

#26

Anthracene

Concen: 0.813 ng

RT: 17.041 min Scan# 1723

Delta R.T. -0.000 min

Lab File: BN033753.D

Acq: 04 Sep 2024 15:18




Tgt Ion:178 Resp: 24820


Ion Ratio Lower Upper

178 100

176 18.5 14.8 22.2

179 15.1 12.4 18.6




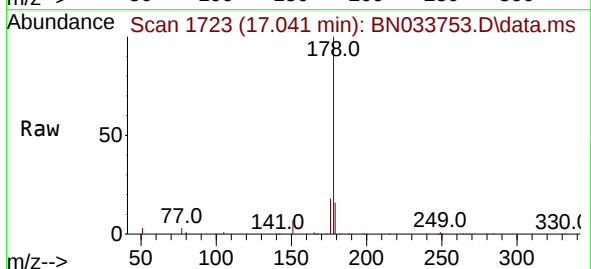


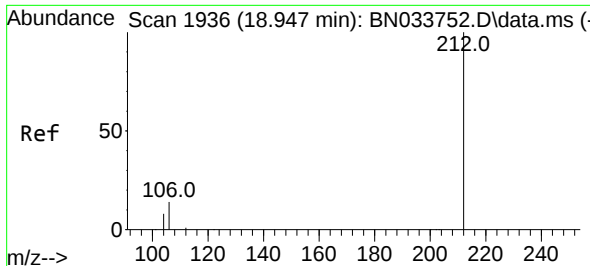

#27
Fluoranthene-d10
Concen: 0.822 ng
RT: 18.947 min Scan# 1936
Delta R.T. -0.000 min
Lab File: BN033753.D
Acq: 04 Sep 2024 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:212 Resp: 25848
Ion Ratio Lower Upper
212 100
106 14.1 11.5 17.3
104 8.3 6.6 9.8

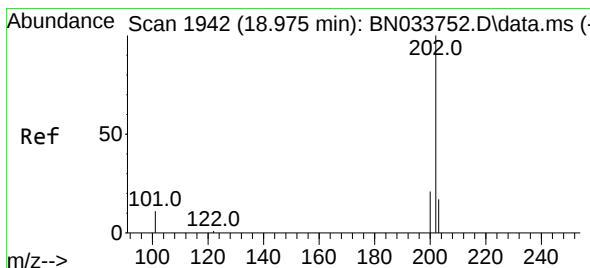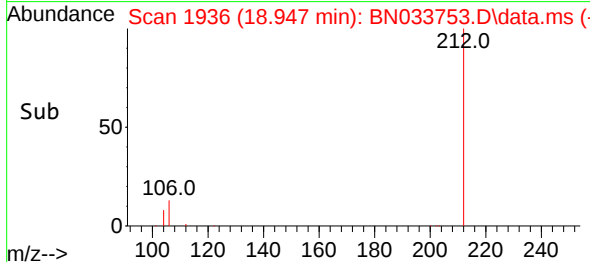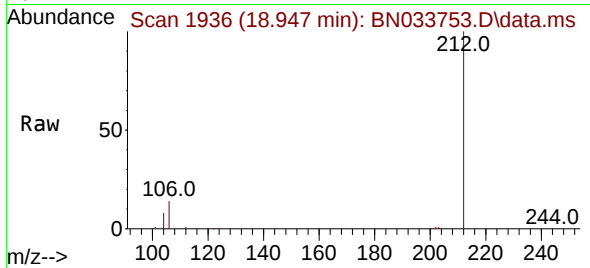

#28
Fluoranthene
Concen: 0.828 ng
RT: 18.980 min Scan# 1943
Delta R.T. 0.005 min
Lab File: BN033753.D
Acq: 04 Sep 2024 15:18

Tgt Ion:202 Resp: 32608
Ion Ratio Lower Upper
202 100
101 11.4 9.2 13.8
203 17.2 13.8 20.6


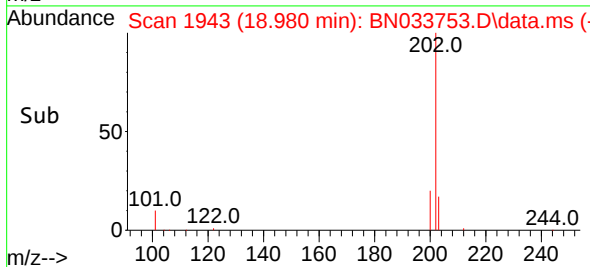

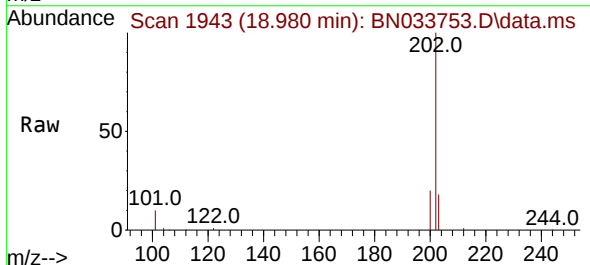




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.112 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN033753.D
Acq: 04 Sep 2024 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:240 Resp: 9954
Ion Ratio Lower Upper
240 100
120 20.1 13.7 20.5
236 28.9 23.4 35.2

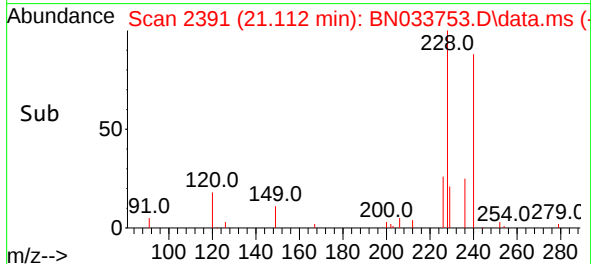

#30
Pyrene
Concen: 0.821 ng
RT: 19.342 min Scan# 2021
Delta R.T. -0.000 min
Lab File: BN033753.D
Acq: 04 Sep 2024 15:18

Tgt Ion:202 Resp: 32920
Ion Ratio Lower Upper
202 100
200 21.0 16.8 25.2
203 17.9 14.4 21.6




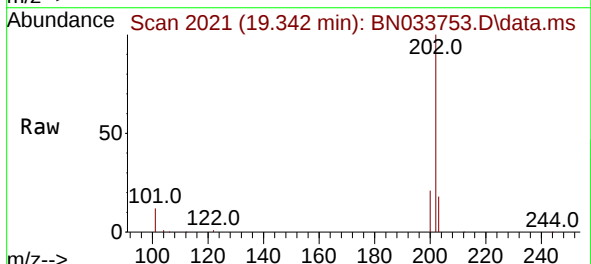


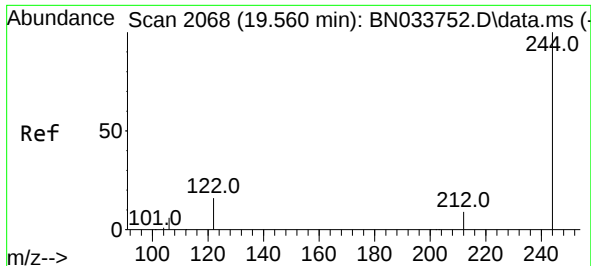

#31
 Terphenyl-d14
 Concen: 0.829 ng
 RT: 19.560 min Scan# 2068
 Delta R.T. -0.000 min
 Lab File: BN033753.D
 Acq: 04 Sep 2024 15:18




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8


Tgt Ion:244 Resp: 17597
 Ion Ratio Lower Upper
 244 100
 212 9.6 7.9 11.9
 122 16.6 13.2 19.8

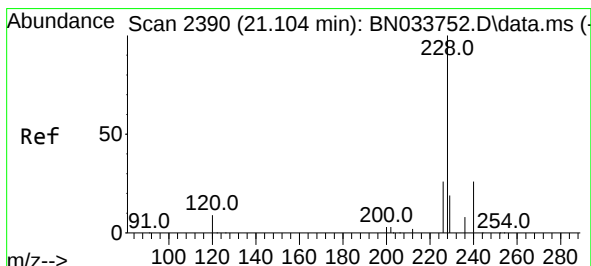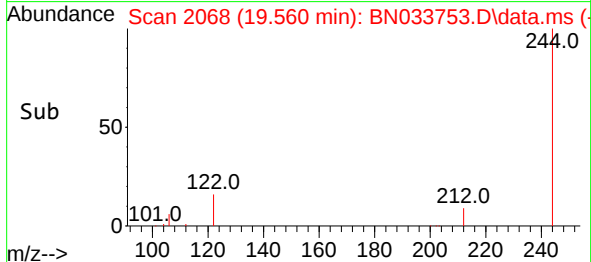

#32
 Benzo(a)anthracene
 Concen: 0.829 ng
 RT: 21.104 min Scan# 2390
 Delta R.T. -0.000 min
 Lab File: BN033753.D
 Acq: 04 Sep 2024 15:18

Tgt Ion:228 Resp: 29462
 Ion Ratio Lower Upper
 228 100
 226 26.6 21.2 31.8
 229 19.9 15.9 23.9



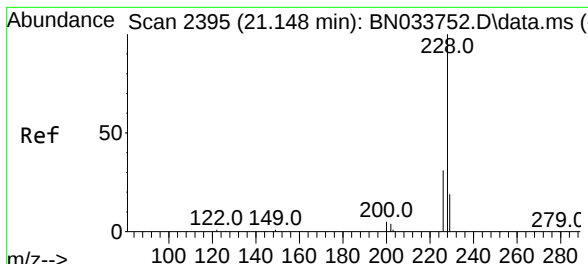

#33

Chrysene

Concen: 0.833 ng

RT: 21.148 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN033753.D

Acq: 04 Sep 2024 15:18

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:228 Resp: 29279

Ion Ratio Lower Upper

228 100

226 30.8 25.0 37.6

229 19.2 15.6 23.4

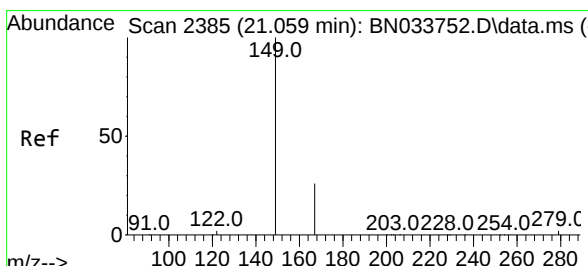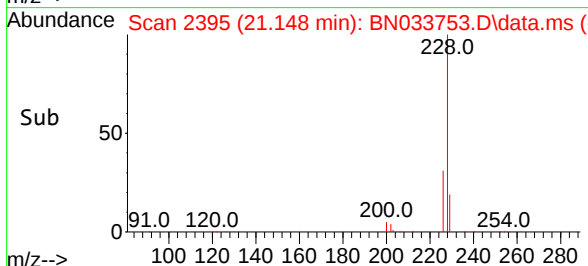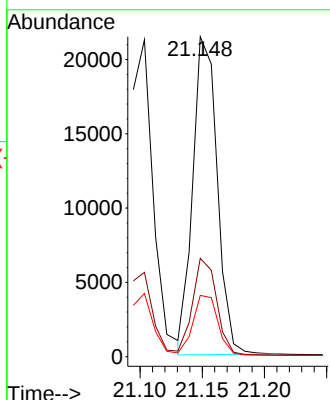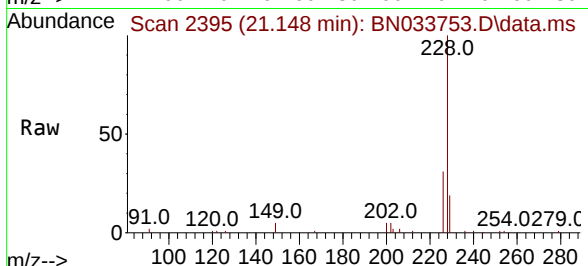

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.797 ng

RT: 21.059 min Scan# 2385

Delta R.T. -0.000 min

Lab File: BN033753.D

Acq: 04 Sep 2024 15:18




Tgt Ion:149 Resp: 15443


Ion Ratio Lower Upper

149 100

167 26.4 21.0 31.4

279 3.1 2.4 3.6


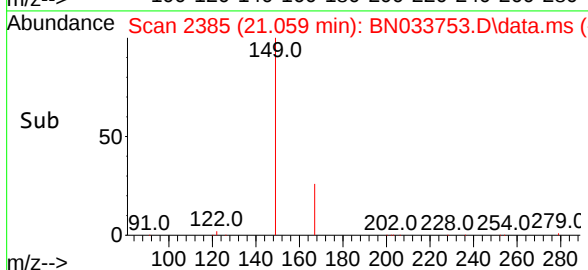
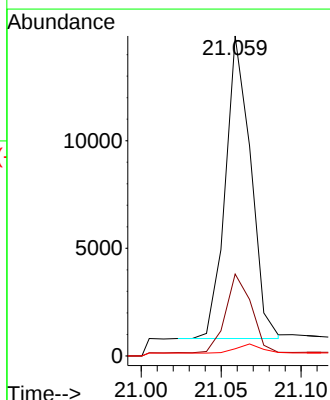
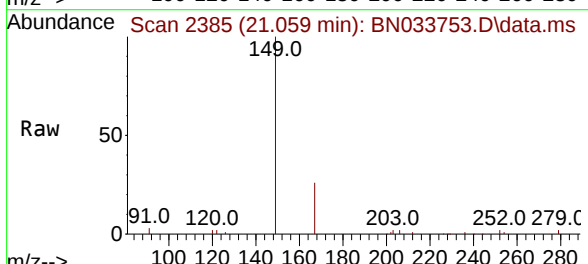




#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.271 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN033753.D
 Acq: 04 Sep 2024 15:18




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

Tgt Ion:264 Resp: 10135
 Ion Ratio Lower Upper
 264 100
 260 26.2 21.1 31.7
 265 89.4 72.0 108.0

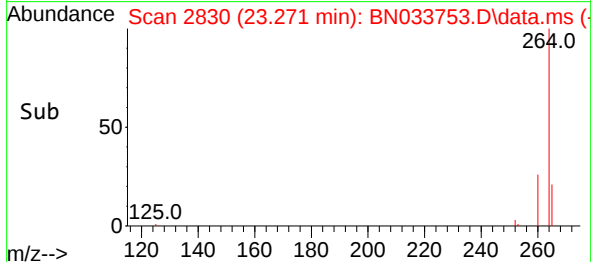

#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.852 ng
 RT: 25.399 min Scan# 3558
 Delta R.T. -0.003 min
 Lab File: BN033753.D
 Acq: 04 Sep 2024 15:18

Tgt Ion:276 Resp: 35682
 Ion Ratio Lower Upper
 276 100
 138 28.5 23.0 34.6
 277 24.7 20.2 30.4




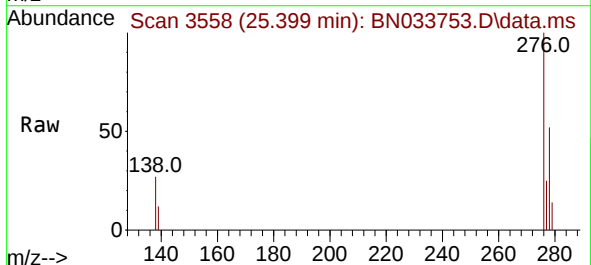




#37
Benzo(b)fluoranthene
Concen: 0.843 ng
RT: 22.633 min Scan# 2611
Delta R.T. 0.003 min
Lab File: BN033753.D
Acq: 04 Sep 2024 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Tgt Ion:252 Resp: 31381
Ion Ratio Lower Upper
252 100
253 24.3 21.8 32.6
125 14.4 15.4 23.0#

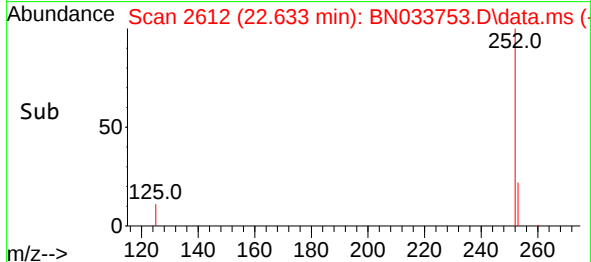

#38
Benzo(k)fluoranthene
Concen: 0.839 ng
RT: 22.674 min Scan# 2626
Delta R.T. -0.000 min
Lab File: BN033753.D
Acq: 04 Sep 2024 15:18

Tgt Ion:252 Resp: 30462
Ion Ratio Lower Upper
252 100
253 24.2 21.8 32.8
125 14.5 15.4 23.2#

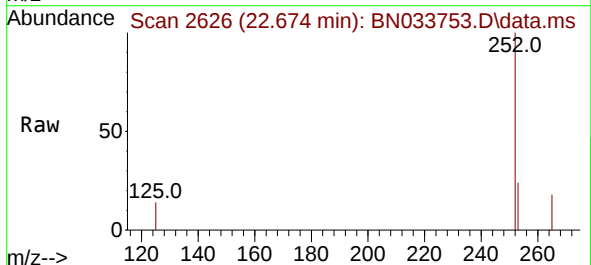



#39

Benzo(a)pyrene

Concen: 0.832 ng

RT: 23.177 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN033753.D


Acq: 04 Sep 2024 15:18

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8






Tgt Ion:252 Resp: 25911

Ion Ratio Lower Upper

252 100

253 25.4 24.0 36.0

125 17.5 19.1 28.7#

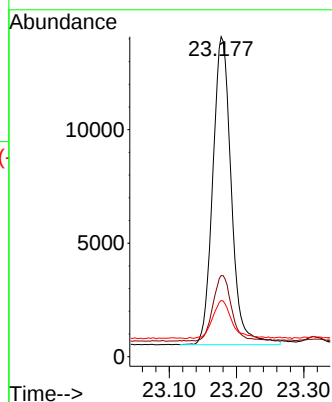

#40

Dibenzo(a,h)anthracene

Concen: 0.853 ng

RT: 25.414 min Scan# 3563

Delta R.T. -0.003 min

Lab File: BN033753.D

Acq: 04 Sep 2024 15:18




Tgt Ion:278 Resp: 28634

Ion Ratio Lower Upper

278 100

139 19.9 16.7 25.1

279 25.4 23.4 35.0





#41

Benzo(g,h,i)perylene

Concen: 0.853 ng

RT: 26.048 min Scan# 31

Delta R.T. -0.000 min

Lab File: BN033753.D


Acq: 04 Sep 2024 15:18

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8

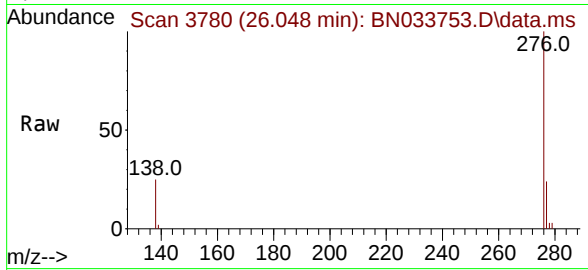

Tgt Ion:276 Resp: 31066

Ion Ratio Lower Upper

276 100

277 24.4 20.3 30.5

138 24.5 20.9 31.3

