

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090424\
 Data File : BN033754.D
 Acq On : 04 Sep 2024 15:54
 Operator : MA/JU
 Sample : SSTDICC1.6
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Quant Time: Sep 04 18:05:29 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN090424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 04 18:03:07 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.516	152	5411	0.400	ng	0.00
7) Naphthalene-d8	10.272	136	13930	0.400	ng	0.00
13) Acenaphthene-d10	14.157	164	6595	0.400	ng	0.00
19) Phenanthrene-d10	16.905	188	12815	0.400	ng	0.00
29) Chrysene-d12	21.113	240	10603	0.400	ng	0.00
35) Perylene-d12	23.271	264	10665	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.154	112	27004	1.630	ng	0.00
5) Phenol-d6	6.707	99	32166	1.640	ng	0.00
8) Nitrobenzene-d5	8.649	82	19563	1.649	ng	0.00
11) 2-Methylnaphthalene-d10	11.873	152	32906	1.671	ng	0.00
14) 2,4,6-Tribromophenol	15.651	330	5530	1.660	ng	0.00
15) 2-Fluorobiphenyl	12.767	172	45458	1.653	ng	0.00
27) Fluoranthene-d10	18.947	212	53870	1.704	ng	0.00
31) Terphenyl-d14	19.560	244	36539	1.616	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.168	88	10043	1.631	ng	98
3) n-Nitrosodimethylamine	3.457	42	12340	1.707	ng	# 97
6) bis(2-Chloroethyl)ether	6.953	93	24581	1.661	ng	99
9) Naphthalene	10.325	128	61713	1.659	ng	99
10) Hexachlorobutadiene	10.624	225	12795	1.652	ng	# 100
12) 2-Methylnaphthalene	11.949	142	38202	1.675	ng	99
16) Acenaphthylene	13.868	152	48158	1.689	ng	100
17) Acenaphthene	14.210	154	32443	1.660	ng	100
18) Fluorene	15.204	166	40575	1.683	ng	100
20) 4,6-Dinitro-2-methylph...	15.290	198	3487	1.723	ng	# 53
21) 4-Bromophenyl-phenylether	16.110	248	12450	1.677	ng	96
22) Hexachlorobenzene	16.209	284	14017	1.646	ng	98
23) Atrazine	16.396	200	10154	1.713	ng	96
24) Pentachlorophenol	16.557	266	5969	1.715	ng	99
25) Phenanthrene	16.942	178	59360	1.681	ng	100
26) Anthracene	17.041	178	51869	1.690	ng	99
28) Fluoranthene	18.975	202	68510	1.731	ng	100
30) Pyrene	19.342	202	68965	1.614	ng	100
32) Benzo(a)anthracene	21.104	228	62876	1.661	ng	100
33) Chrysene	21.148	228	61836	1.652	ng	99
34) Bis(2-ethylhexyl)phtha...	21.059	149	32496	1.574	ng	99
36) Indeno(1,2,3-cd)pyrene	25.402	276	74558	1.691	ng	99
37) Benzo(b)fluoranthene	22.633	252	66033	1.685	ng	# 89
38) Benzo(k)fluoranthene	22.674	252	64560	1.690	ng	# 89
39) Benzo(a)pyrene	23.177	252	54955	1.677	ng	# 85
40) Dibenzo(a,h)anthracene	25.420	278	60034	1.699	ng	93
41) Benzo(g,h,i)perylene	26.045	276	64526	1.684	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090424\
Data File : BN033754.D
Acq On : 04 Sep 2024 15:54
Operator : MA/JU
Sample : SSTDICC1.6
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Quant Time: Sep 04 18:05:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 18:03:07 2024
Response via : Initial Calibration



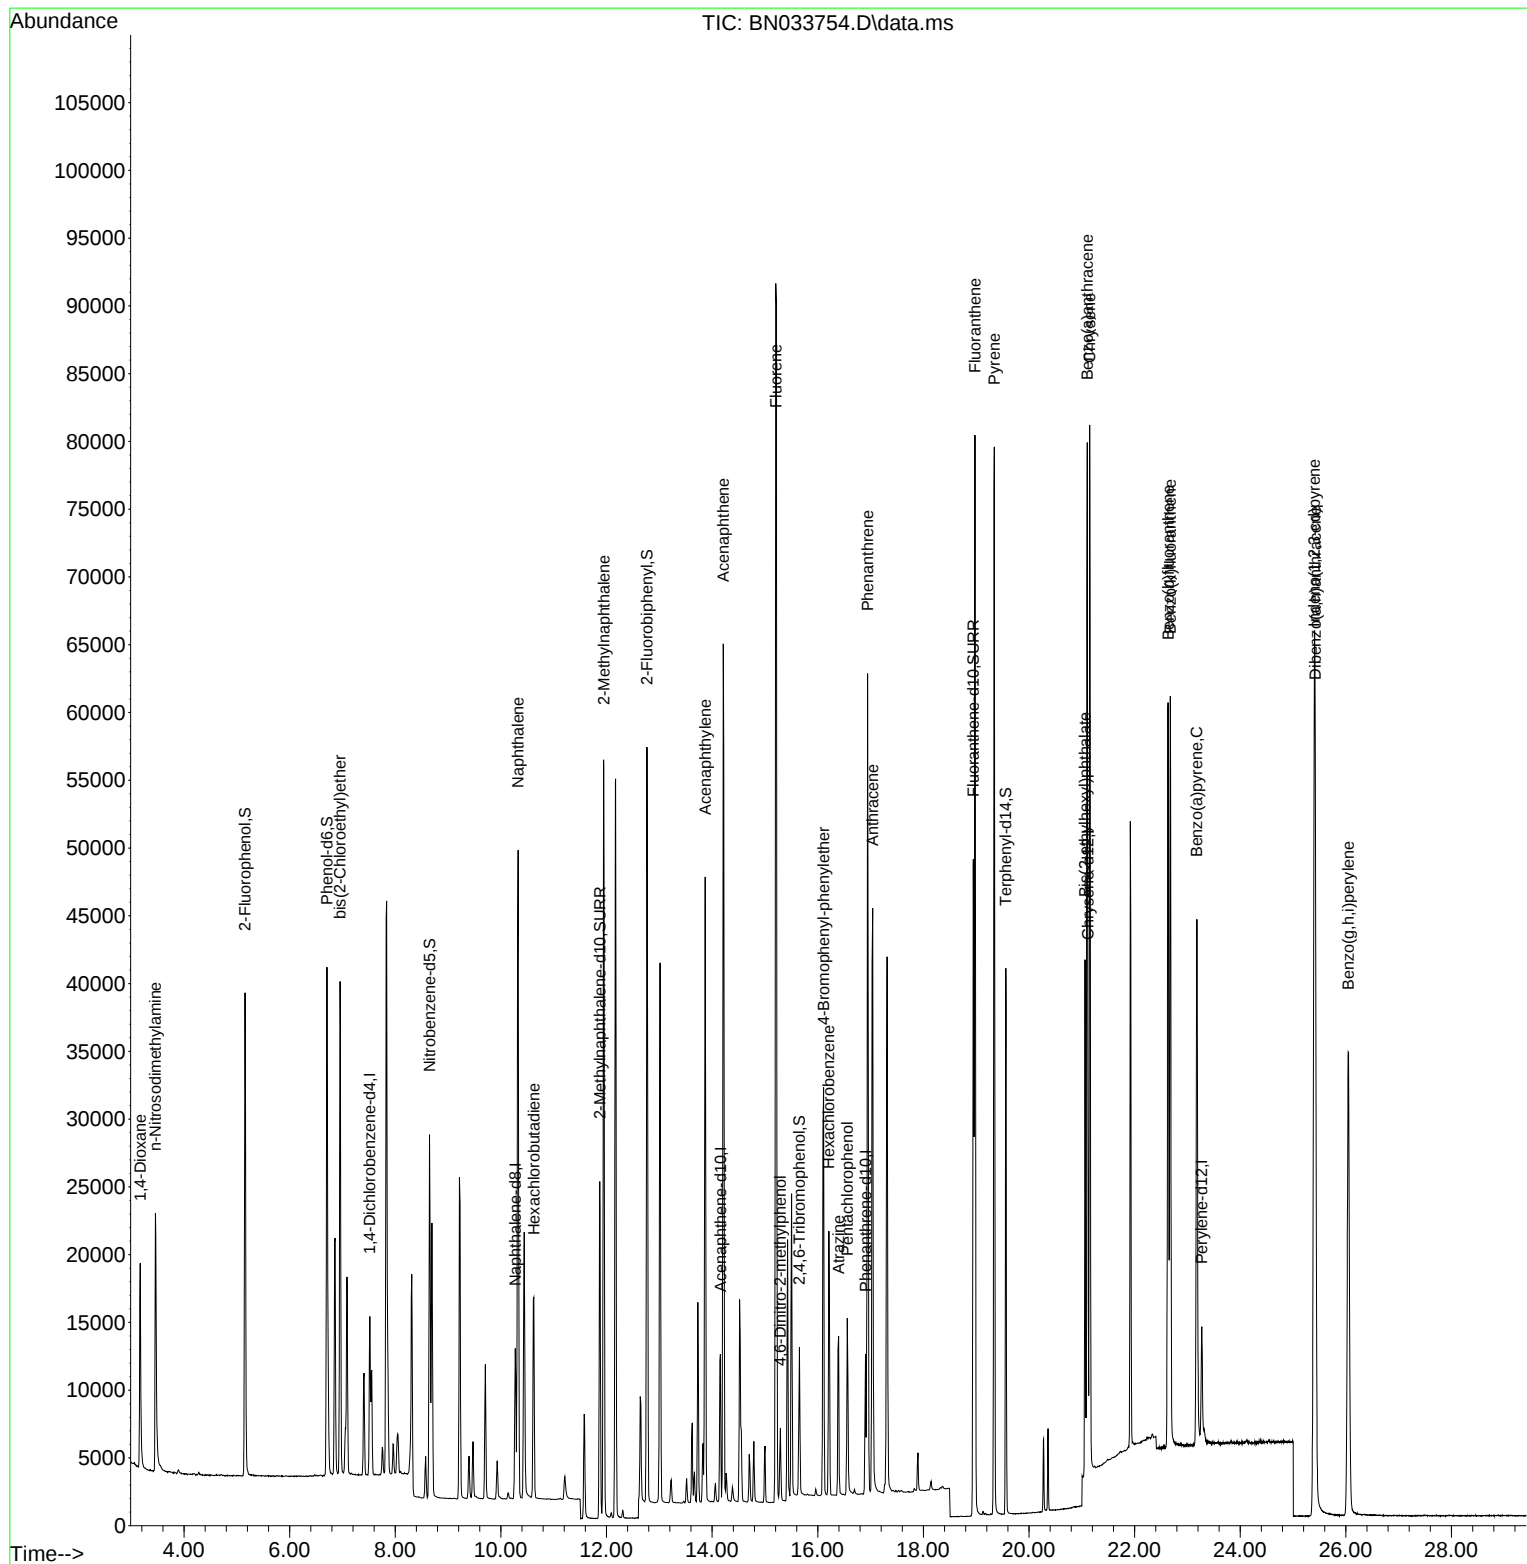




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.516 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN033754.D
 Acq: 04 Sep 2024 15:54




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:152 Resp: 5411
 Ion Ratio Lower Upper
 152 100
 150 154.4 123.3 184.9
 115 63.0 51.0 76.4

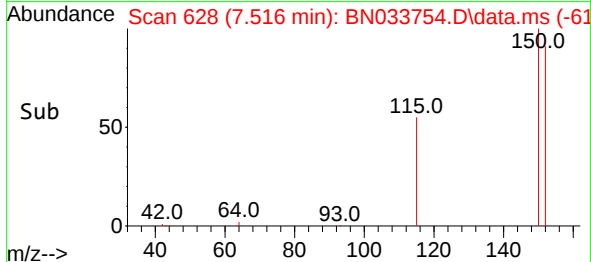

#2
 1,4-Dioxane
 Concen: 1.631 ng
 RT: 3.168 min Scan# 26
 Delta R.T. -0.000 min
 Lab File: BN033754.D
 Acq: 04 Sep 2024 15:54

Tgt Ion: 88 Resp: 10043
 Ion Ratio Lower Upper
 88 100
 43 33.6 29.0 43.4
 58 79.7 64.1 96.1




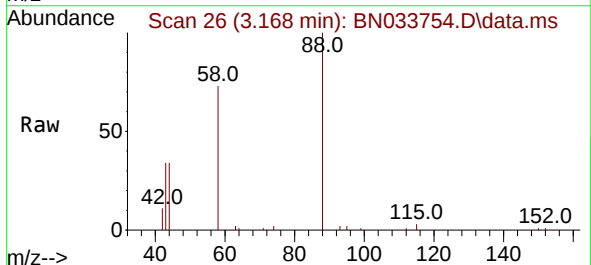


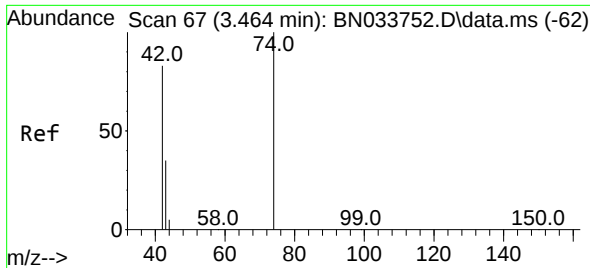

#3
n-Nitrosodimethylamine
Concen: 1.707 ng
RT: 3.457 min Scan# 60
Delta R.T. -0.007 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 42 Resp: 12340
Ion Ratio Lower Upper
42 100
74 114.3 93.5 140.3
44 6.5 7.4 11.0#

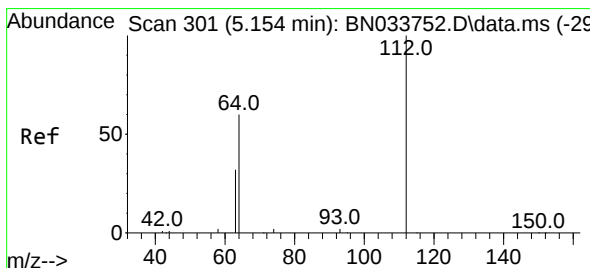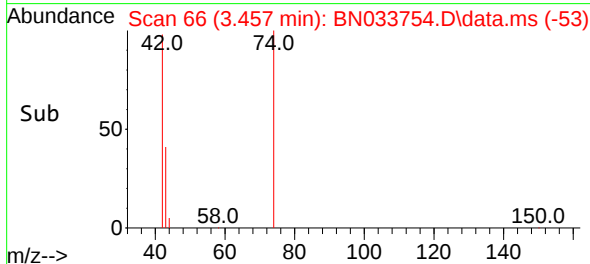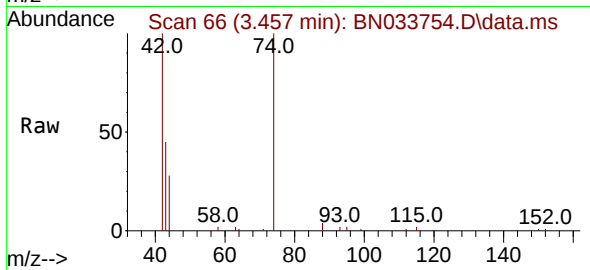

#4
2-Fluorophenol
Concen: 1.630 ng
RT: 5.154 min Scan# 301
Delta R.T. -0.000 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54

Tgt Ion: 112 Resp: 27004
Ion Ratio Lower Upper
112 100
64 60.0 47.6 71.4
63 32.4 25.9 38.9


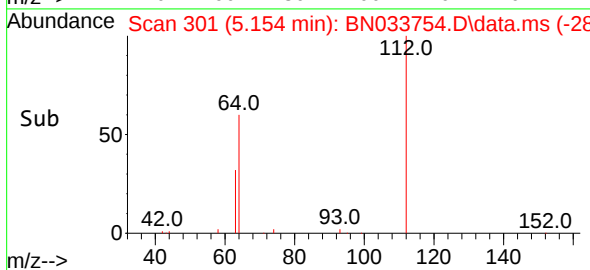

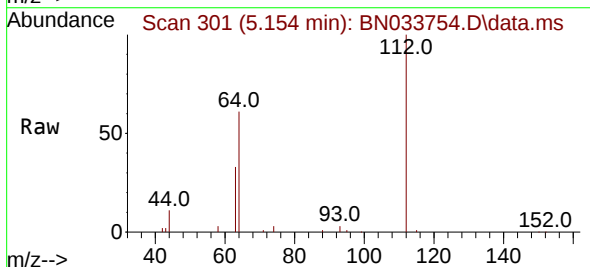




#5
Phenol-d6
Concen: 1.640 ng
RT: 6.707 min Scan# 516
Delta R.T. -0.000 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 99 Resp: 32166
Ion Ratio Lower Upper
99 100
42 21.9 18.0 27.0
71 35.8 28.7 43.1

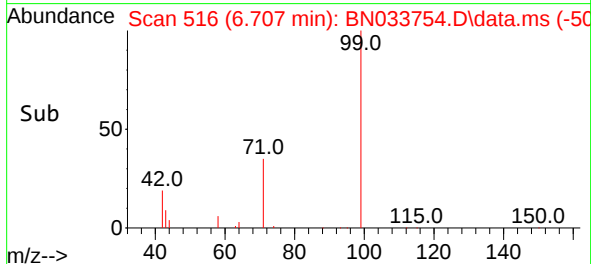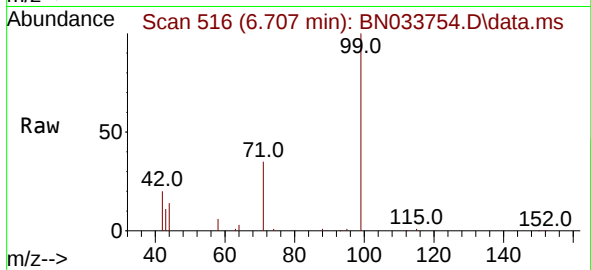

#6
bis(2-Chloroethyl)ether
Concen: 1.661 ng
RT: 6.953 min Scan# 550
Delta R.T. -0.007 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54

Tgt Ion: 93 Resp: 24581
Ion Ratio Lower Upper
93 100
63 80.0 64.4 96.6
95 32.7 26.5 39.7









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.272 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	136	Resp:	13930
Ion	Ratio	Lower	Upper
136	100		
137	11.5	9.0	13.4
54	9.7	8.1	12.1
68	6.9	5.8	8.8

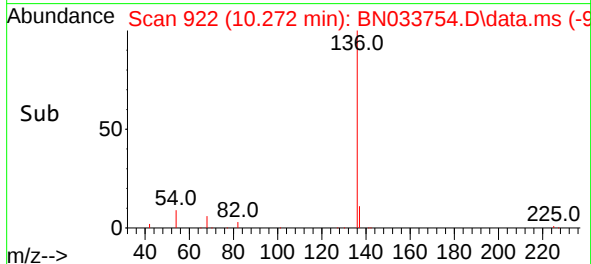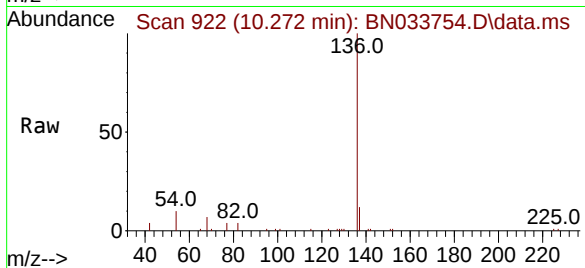

#8
Nitrobenzene-d5
Concen: 1.649 ng
RT: 8.649 min Scan# 770
Delta R.T. -0.000 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54

Tgt Ion:	82	Resp:	19563
Ion	Ratio	Lower	Upper
82	100		
128	38.1	31.3	46.9
54	56.8	46.9	70.3




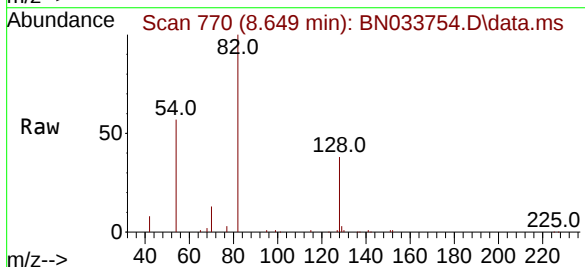


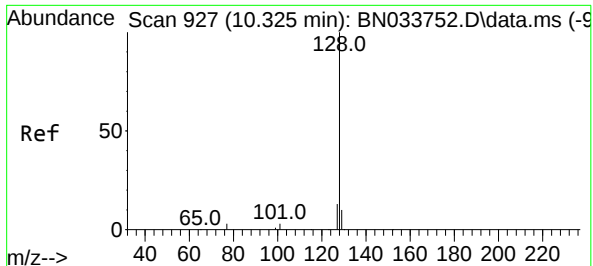

#9
Naphthalene
Concen: 1.659 ng
RT: 10.325 min Scan# 912
Delta R.T. -0.000 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Tgt Ion:128 Resp: 61713
Ion Ratio Lower Upper
128 100
129 11.0 8.9 13.3
127 13.1 10.8 16.2

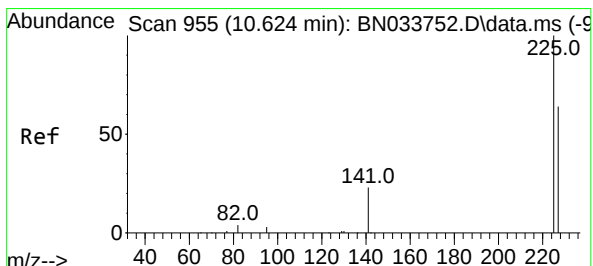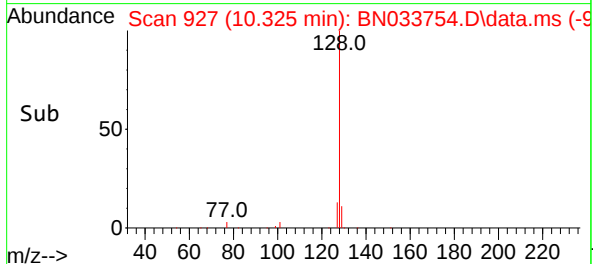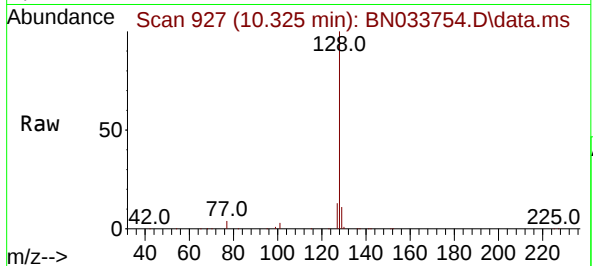

#10
Hexachlorobutadiene
Concen: 1.652 ng
RT: 10.624 min Scan# 955
Delta R.T. -0.000 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54

Tgt Ion:225 Resp: 12795
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.8 51.2 76.8

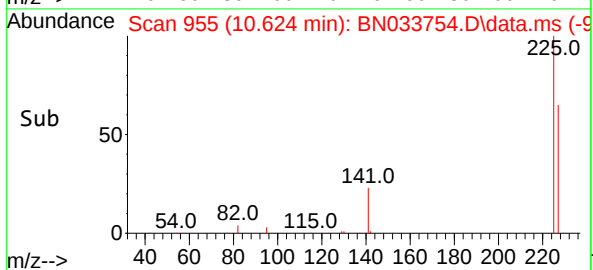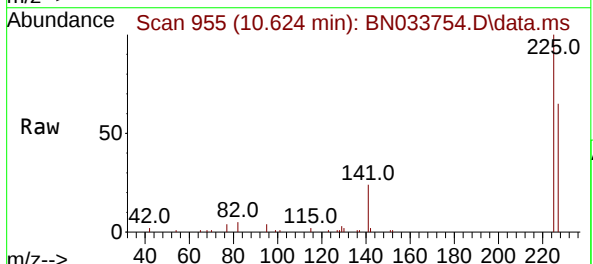



#11

2-Methylnaphthalene-d10

Concen: 1.671 ng

RT: 11.873 min Scan# 1134

Delta R.T. -0.000 min

Lab File: BN033754.D

Acq: 04 Sep 2024 15:54

Instrument :

BNA_N

ClientSampleId :





SSTDICC1.6

Tgt Ion:152 Resp: 32906

Ion Ratio Lower Upper

152 100

151 20.6 16.7 25.1

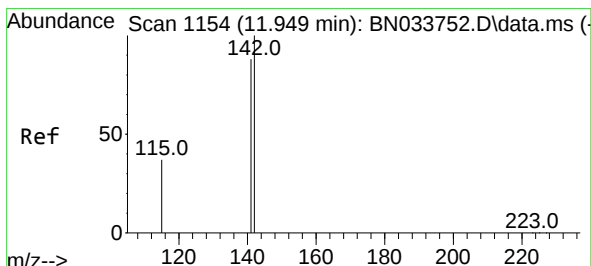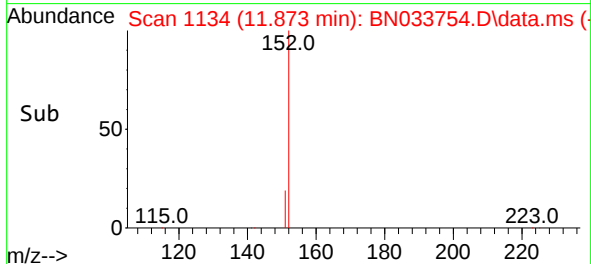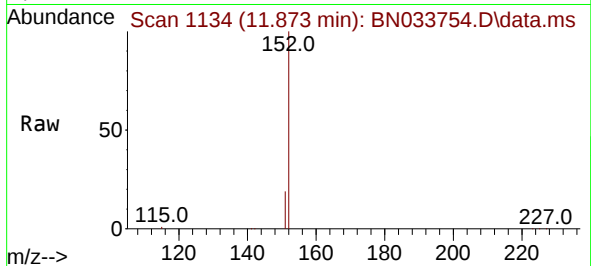

#12

2-Methylnaphthalene

Concen: 1.675 ng

RT: 11.949 min Scan# 1154

Delta R.T. -0.000 min

Lab File: BN033754.D

Acq: 04 Sep 2024 15:54




Tgt Ion:142 Resp: 38202


Ion Ratio Lower Upper

142 100

141 88.4 70.9 106.3

115 37.2 31.0 46.4



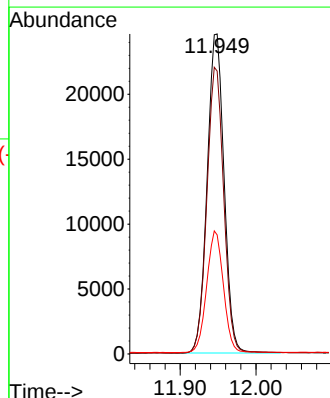
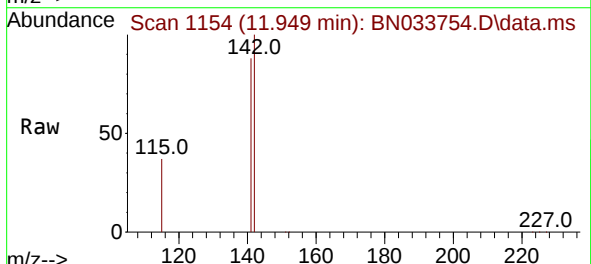




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.157 min Scan# 1473
Delta R.T. -0.000 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:164 Resp: 6595
Ion Ratio Lower Upper
164 100
162 102.3 82.0 123.0
160 48.7 39.1 58.7

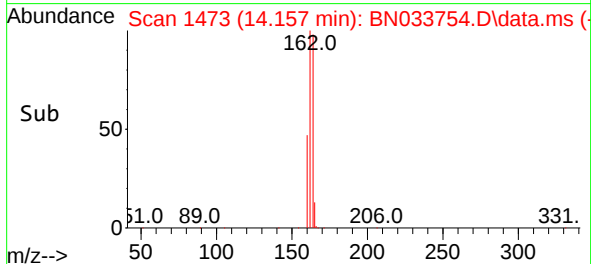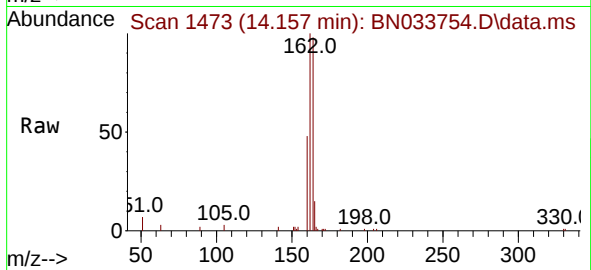

#14
2,4,6-Tribromophenol
Concen: 1.660 ng
RT: 15.651 min Scan# 1611
Delta R.T. -0.000 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54

Tgt Ion:330 Resp: 5530
Ion Ratio Lower Upper
330 100
332 97.6 74.2 111.4
141 43.6 33.9 50.9


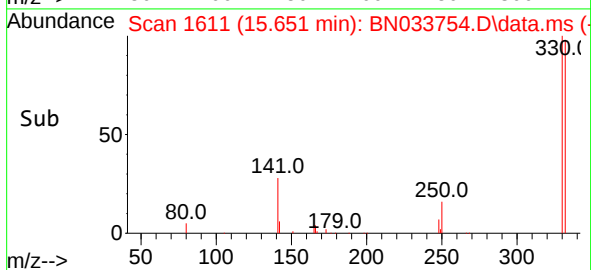




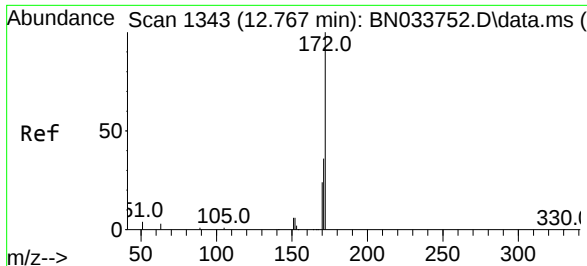

#15
2-Fluorobiphenyl
Concen: 1.653 ng
RT: 12.767 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:172 Resp: 45458
Ion Ratio Lower Upper
172 100
171 35.2 28.8 43.2
170 23.9 19.7 29.5

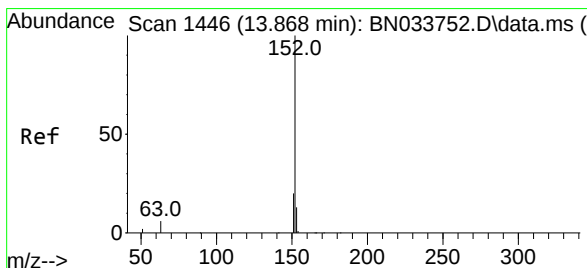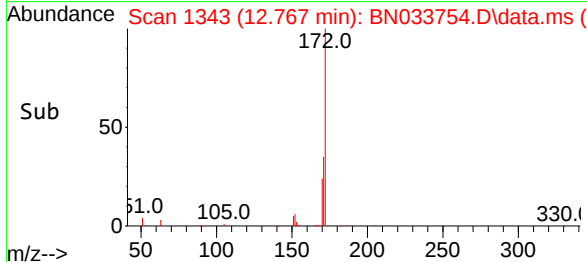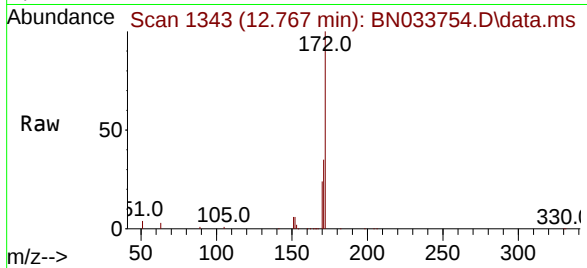

#16
Acenaphthylene
Concen: 1.689 ng
RT: 13.868 min Scan# 1446
Delta R.T. -0.000 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54

Tgt Ion:152 Resp: 48158
Ion Ratio Lower Upper
152 100
151 19.4 15.6 23.4
153 12.9 10.3 15.5

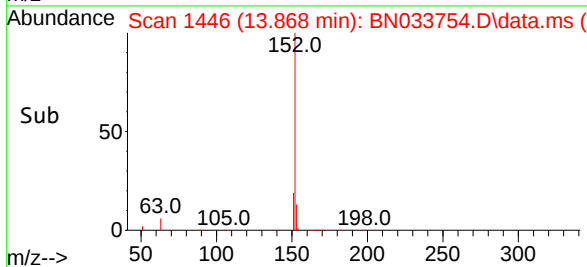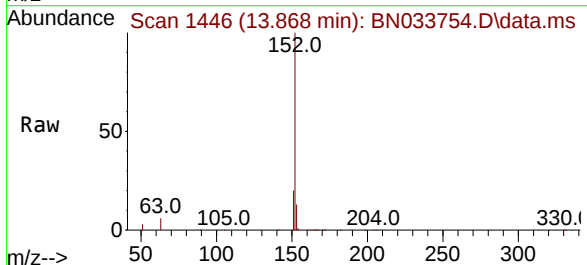

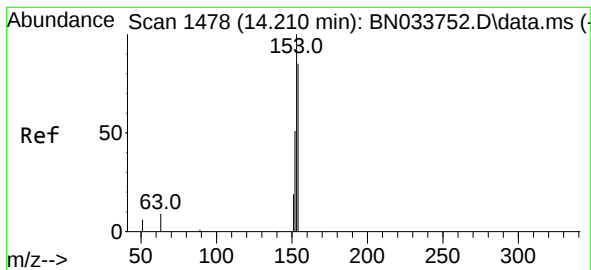

#17

Acenaphthene

Concen: 1.660 ng

RT: 14.210 min Scan# 1478

Delta R.T. -0.000 min

Lab File: BN033754.D

Acq: 04 Sep 2024 15:54

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:154 Resp: 32443

Ion Ratio Lower Upper

154 100

153 114.6 91.4 137.2

152 57.4 45.8 68.6

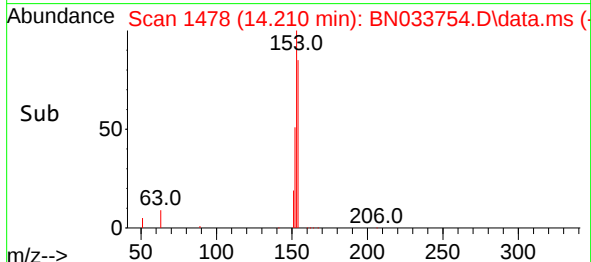

#18

Fluorene

Concen: 1.683 ng

RT: 15.204 min Scan# 1571

Delta R.T. -0.000 min

Lab File: BN033754.D

Acq: 04 Sep 2024 15:54




Tgt Ion:166 Resp: 40575


Ion Ratio Lower Upper

166 100

165 98.4 78.8 118.2

167 13.4 10.6 16.0

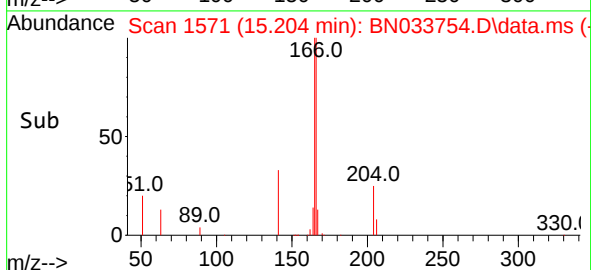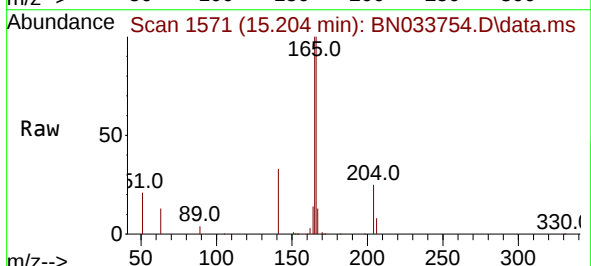

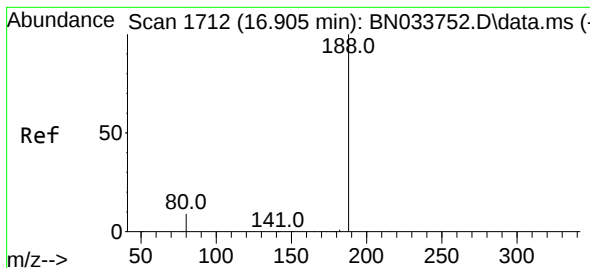

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.905 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN033754.D

Acq: 04 Sep 2024 15:54

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:188 Resp: 12815

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 10.1 7.9 11.9

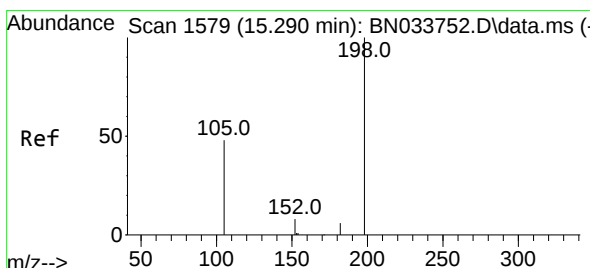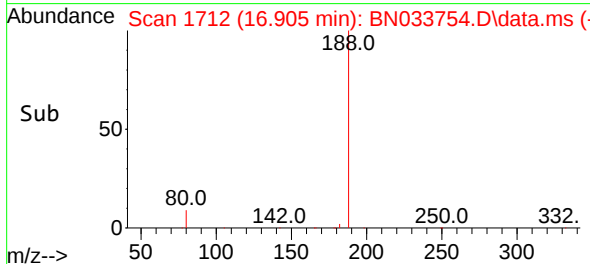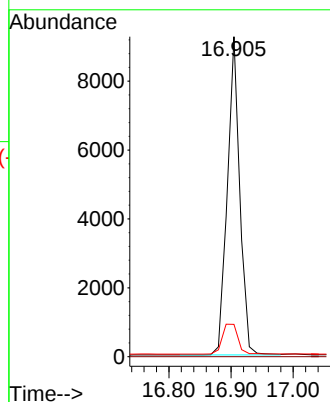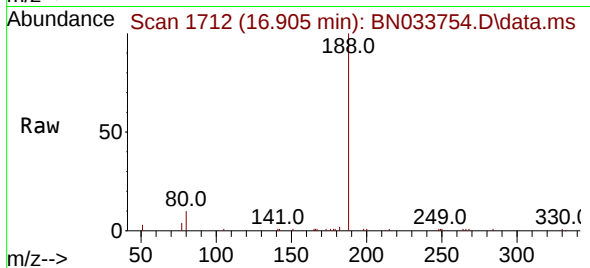

#20

4,6-Dinitro-2-methylphenol

Concen: 1.723 ng

RT: 15.290 min Scan# 1579

Delta R.T. -0.000 min

Lab File: BN033754.D

Acq: 04 Sep 2024 15:54




Tgt Ion:198 Resp: 3487


Ion Ratio Lower Upper

198 100

51 53.7 92.8 139.2#

105 48.7 59.4 89.0#


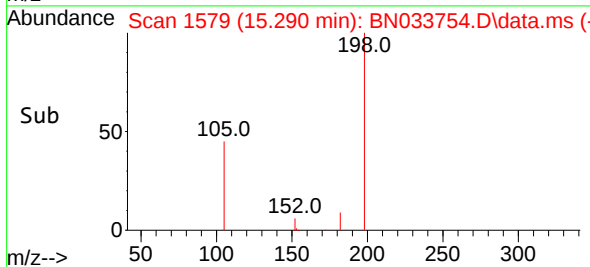
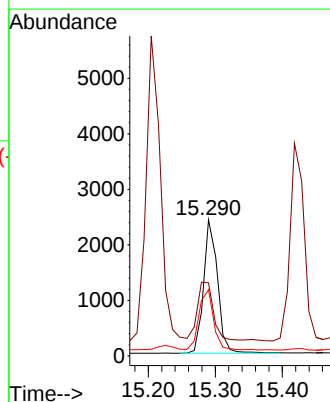
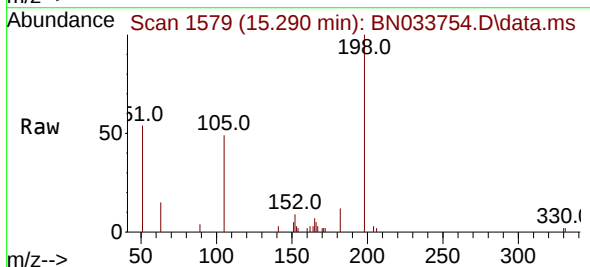


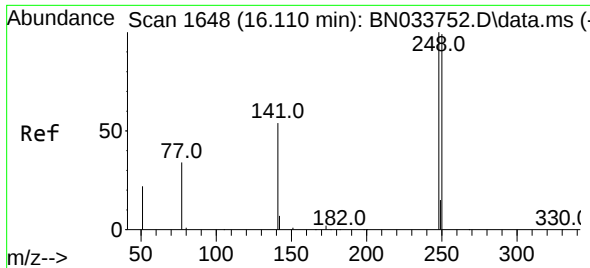

#21
4-Bromophenyl-phenylether
Concen: 1.677 ng
RT: 16.110 min Scan# 1648
Delta R.T. -0.000 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:248 Resp: 12450
Ion Ratio Lower Upper
248 100
250 98.6 79.5 119.3
141 49.6 44.9 67.3

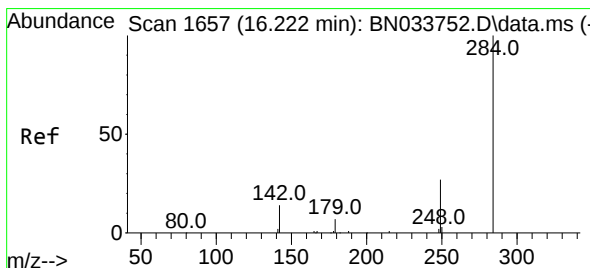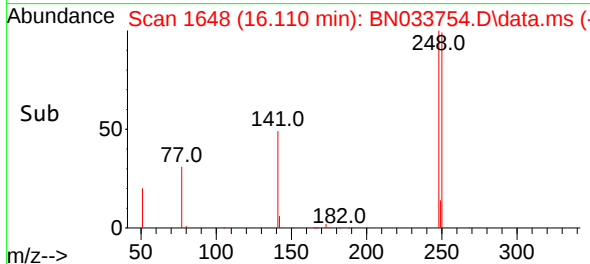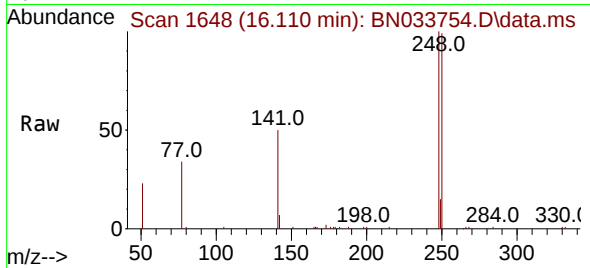

#22
Hexachlorobenzene
Concen: 1.646 ng
RT: 16.209 min Scan# 1656
Delta R.T. -0.012 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54

Tgt Ion:284 Resp: 14017
Ion Ratio Lower Upper
284 100
142 42.8 32.8 49.2
249 32.6 26.2 39.2


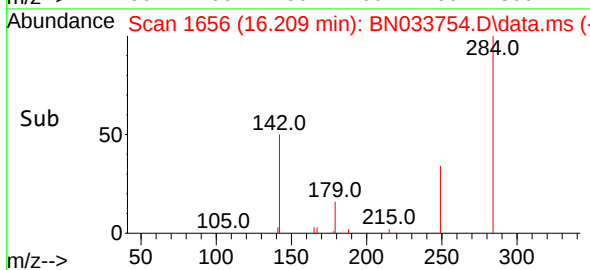

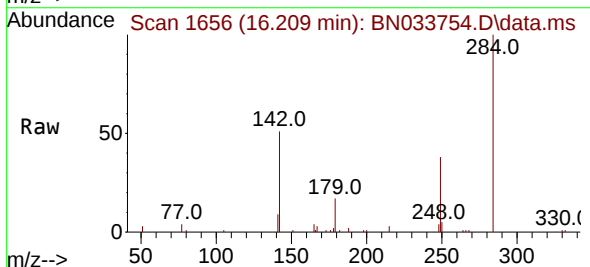


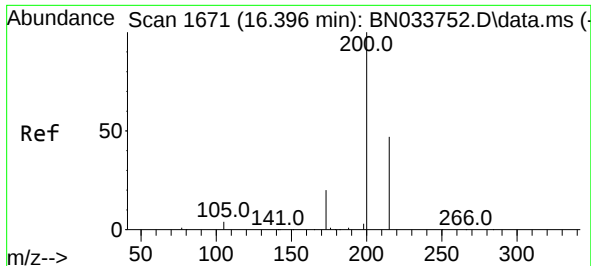

#23
Atrazine
Concen: 1.713 ng
RT: 16.396 min Scan# 1671
Delta R.T. -0.000 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:200 Resp: 10154
Ion Ratio Lower Upper
200 100
173 20.3 18.2 27.4
215 46.8 39.0 58.4

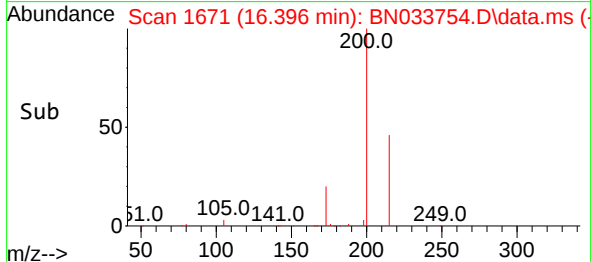

#24
Pentachlorophenol
Concen: 1.715 ng
RT: 16.557 min Scan# 1684
Delta R.T. -0.012 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54

Tgt Ion:266 Resp: 5969
Ion Ratio Lower Upper
266 100
264 62.4 49.6 74.4
268 64.8 52.2 78.4

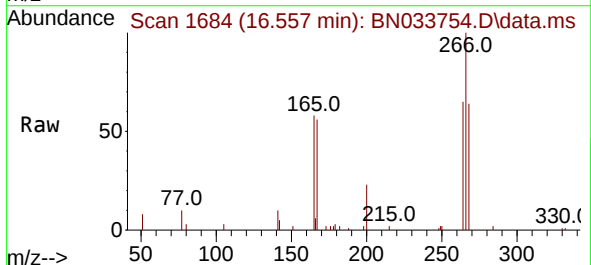

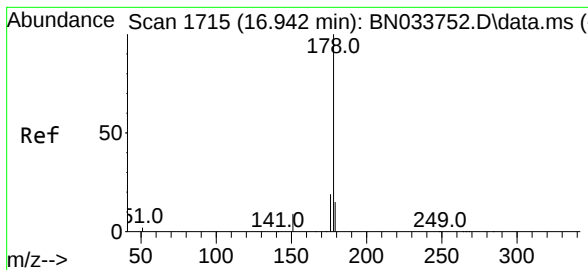

#25

Phenanthrene

Concen: 1.681 ng

RT: 16.942 min Scan# 1715

Delta R.T. -0.000 min

Lab File: BN033754.D

Acq: 04 Sep 2024 15:54

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:178 Resp: 59360

Ion Ratio Lower Upper

178 100

176 19.3 15.4 23.0

179 15.2 12.2 18.4

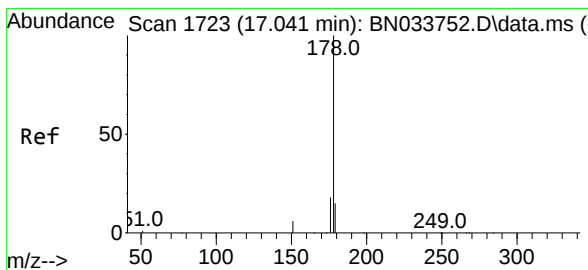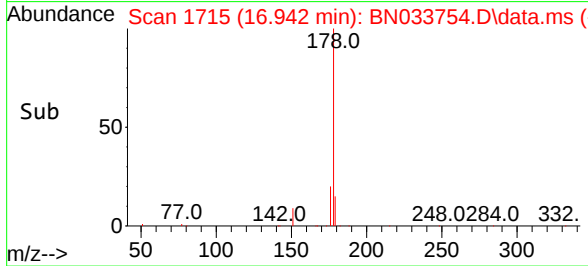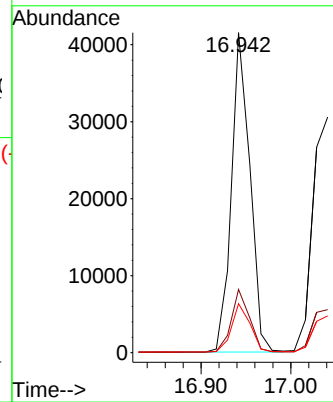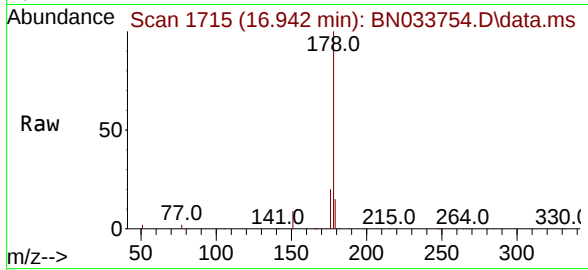

#26

Anthracene

Concen: 1.690 ng

RT: 17.041 min Scan# 1723

Delta R.T. -0.000 min

Lab File: BN033754.D

Acq: 04 Sep 2024 15:54




Tgt Ion:178 Resp: 51869


Ion Ratio Lower Upper

178 100

176 18.7 14.8 22.2

179 15.1 12.4 18.6


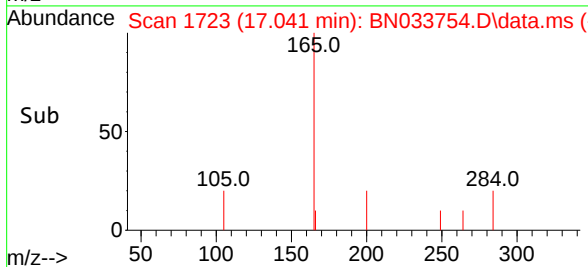
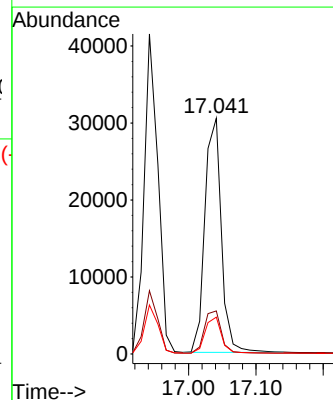
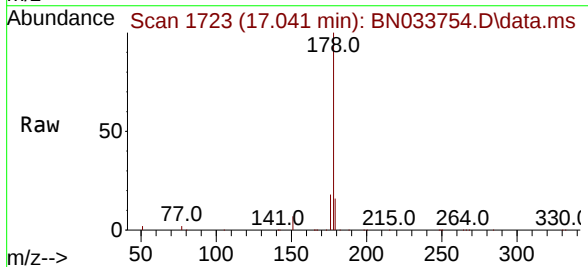


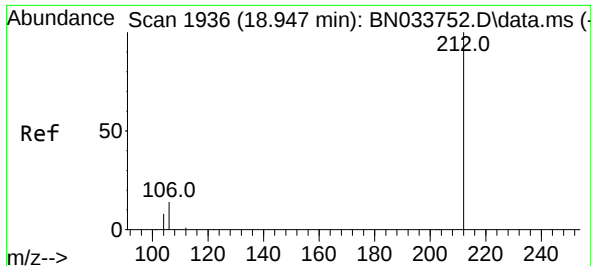

#27
Fluoranthene-d10
Concen: 1.704 ng
RT: 18.947 min Scan# 1936
Delta R.T. -0.000 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:212 Resp: 53870
Ion Ratio Lower Upper
212 100
106 14.3 11.5 17.3
104 8.3 6.6 9.8

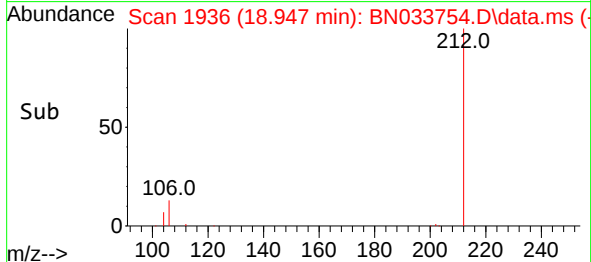

#28
Fluoranthene
Concen: 1.731 ng
RT: 18.975 min Scan# 1942
Delta R.T. -0.000 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54

Tgt Ion:202 Resp: 68510
Ion Ratio Lower Upper
202 100
101 11.2 9.2 13.8
203 17.1 13.8 20.6




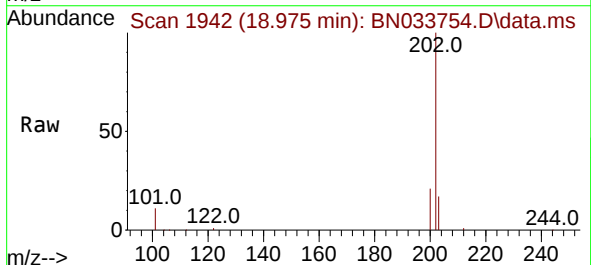




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.113 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:240 Resp: 10603
Ion Ratio Lower Upper
240 100
120 17.8 13.7 20.5
236 29.6 23.4 35.2

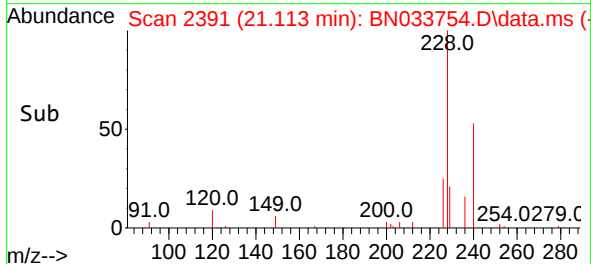

#30
Pyrene
Concen: 1.614 ng
RT: 19.342 min Scan# 2021
Delta R.T. -0.000 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54

Tgt Ion:202 Resp: 68965
Ion Ratio Lower Upper
202 100
200 20.9 16.8 25.2
203 17.7 14.4 21.6


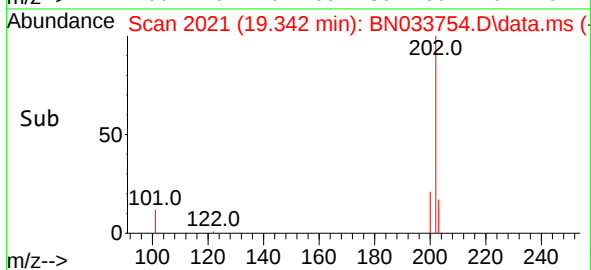




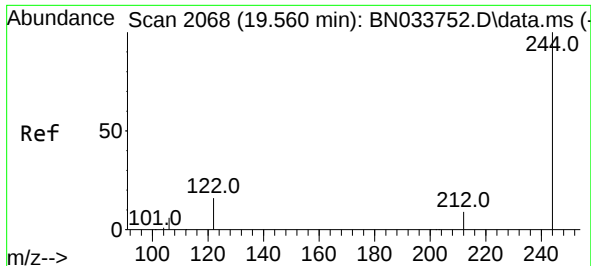

#31
Terphenyl-d14
Concen: 1.616 ng
RT: 19.560 min Scan# 2068
Delta R.T. -0.000 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:244 Resp: 36539
Ion Ratio Lower Upper
244 100
212 9.5 7.9 11.9
122 16.5 13.2 19.8

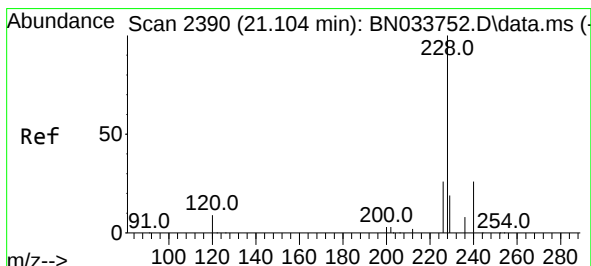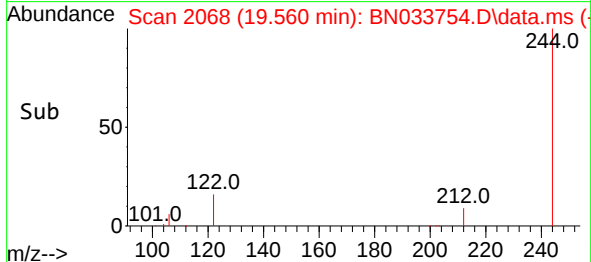

#32
Benzo(a)anthracene
Concen: 1.661 ng
RT: 21.104 min Scan# 2390
Delta R.T. -0.000 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54

Tgt Ion:228 Resp: 62876
Ion Ratio Lower Upper
228 100
226 26.7 21.2 31.8
229 19.9 15.9 23.9







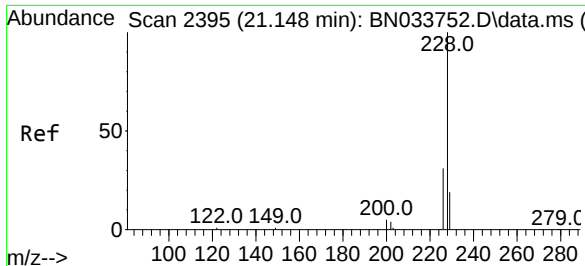

#33
Chrysene
Concen: 1.652 ng
RT: 21.148 min Scan# 2114
Delta R.T. -0.000 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:228 Resp: 61836
Ion Ratio Lower Upper
228 100
226 30.8 25.0 37.6
229 19.0 15.6 23.4

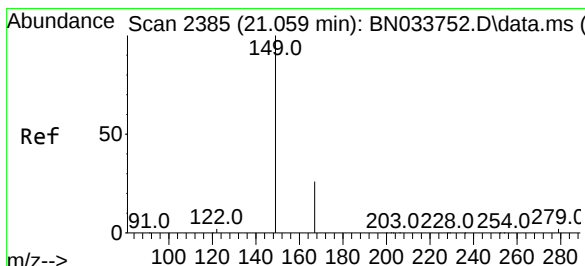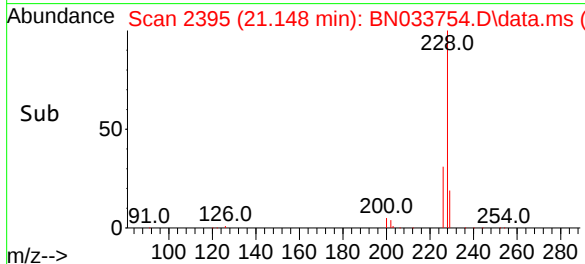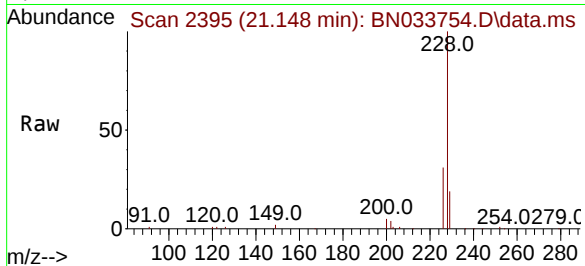

#34
Bis(2-ethylhexyl)phthalate
Concen: 1.574 ng
RT: 21.059 min Scan# 2385
Delta R.T. -0.000 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54

Tgt Ion:149 Resp: 32496
Ion Ratio Lower Upper
149 100
167 26.7 21.0 31.4
279 2.9 2.4 3.6

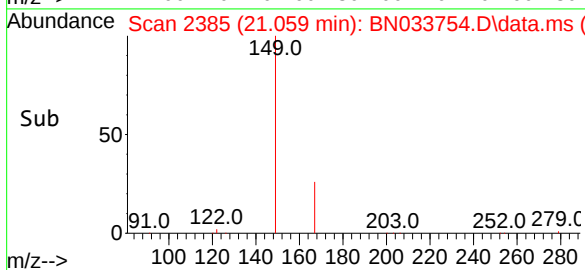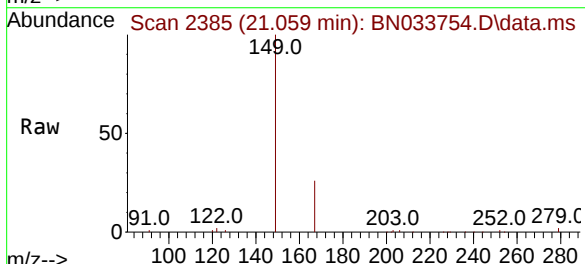



#35

Perylene-d12

Concen: 0.400 ng

RT: 23.271 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN033754.D


Acq: 04 Sep 2024 15:54

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6

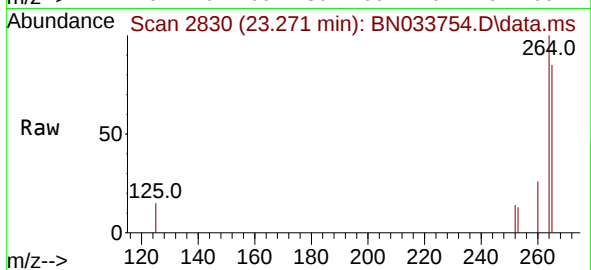




Tgt Ion:264 Resp: 10665

Ion Ratio Lower Upper

264 100

260 26.1 21.1 31.7

265 85.0 72.0 108.0

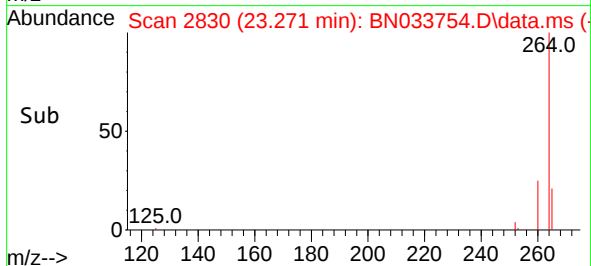

#36

Indeno(1,2,3-cd)pyrene

Concen: 1.691 ng

RT: 25.402 min Scan# 3559

Delta R.T. -0.000 min

Lab File: BN033754.D

Acq: 04 Sep 2024 15:54




Tgt Ion:276 Resp: 74558

Ion Ratio Lower Upper

276 100

138 28.7 23.0 34.6

277 24.8 20.2 30.4


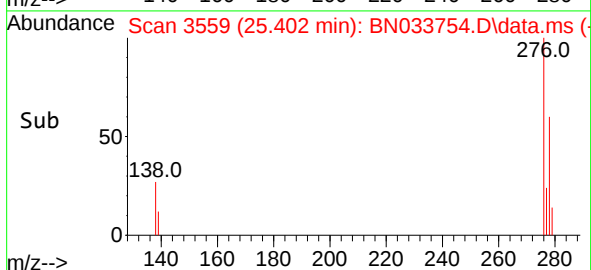

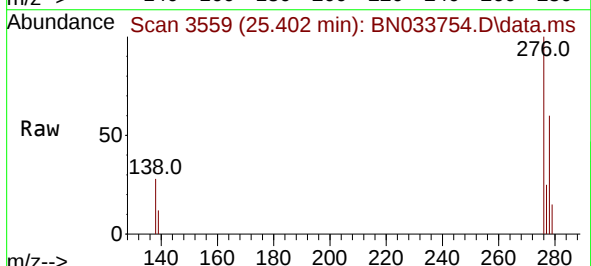




#37
Benzo(b)fluoranthene
Concen: 1.685 ng
RT: 22.633 min Scan# 2611
Delta R.T. 0.003 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Tgt Ion:252 Resp: 66033
Ion Ratio Lower Upper
252 100
253 22.7 21.8 32.6
125 12.8 15.4 23.0#

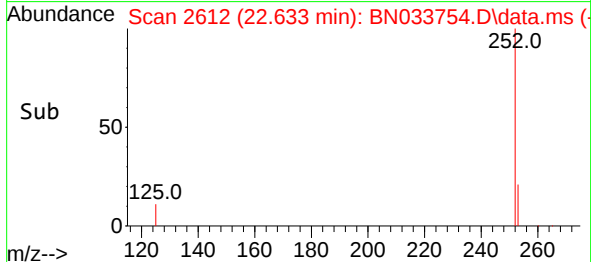

#38
Benzo(k)fluoranthene
Concen: 1.690 ng
RT: 22.674 min Scan# 2626
Delta R.T. -0.000 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54


Tgt Ion:252 Resp: 64560
Ion Ratio Lower Upper
252 100
253 22.7 21.8 32.8
125 12.8 15.4 23.2#

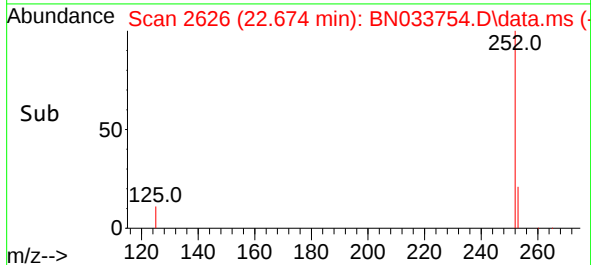





#39
Benzo(a)pyrene
Concen: 1.677 ng
RT: 23.177 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6






Tgt Ion:252 Resp: 54955
Ion Ratio Lower Upper
252 100
253 23.3 24.0 36.0#
125 14.5 19.1 28.7#



#40
Dibenzo(a,h)anthracene
Concen: 1.699 ng
RT: 25.420 min Scan# 3565
Delta R.T. 0.003 min
Lab File: BN033754.D
Acq: 04 Sep 2024 15:54

Tgt Ion:278 Resp: 60034
Ion Ratio Lower Upper
278 100
139 18.7 16.7 25.1
279 24.1 23.4 35.0

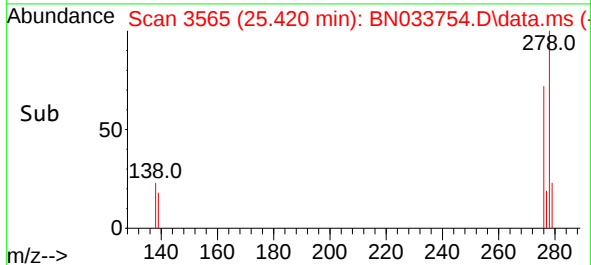



#41
 Benzo(g,h,i)perylene
 Concen: 1.684 ng
 RT: 26.045 min Scan# 31
 Delta R.T. -0.003 min
 Lab File: BN033754.D
 Acq: 04 Sep 2024 15:54

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Tgt Ion:	276	Resp:	64526
Ion Ratio	Lower	Upper	
276	100		
277	24.1	20.3	30.5
138	24.8	20.9	31.3

