

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090424\
 Data File : BN033758.D
 Acq On : 04 Sep 2024 19:32
 Operator : MA/JU
 Sample : PB163098BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB163098BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN090424.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BN033758.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.825	114	117	124	rVB	3310	4758	1.65%	1.025%
2	4.396	193	196	199	rBV	2801	3328	1.16%	0.717%
3	4.707	235	239	256	rVB	218454	287971	100.00%	62.043%
4	5.162	298	302	309	rVB	6759	10331	3.59%	2.226%
5	6.707	512	516	525	rVB	6336	10110	3.51%	2.178%
6	7.516	624	628	634	rVB	10629	15905	5.52%	3.427%
7	8.649	767	770	782	rVB	5047	9056	3.14%	1.951%
8	10.272	918	922	930	rBV	9324	16696	5.80%	3.597%
9	11.873	1123	1134	1152	rBV2	4791	8386	2.91%	1.807%
10	12.767	1340	1343	1354	rBV	10285	17649	6.13%	3.802%
11	14.157	1469	1473	1484	rBV	9513	15715	5.46%	3.386%
12	16.904	1709	1712	1721	rBV	8253	12818	4.45%	2.762%
13	18.947	1928	1936	1952	rBV2	10044	14103	4.90%	3.038%
14	19.560	2061	2068	2079	rBV	8307	10394	3.61%	2.239%
15	21.023	2377	2381	2382	rBV3	1956	3347	1.16%	0.721%
16	21.112	2388	2391	2395	rBV	9086	12331	4.28%	2.657%
17	23.271	2823	2830	2851	rVB	6349	11252	3.91%	2.424%




Sum of corrected areas: 464150

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090424\
Data File : BN033758.D
Acq On : 04 Sep 2024 19:32
Operator : MA/JU
Sample : PB163098BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB163098BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

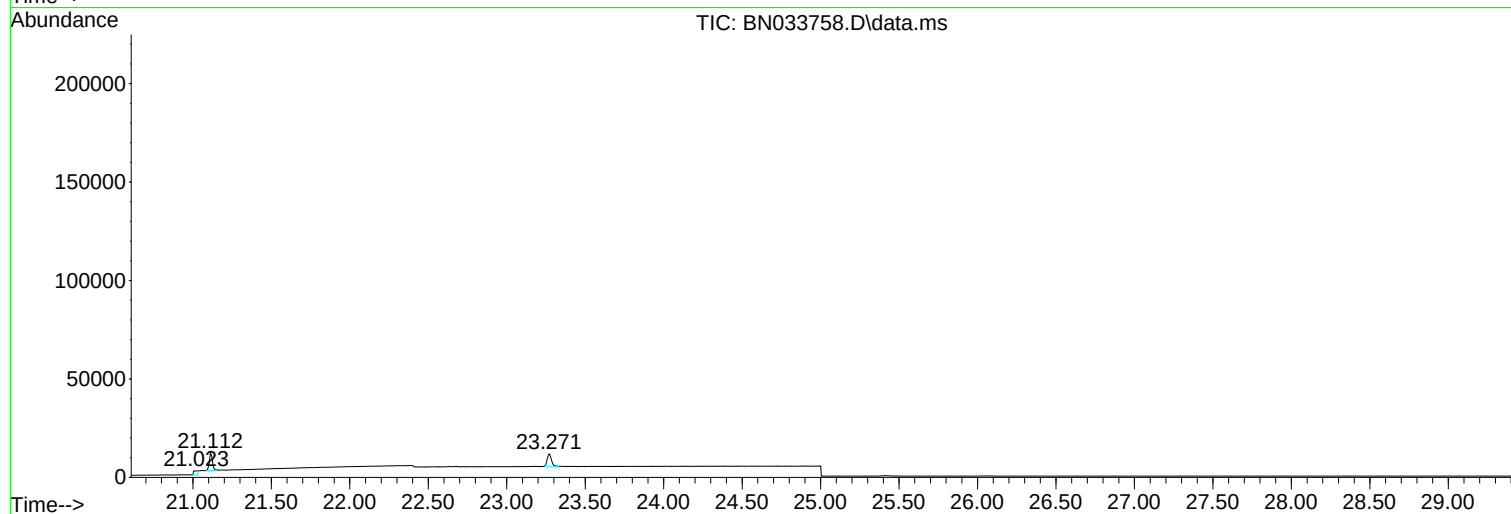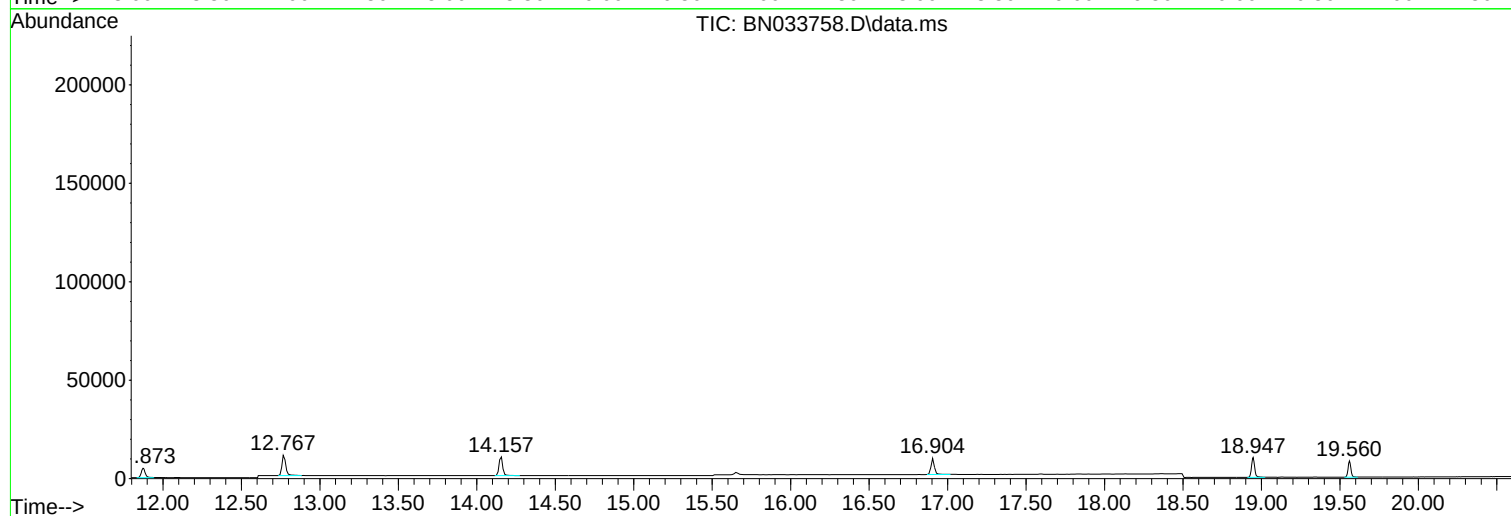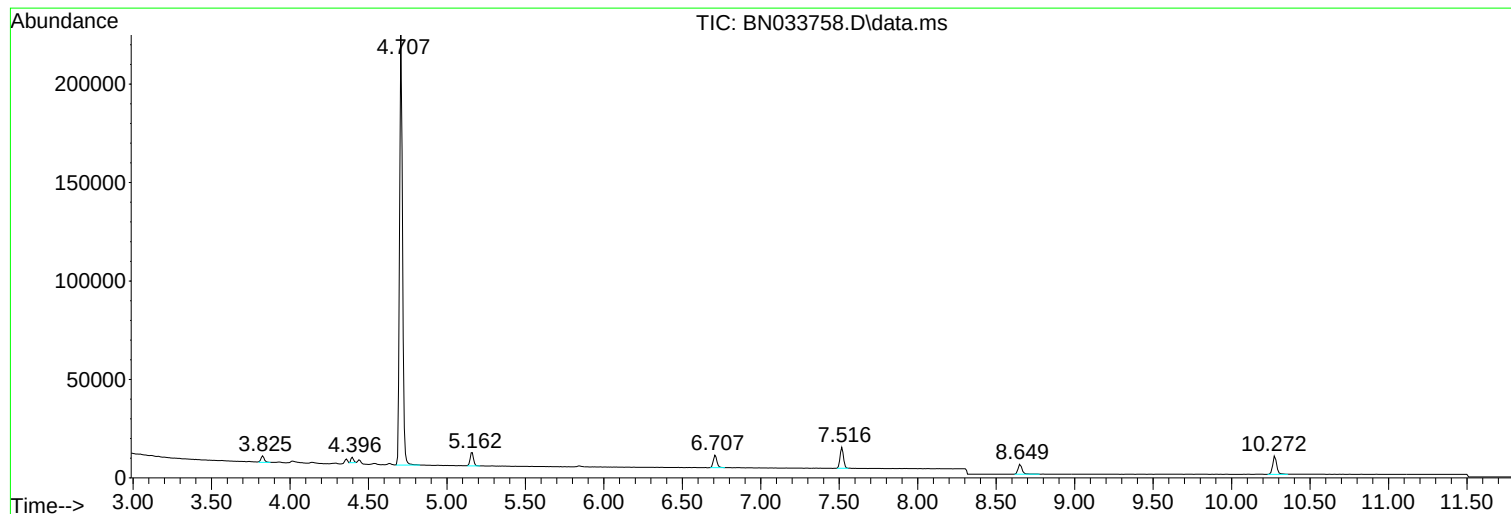

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090424\
Data File : BN033758.D
Acq On : 04 Sep 2024 19:32
Operator : MA/JU
Sample : PB163098BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB163098BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090424\
Data File : BN033758.D
Acq On : 04 Sep 2024 19:32
Operator : MA/JU
Sample : PB163098BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB163098BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------