
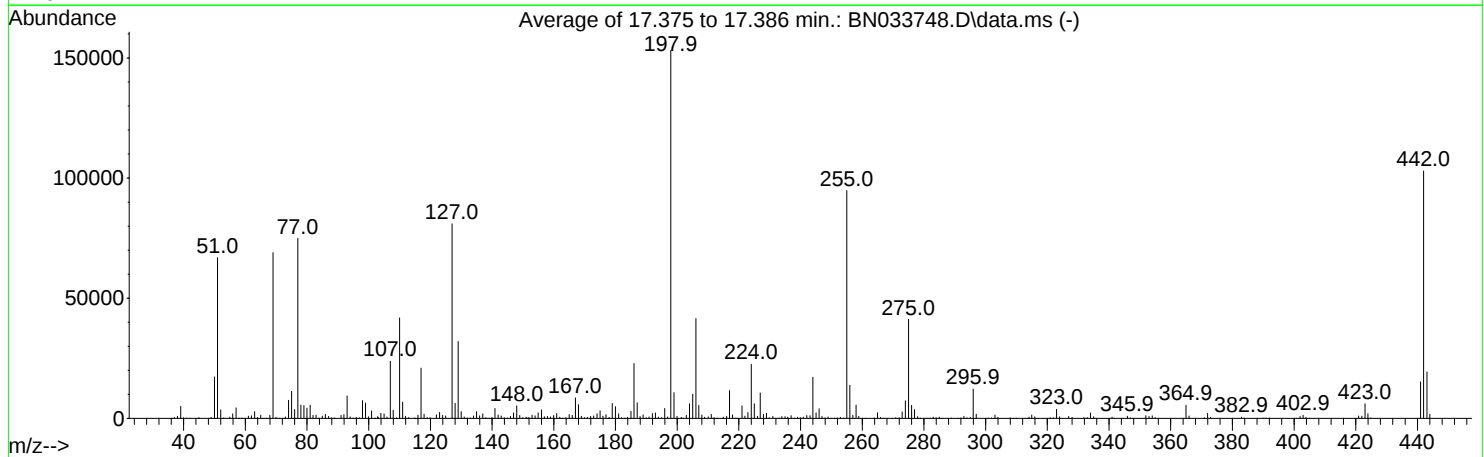


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090424\
Data File : BN033748.D
Acq On : 04 Sep 2024 10:22
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN090424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 04 18:36:01 2024

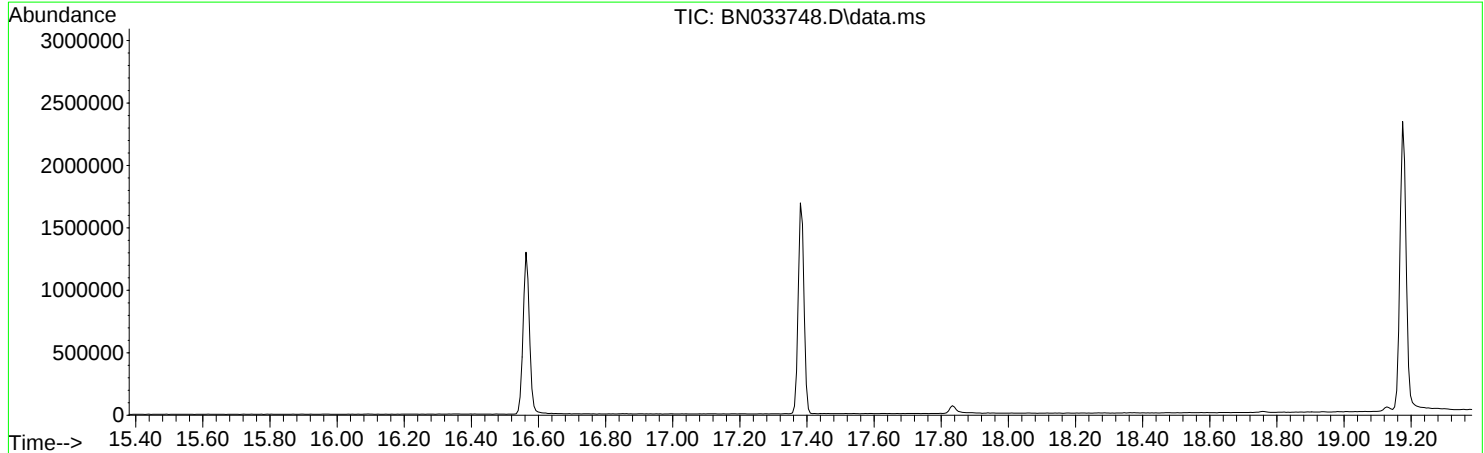




AutoFind: Scans 2446, 2447, 2448; Background Corrected with Scan 2440

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.7	66902	PASS
68	69	0.00	2	1.9	1282	PASS
69	198	0.00	100	45.1	68992	PASS
70	69	0.00	2	0.7	488	PASS
127	198	10	80	52.9	81005	PASS
197	198	0.00	2	0.4	587	PASS
198	198	100	100	100.0	153107	PASS
199	198	5	9	7.0	10758	PASS
275	198	10	60	26.9	41195	PASS
365	198	1	100	3.6	5437	PASS
441	198	0.01	100	9.9	15192	PASS
442	442	50	100	100.0	102960	PASS
443	442	15	24	18.7	19300	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090424\
Data File : BN033748.D
Acq On : 04 Sep 2024 10:22
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 05 18:53:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 04:54:27 2024
Response via : Initial Calibration

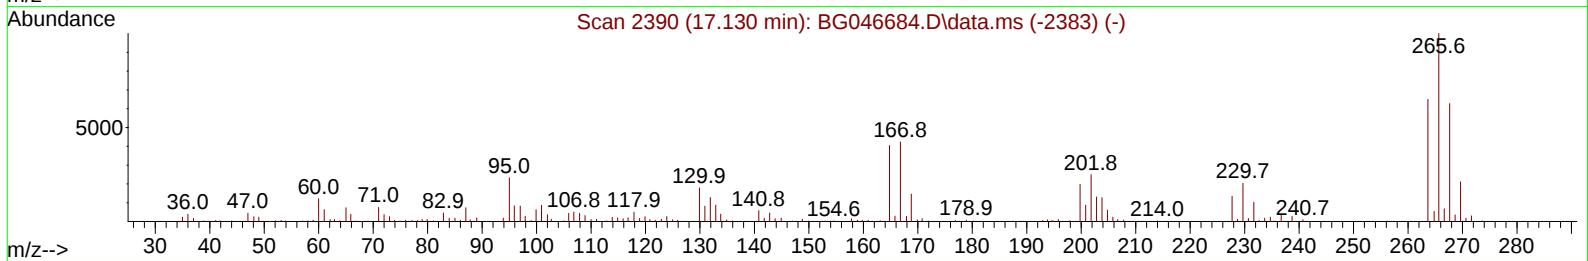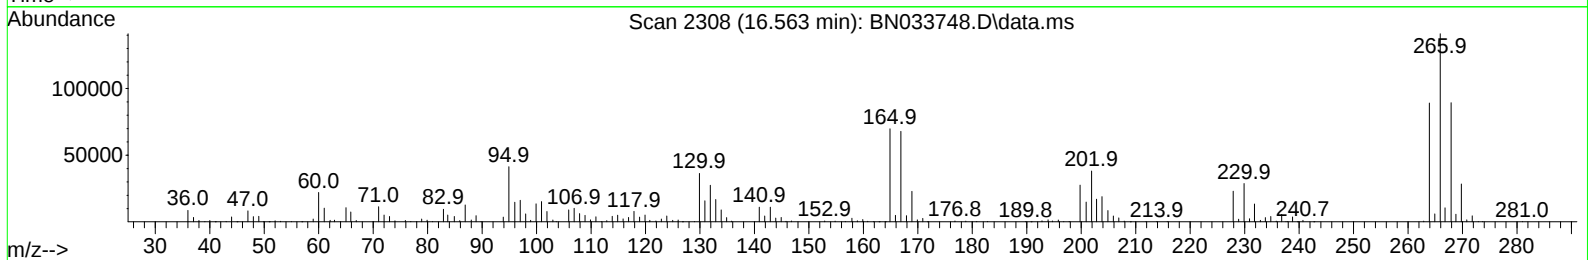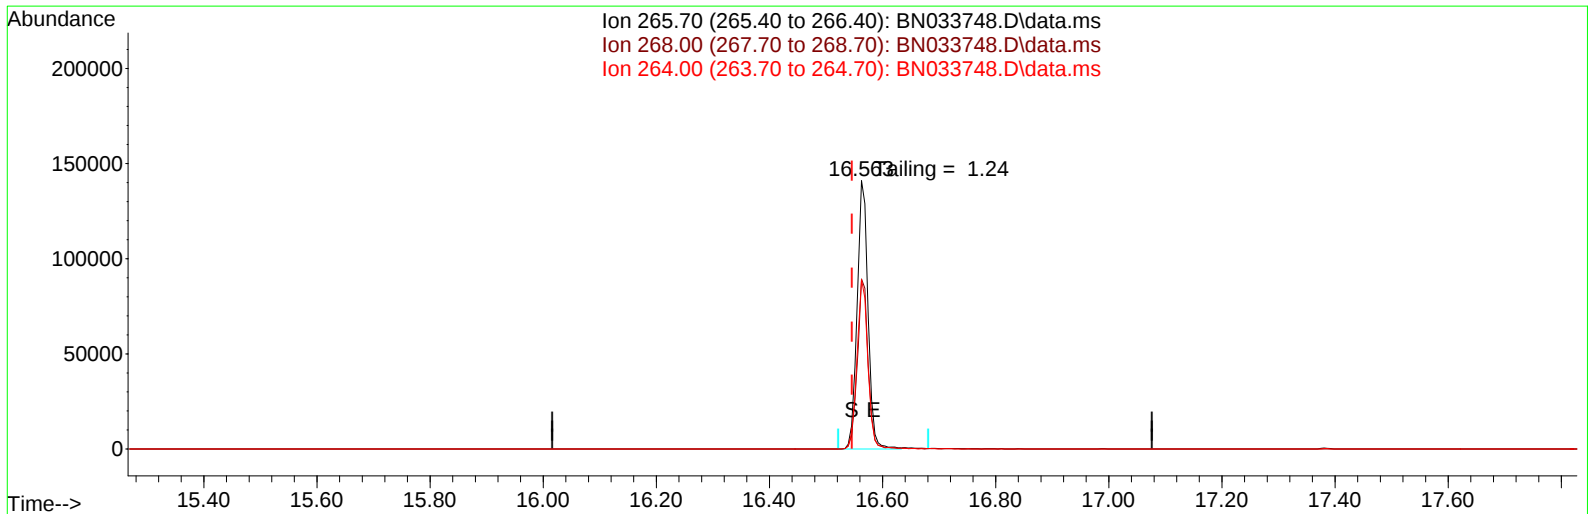

TIC: BN033748.D\data.ms

(70) Pentachlorophenol (C)

16.563min (+ 0.017) 22675.23 ng




response 190228

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.37
264.00	61.60	63.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090424\
Data File : BN033748.D
Acq On : 04 Sep 2024 10:22
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 05 18:53:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 04:54:27 2024
Response via : Initial Calibration

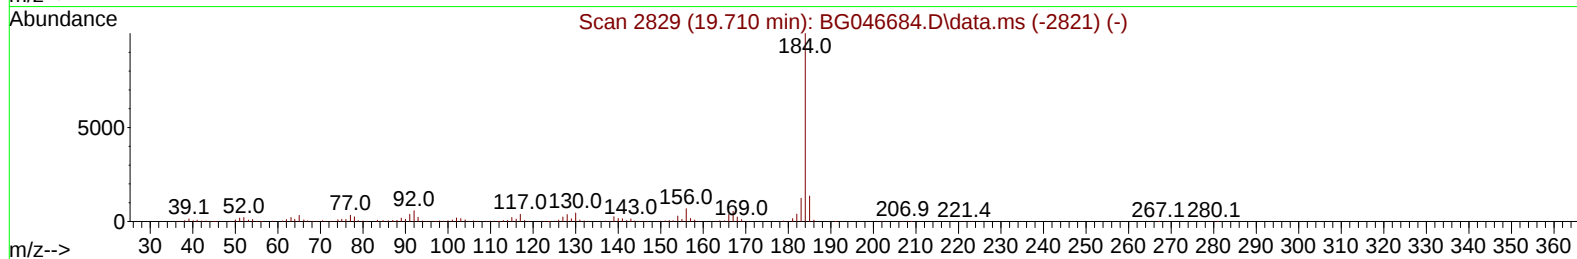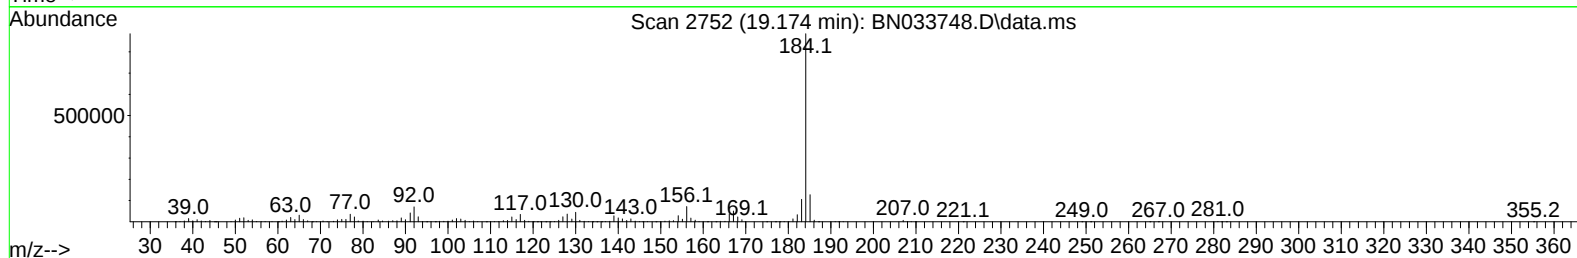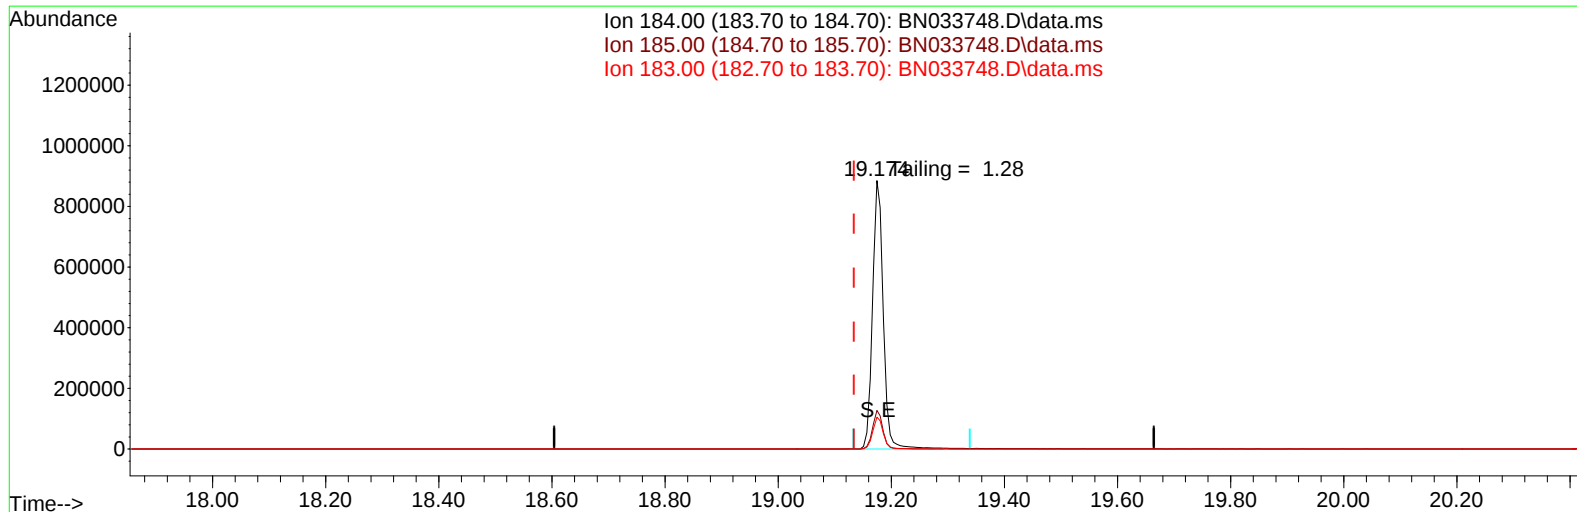

TIC: BN033748.D\data.ms

(77) Benzidine

19.174min (+ 0.040) 0.00 ng

response 1173747

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.39
183.00	13.20	11.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/4/2024	BNA_N	<u>BN033748.D</u>
Compound Name	Response	Retention Time
DDT	639689	20.427
DDD	18678	19.98
DDE	1144	19.474
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19822	659511	3.01

Instrument :
BNA_N
ClientSampleId :
DFTPP