
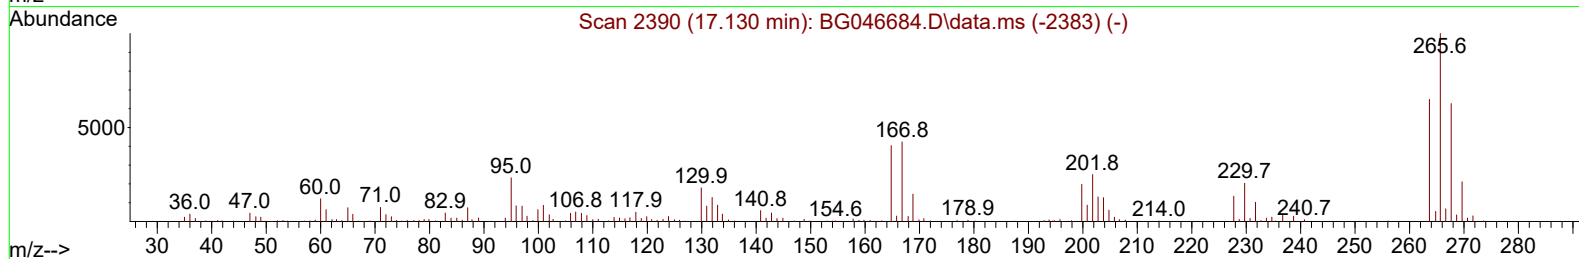
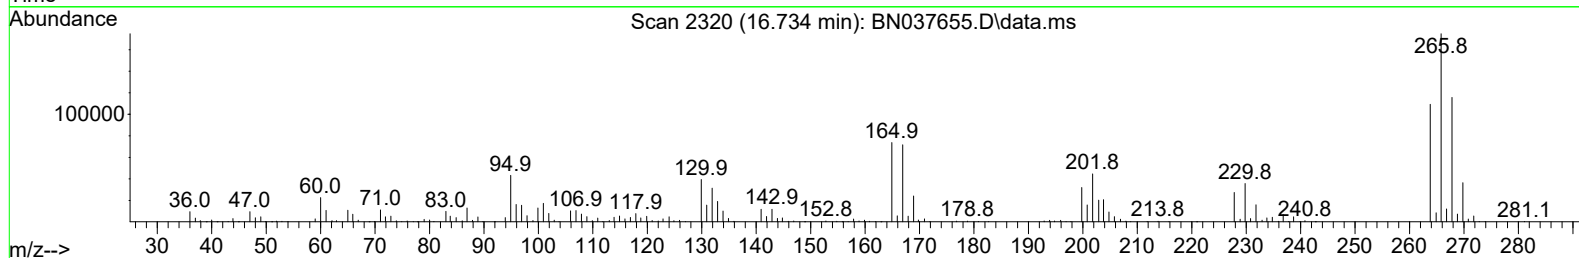


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090425\
Data File : BN037655.D
Acq On : 04 Sep 2025 10:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 07:32:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

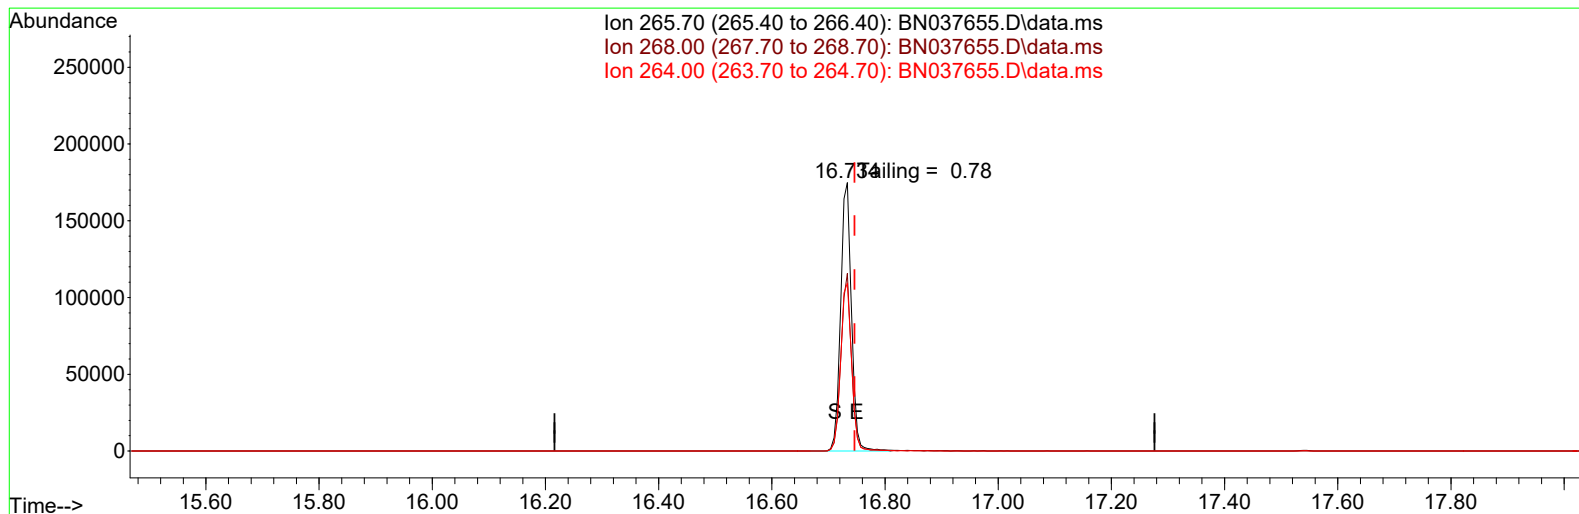

TIC: BN037655.D\data.ms

(70) Pentachlorophenol (C)




16.734min (-0.012) 25239.95 ng

response 232146

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.15
264.00	61.60	62.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090425\
Data File : BN037655.D
Acq On : 04 Sep 2025 10:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 07:32:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

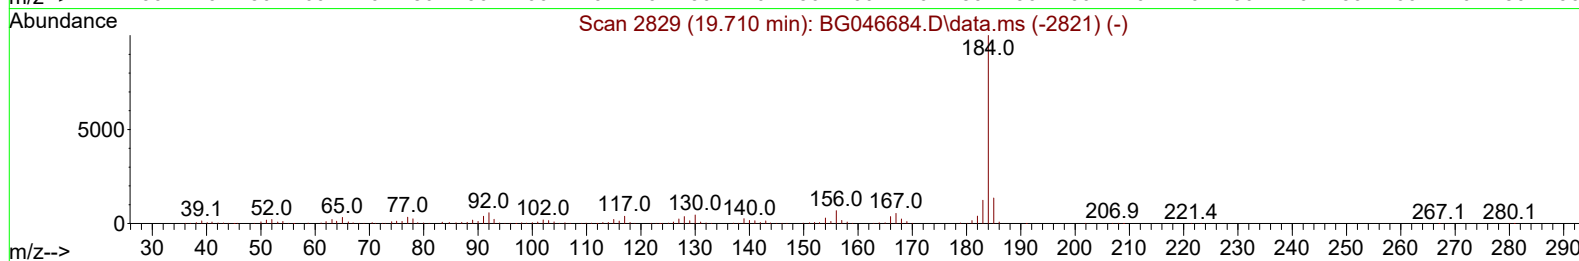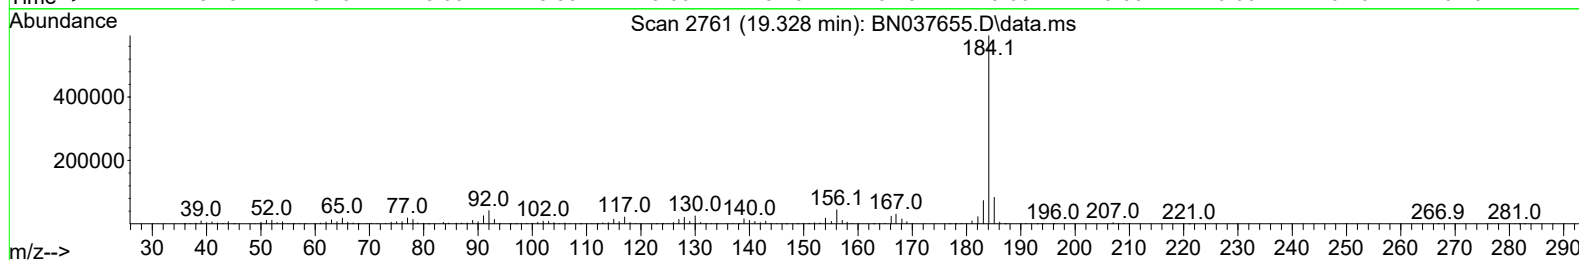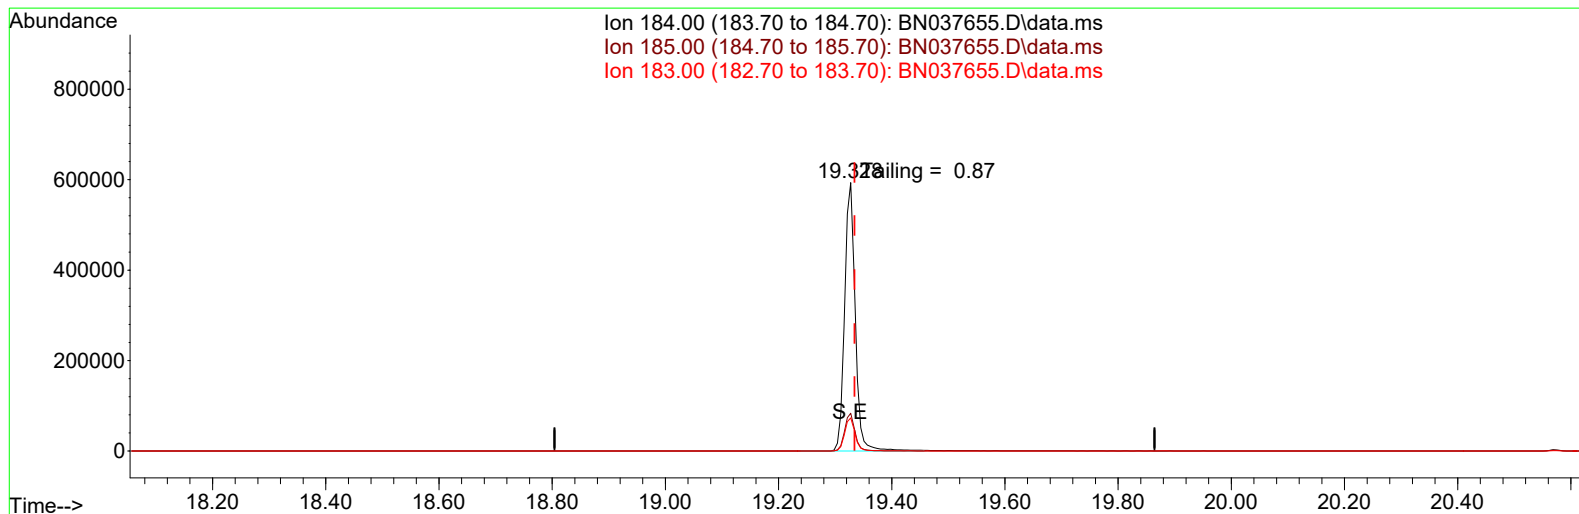

TIC: BN037655.D\data.ms

(77) Benzidine

19.328min (-0.007) 0.00 ng

response 769171

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.10
183.00	13.20	12.33
0.00	0.00	0.00