


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090425\
Data File : BN037655.D
Acq On : 04 Sep 2025 10:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN090425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 04 18:19:43 2025

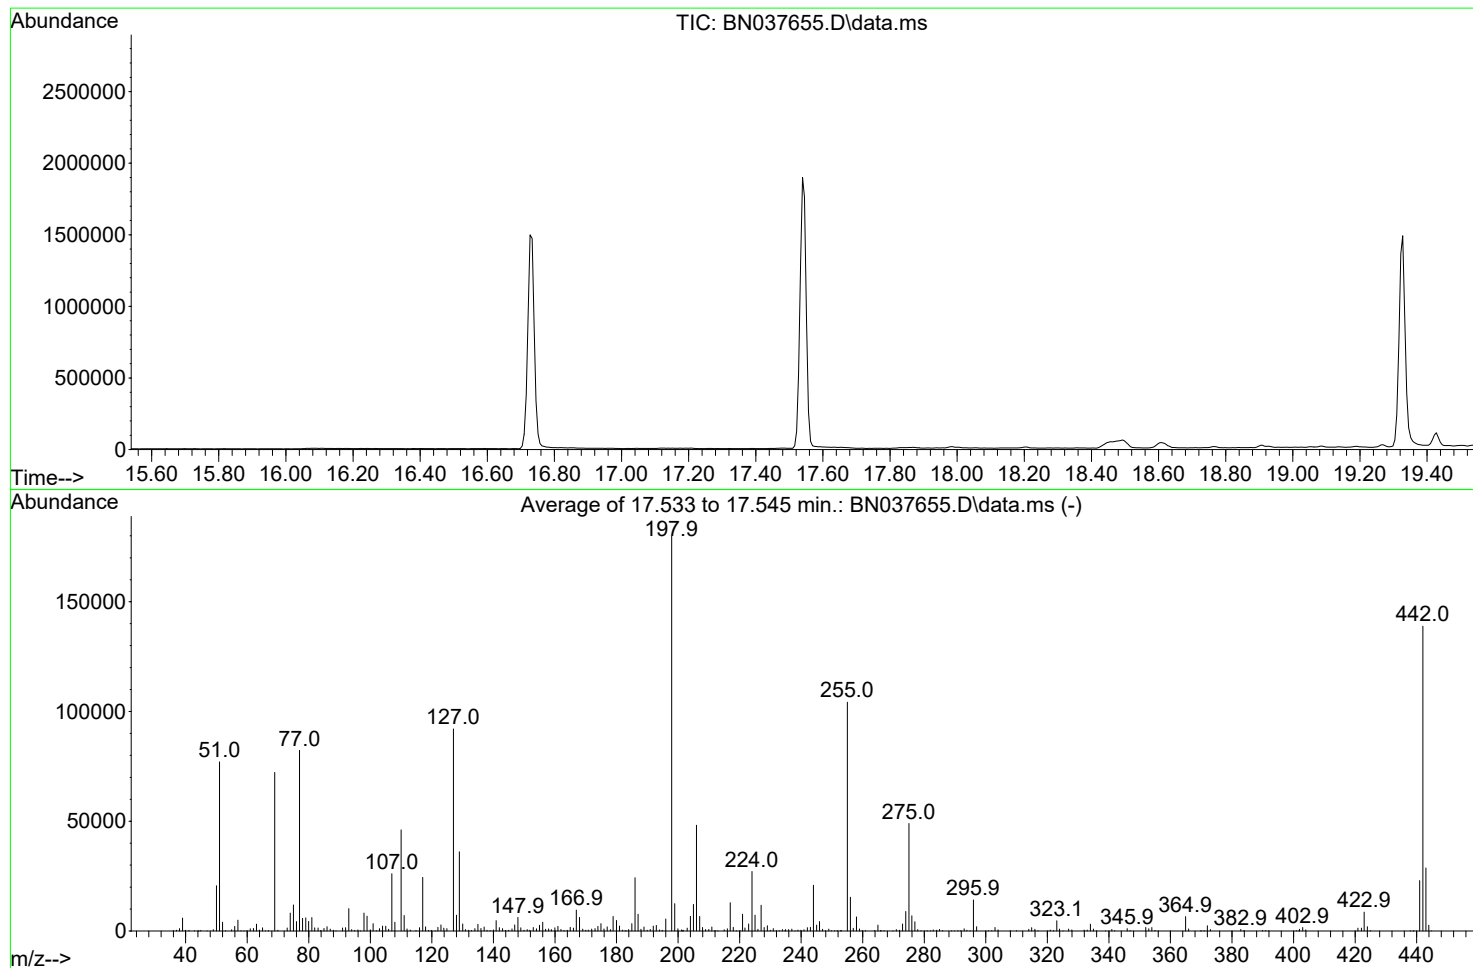

AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	72227	PASS
70	69	0.00	2	0.5	360	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	179861	PASS
199	198	5	9	6.9	12483	PASS
365	198	1	100	3.6	6546	PASS
441	443	0.01	150	80.1	22979	PASS
442	442	100	100	100.0	138835	PASS
443	442	15	24	20.7	28697	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/4/2025	BNA_N	<u>BN037655.D</u>
Compound Name	Response	Retention Time
DDT	623059	20.574
DDD	4529	20.127
DDE	684	19.622
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5213	628272	0.83

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090425\
Data File : BN037655.D
Acq On : 04 Sep 2025 10:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 05 07:32:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

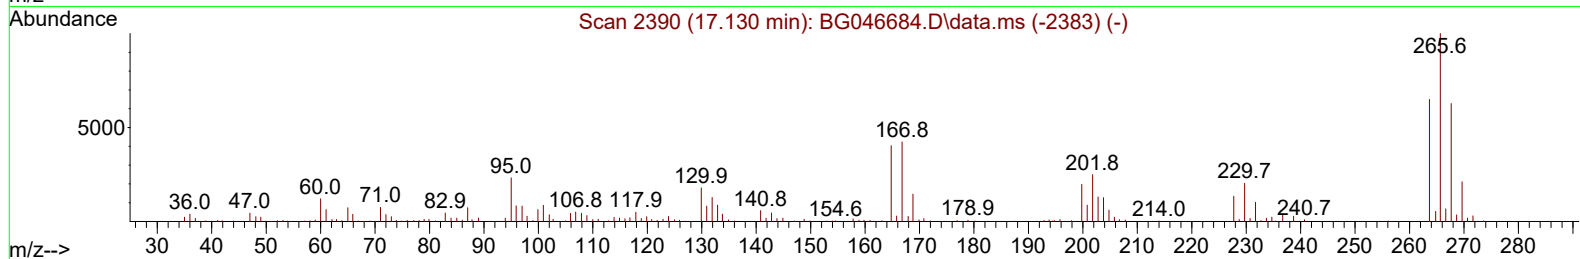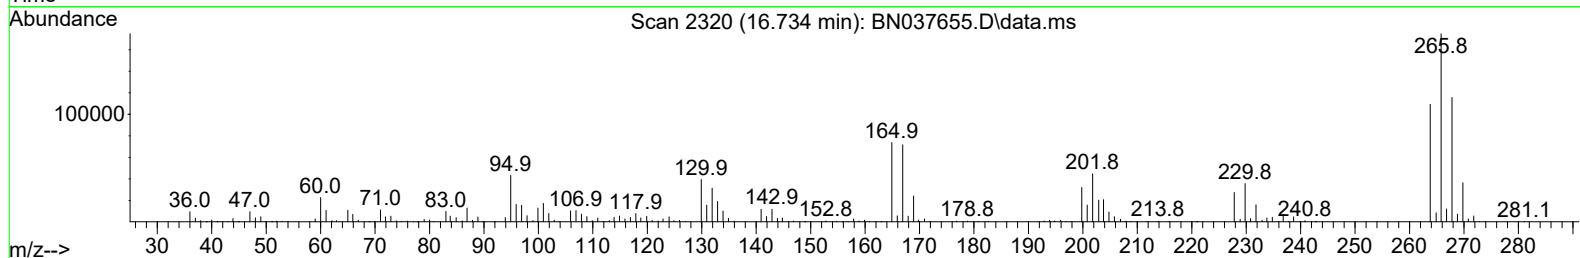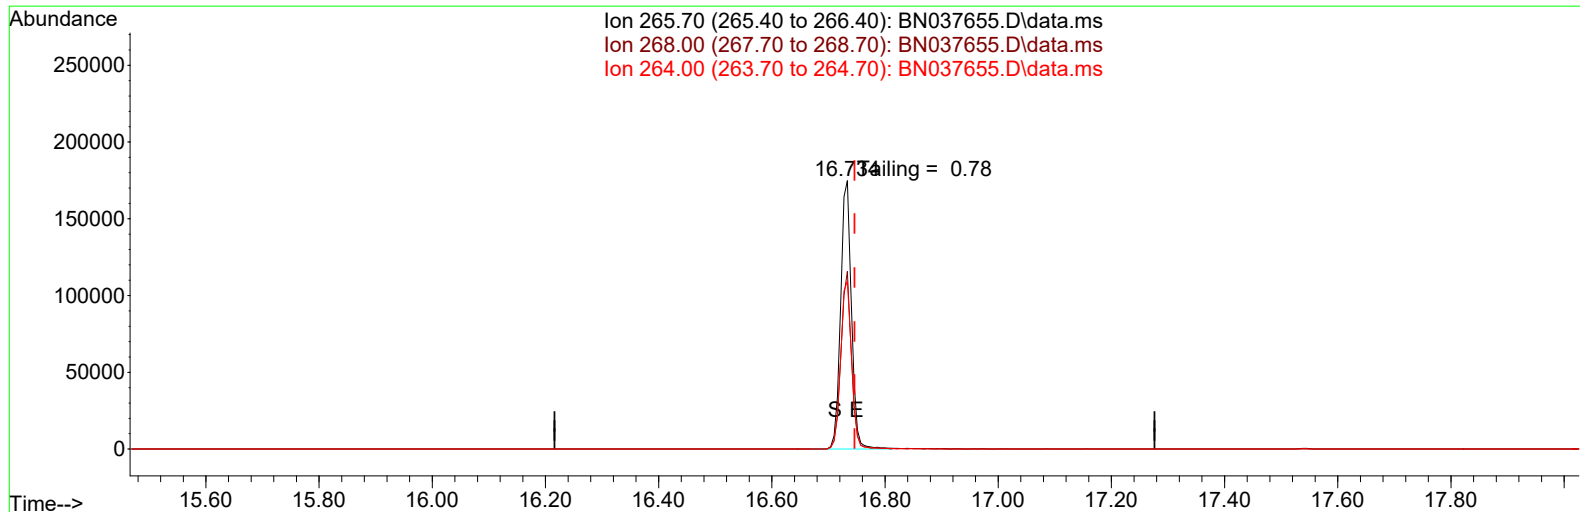

TIC: BN037655.D\data.ms

(70) Pentachlorophenol (C)

16.734min (-0.012) 25239.95 ng




response 232146

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.15
264.00	61.60	62.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090425\
Data File : BN037655.D
Acq On : 04 Sep 2025 10:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 05 07:32:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

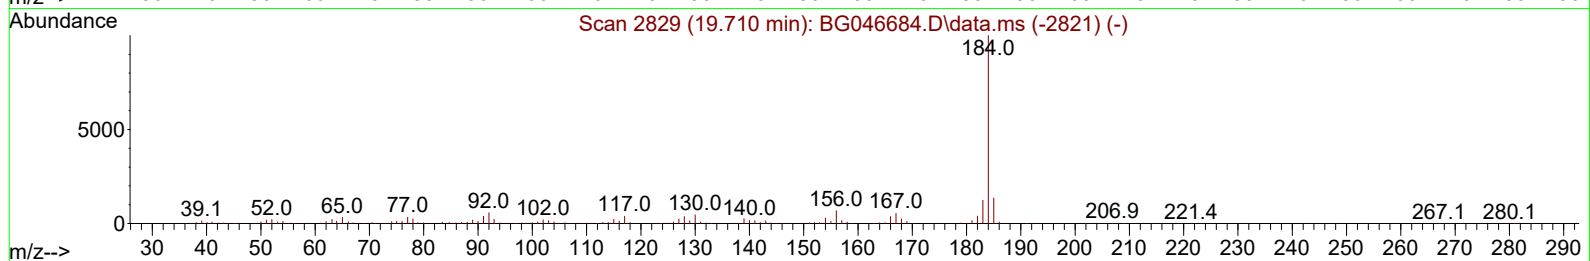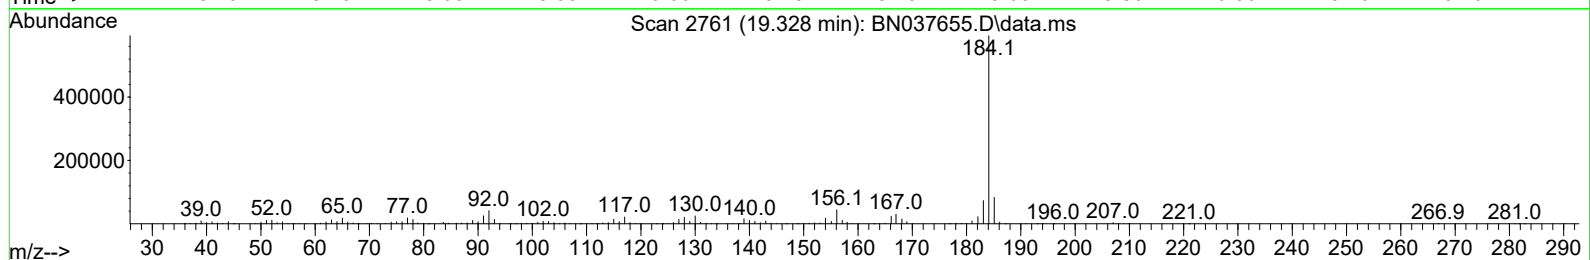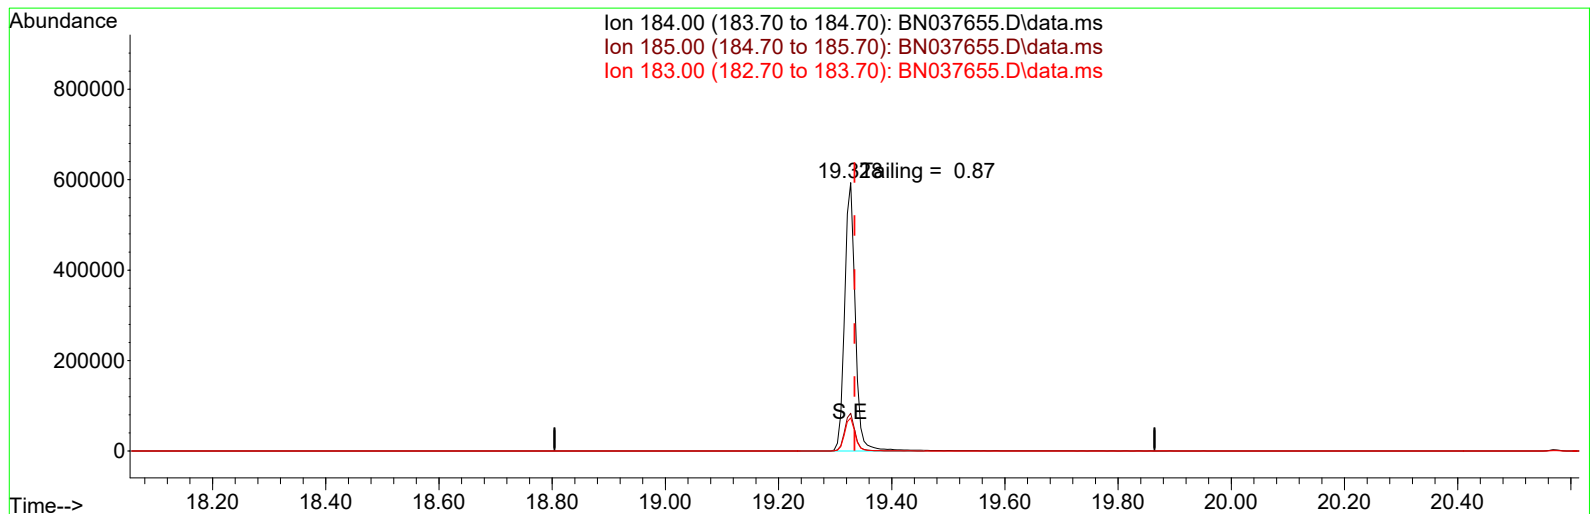

TIC: BN037655.D\data.ms

(77) Benzidine

19.328min (-0.007) 0.00 ng

response 769171

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.10
183.00	13.20	12.33
0.00	0.00	0.00