


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN090519\
 Data File : BN007535.D
 Acq On : 05 Sep 2019 14:52
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 29 12:18:45 2019

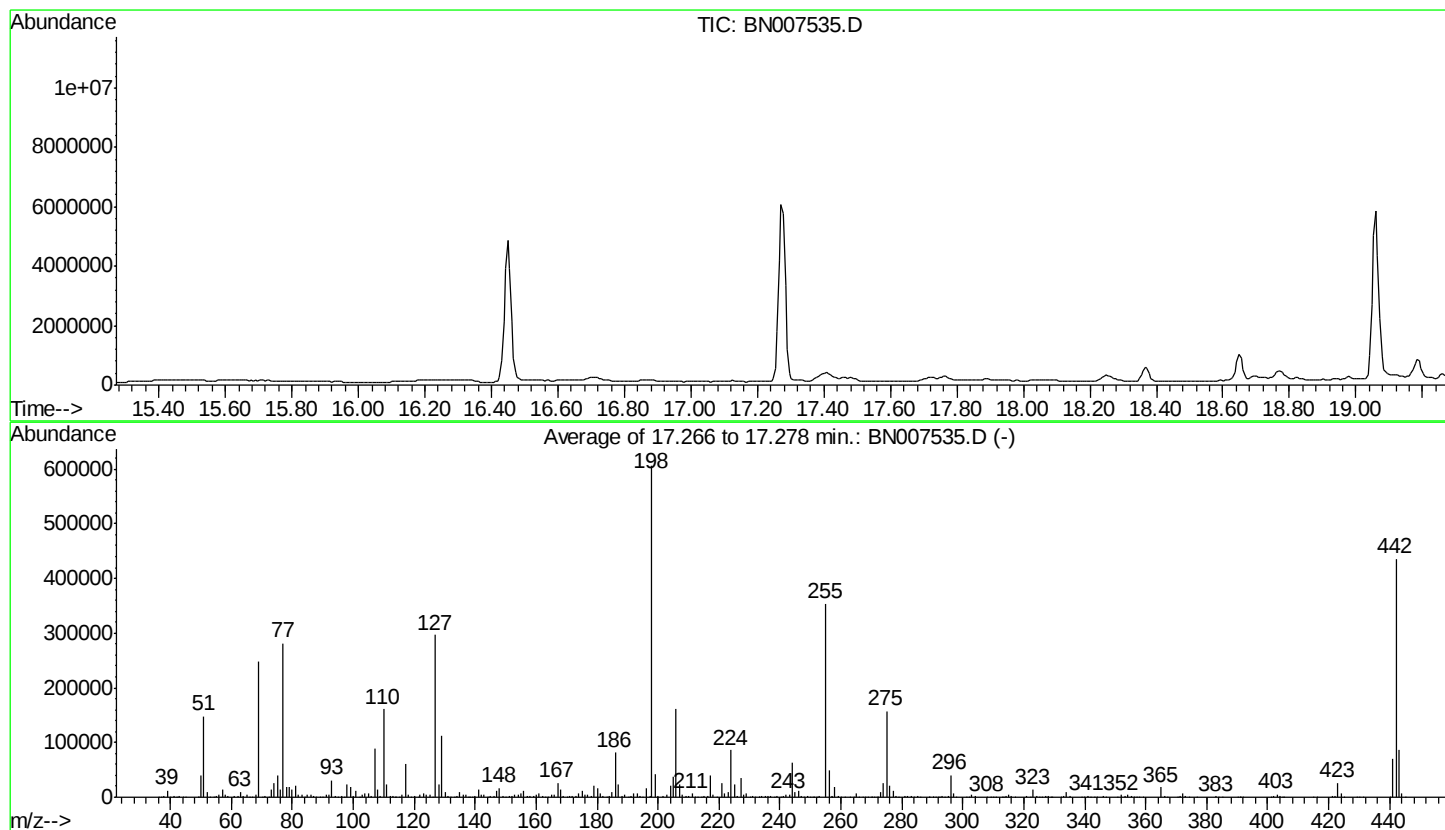

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.4	147918	PASS
68	69	0.00	2	1.7	4167	PASS
69	198	0.00	100	40.9	247851	PASS
70	69	0.00	2	0.4	929	PASS
127	198	10	80	49.0	296798	PASS
197	198	0.00	2	0.3	1589	PASS
198	198	100	100	100.0	606130	PASS
199	198	5	9	6.9	42112	PASS
275	198	10	60	26.0	157882	PASS
365	198	1	100	2.9	17737	PASS
441	198	0.01	100	11.4	69133	PASS
442	198	50	100	71.9	435946	PASS
443	442	15	24	19.7	85981	PASS