
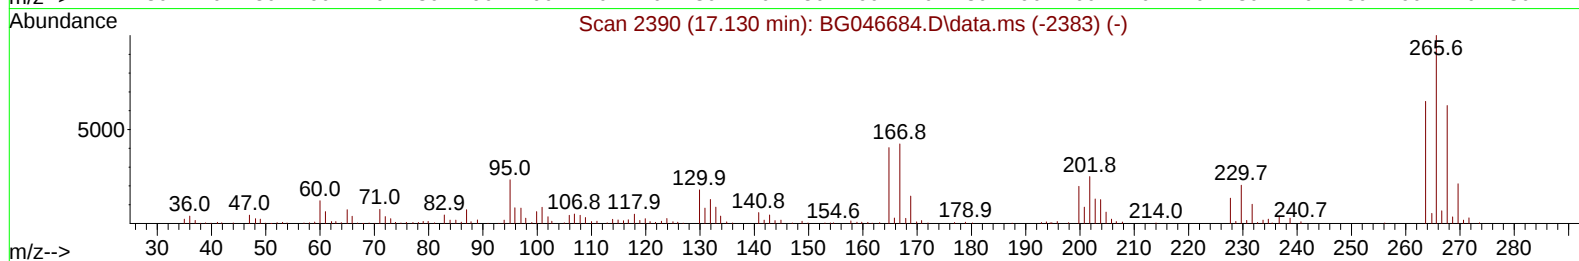
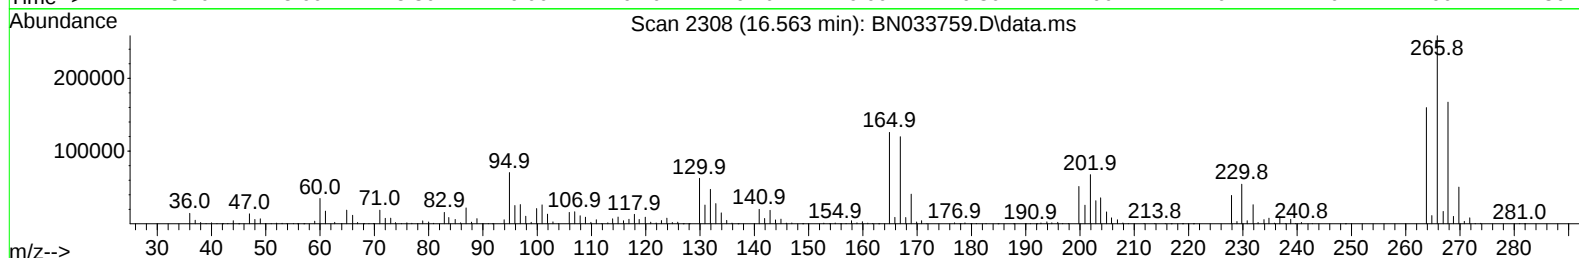


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN090524\  
Data File : BN033759.D  
Acq On : 05 Sep 2024 09:17  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 17:05:55 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Aug 31 04:54:27 2024  
Response via : Initial Calibration

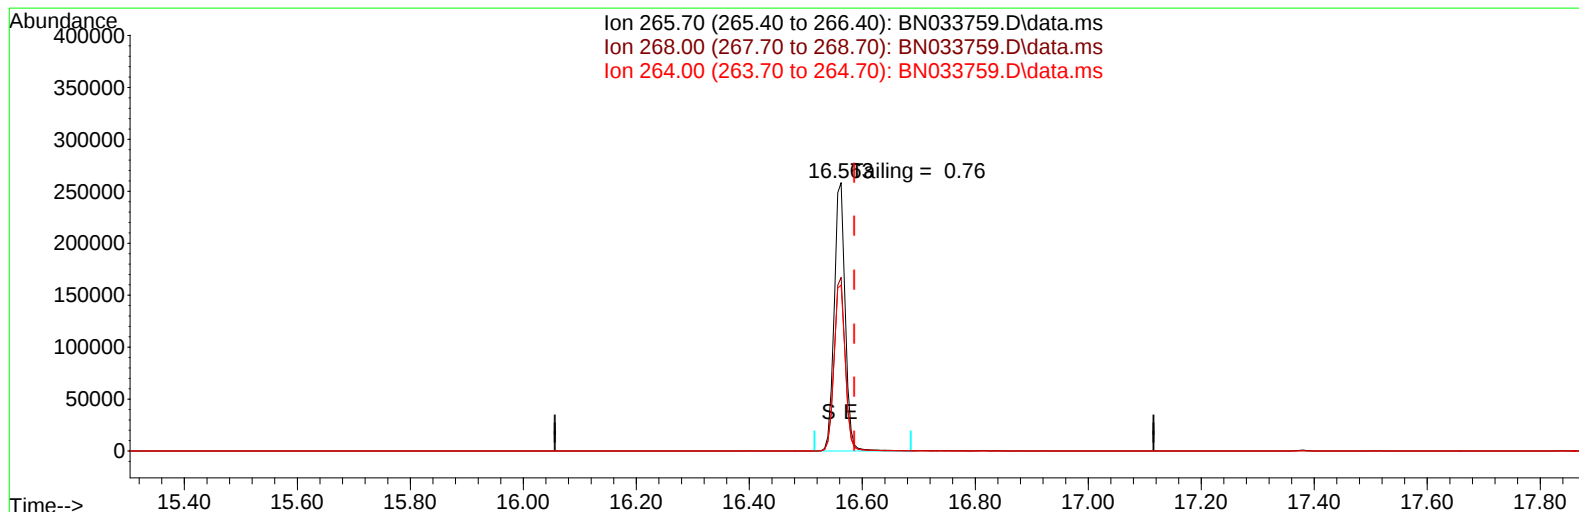

TIC: BN033759.D\data.ms

**(70) Pentachlorophenol (C)**




**16.563min (-0.023) 22225.18 ng**

**response 349184**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 64.73  |
| 264.00 | 61.60  | 61.83  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN090524\  
Data File : BN033759.D  
Acq On : 05 Sep 2024 09:17  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 17:05:55 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Aug 31 04:54:27 2024  
Response via : Initial Calibration

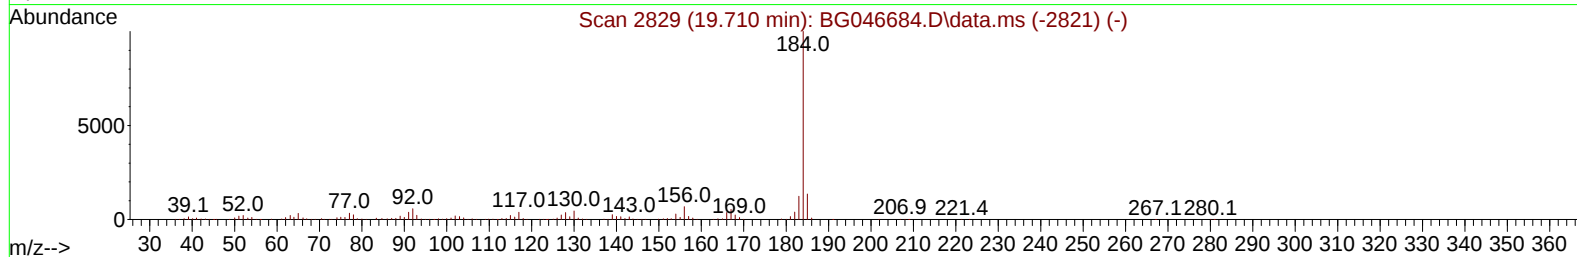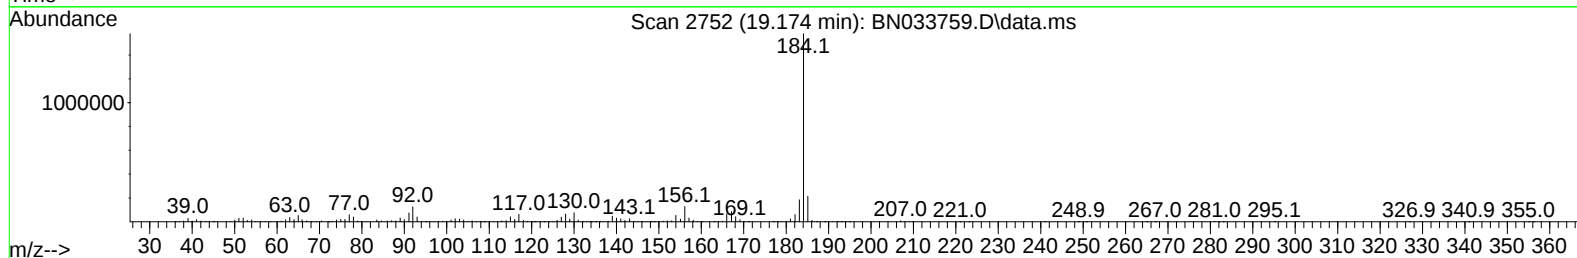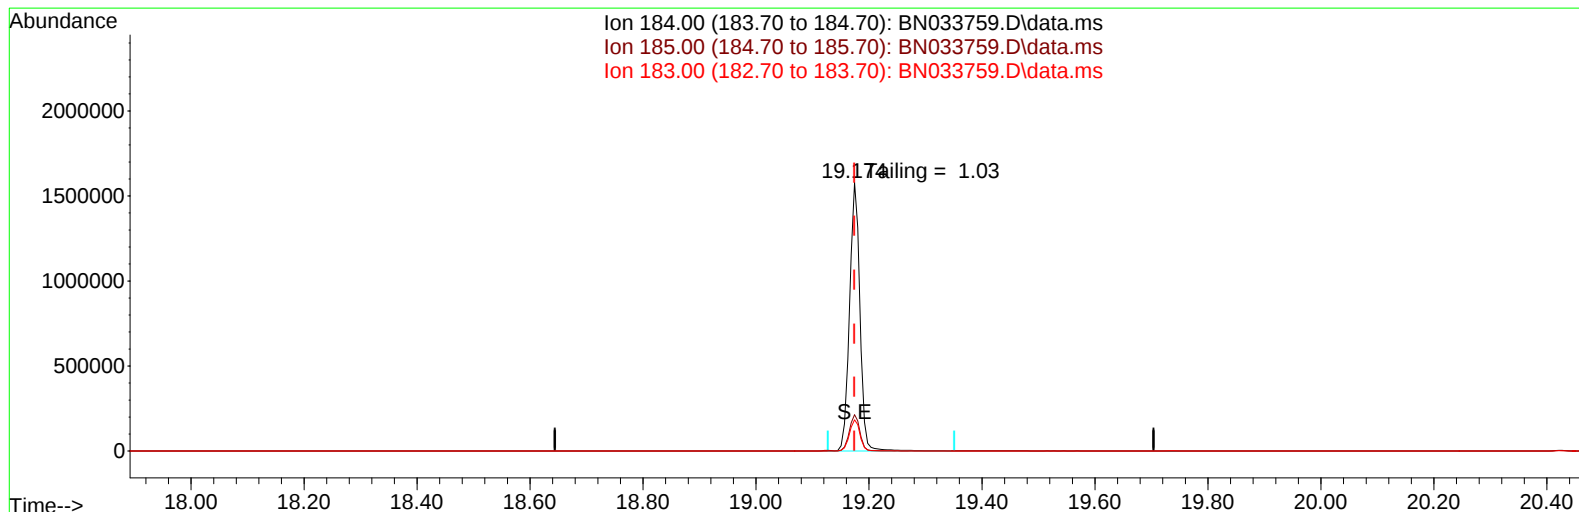

TIC: BN033759.D\data.ms

**(77) Benzidine**

19.174min (+ 0.000) 0.00 ng

response 2020794

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.57  |
| 183.00 | 13.20  | 11.64  |
| 0.00   | 0.00   | 0.00   |