

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
 Data File : BN021605.D
 Acq On : 06 Sep 2022 17:44
 Operator : CG/JU
 Sample : PB147444BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK444

Quant Time: Sep 07 01:05:41 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 07 01:01:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.063	152	183746	20.000	ng/ul	0.00
20) Naphthalene-d8	10.898	136	829918	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.722	164	535612	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.469	188	1079507	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.657	240	928935	20.000	ng/ul	# 0.00
88) Perylene-d12	24.180	264	822726	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	31529	6.443	ng/uL	0.00
4) Pyridine-d5	3.793	84	395445	29.648	ng/ul	0.00
7) Phenol-d5	7.210	99	523309	31.401	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.381	67	340609	33.765	ng/ul	0.00
11) 2-Chlorophenol-d4	7.587	132	412881	34.053	ng/ul	0.00
15) 4-Methylphenol-d8	8.775	113	417436	31.924	ng/ul	0.00
21) Nitrobenzene-d5	9.240	128	210510	37.230	ng/ul	0.00
24) 2-Nitrophenol-d4	9.969	143	218900	43.343	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.510	165	387530	34.647	ng/ul	0.00
31) 4-Chloroaniline-d4	11.034	131	539052	28.378	ng/ul	0.00
46) Dimethylphthalate-d6	14.128	166	1262853	34.496	ng/ul	0.00
49) Acenaphthylene-d8	14.416	160	1469339	34.428	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	209090	28.702	ng/ul	0.00
60) Fluorene-d10	15.710	176	1089600	34.205	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.822	200	155738	36.069	ng/ul	0.00
73) Anthracene-d10	17.569	188	1644779	34.574	ng/ul	0.00
81) Pyrene-d10	19.863	212	1822710	41.259	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.010	264	1455931	37.335	ng/ul	0.00
Target Compounds						
					Qvalue	
17) N-Nitroso-di-n-propyla...	8.775	70	10400	1.010	ng/ul#	1
48) 2,6-Dinitrotoluene	14.134	165	6646	1.035	ng/ul#	37


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
Data File : BN021605.D
Acq On : 06 Sep 2022 17:44
Operator : CG/JU
Sample : PB147444BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK444

Quant Time: Sep 07 01:05:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 07 01:01:49 2022
Response via : Initial Calibration




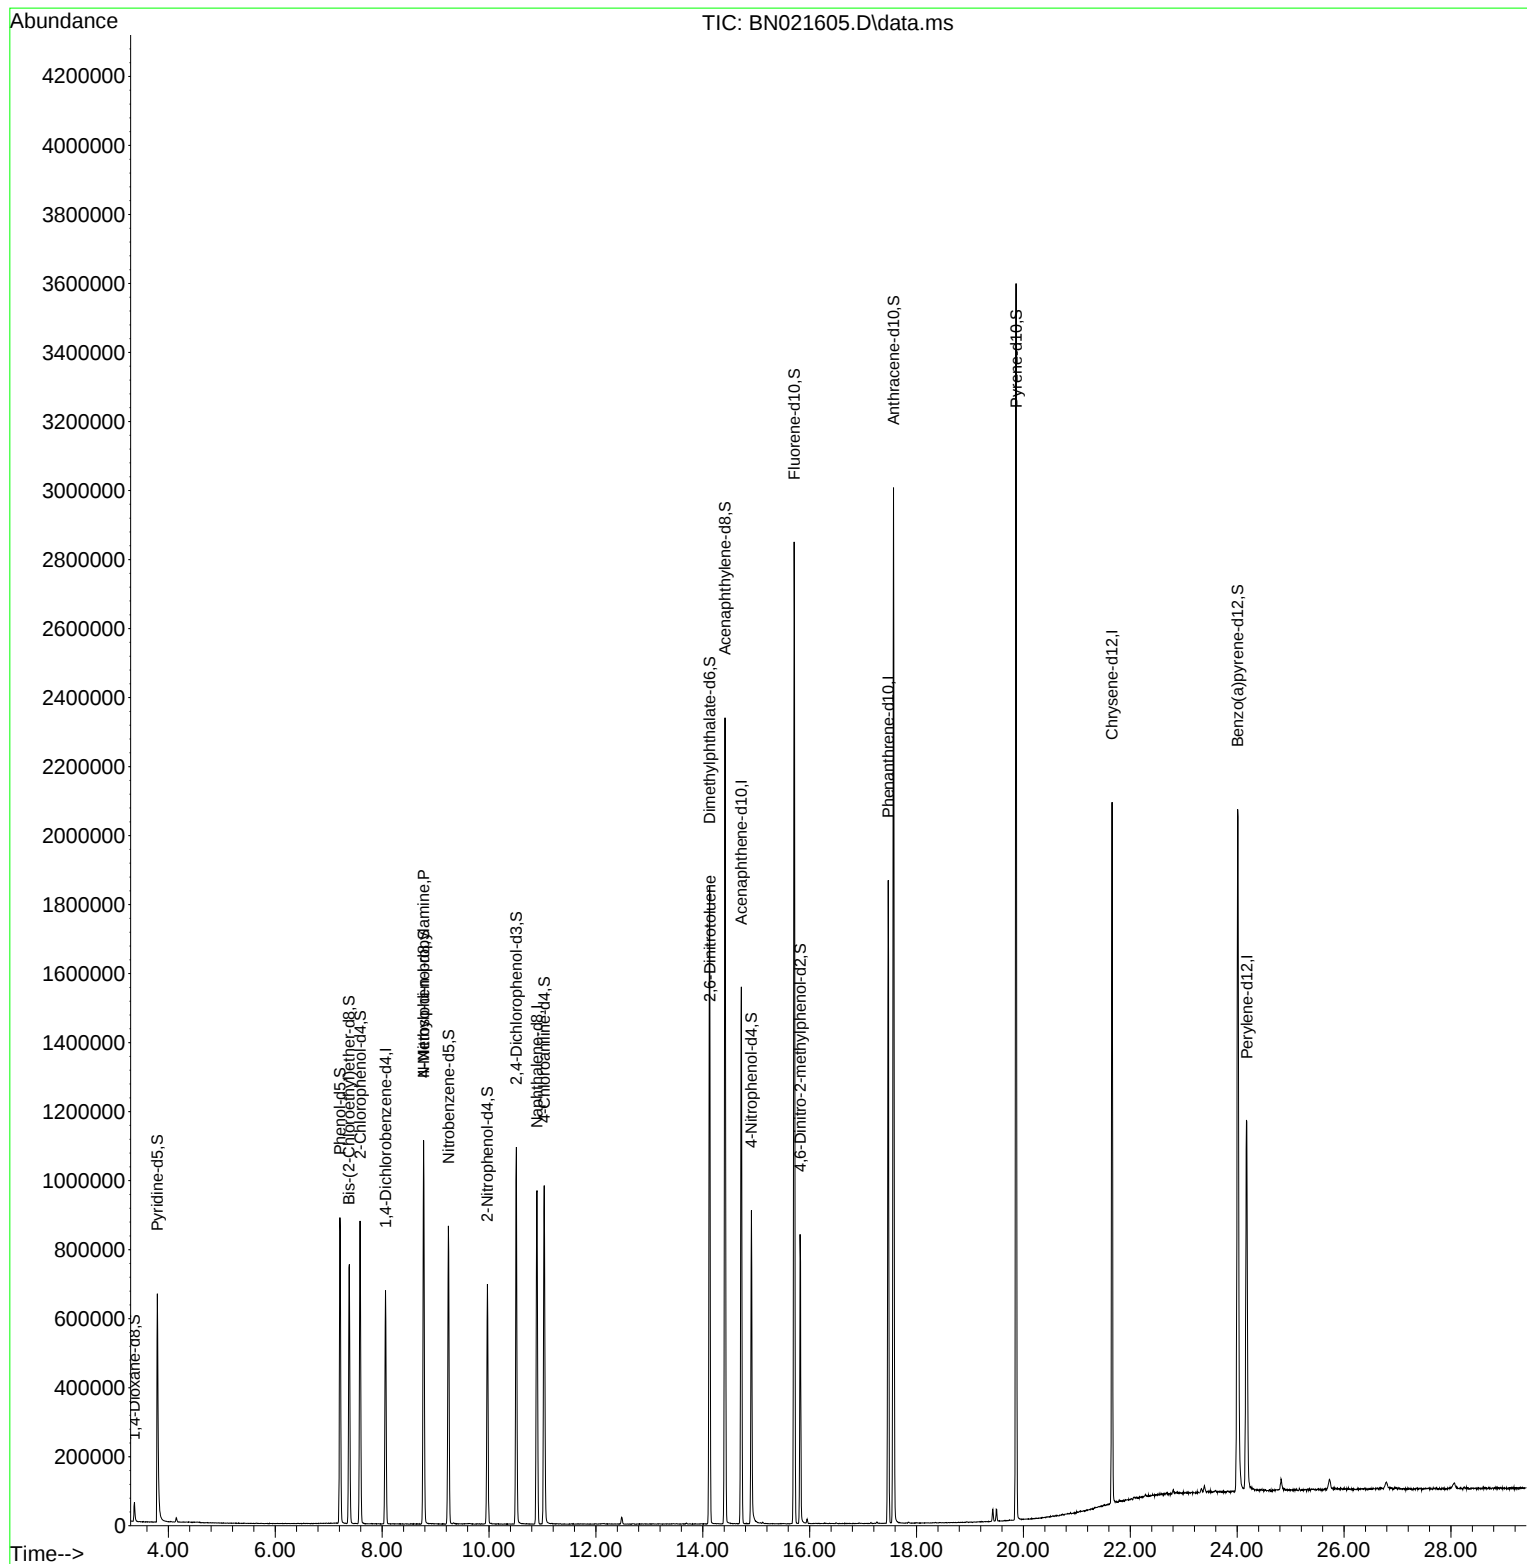


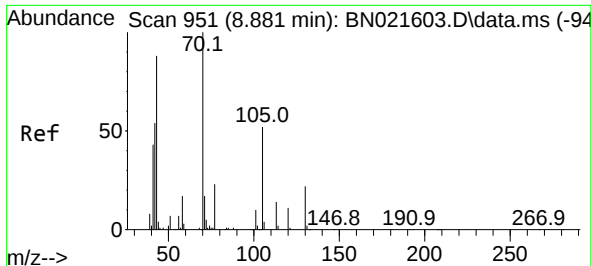

#17
N-Nitroso-di-n-propylamine
Concen: 1.010 ng/ul
RT: 8.775 min Scan# 91
Delta R.T. -0.106 min
Lab File: BN021605.D
Acq: 06 Sep 2022 17:44

Instrument :
BNA_N
ClientSampleId :
SBLK444

Tgt Ion: 70 Resp: 10400
Ion Ratio Lower Upper
70 100
42 339.2 47.8 71.6#
101 0.0 7.8 11.6#
130 0.0 15.8 23.8#

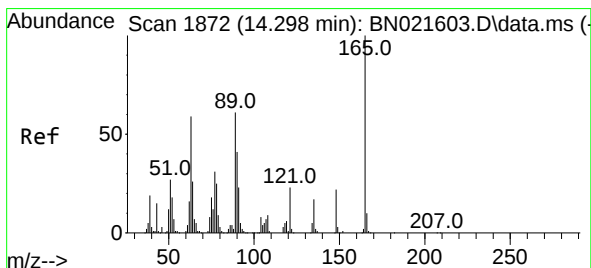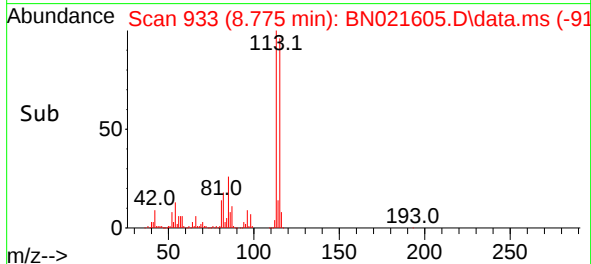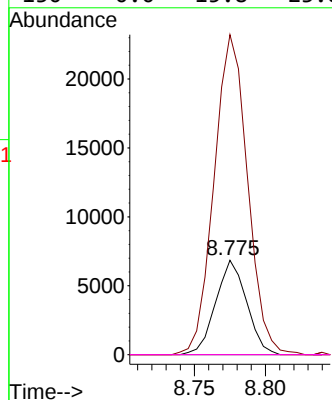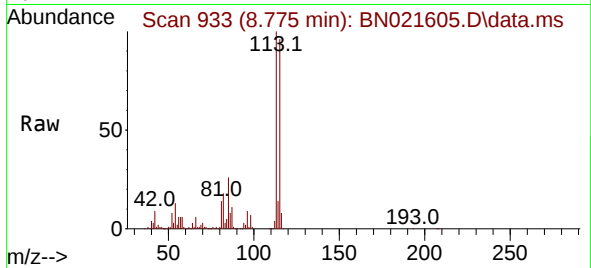

#48
2,6-Dinitrotoluene
Concen: 1.035 ng/ul
RT: 14.134 min Scan# 1844
Delta R.T. -0.165 min
Lab File: BN021605.D
Acq: 06 Sep 2022 17:44

Tgt Ion: 165 Resp: 6646
Ion Ratio Lower Upper
165 100
89 0.0 50.6 75.8#
121 27.9 17.9 26.9#

