

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
 Data File : BN021606.D
 Acq On : 06 Sep 2022 18:22
 Operator : CG/JU
 Sample : N4482-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW366

Quant Time: Sep 07 01:05:58 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 07 01:01:49 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.063	152	170461	20.000	ng/ul	0.00
20) Naphthalene-d8	10.898	136	766129	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.722	164	501155	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.469	188	1013252	20.000	ng/ul	0.00
79) Chrysene-d12	21.662	240	884554	20.000	ng/ul	0.00
88) Perylene-d12	24.180	264	761926	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	23614	5.201	ng/uL	0.00
4) Pyridine-d5	3.799	84	106076	8.573	ng/ul	0.00
7) Phenol-d5	7.216	99	112679	7.288	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.387	67	324428	34.667	ng/ul	0.00
11) 2-Chlorophenol-d4	7.587	132	291599	25.924	ng/ul	0.00
15) 4-Methylphenol-d8	8.775	113	206940	17.059	ng/ul	0.00
21) Nitrobenzene-d5	9.240	128	200328	38.379	ng/ul	0.00
24) 2-Nitrophenol-d4	9.969	143	188101	40.346	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.510	165	325437	31.518	ng/ul	0.00
31) 4-Chloroaniline-d4	11.034	131	427105	24.357	ng/ul	0.00
46) Dimethylphthalate-d6	14.128	166	1265719	36.951	ng/ul	0.00
49) Acenaphthylene-d8	14.416	160	1431427	35.846	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	37597	5.516	ng/ul	0.00
60) Fluorene-d10	15.710	176	1115295	37.419	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.822	200	162303	40.047	ng/ul	0.00
73) Anthracene-d10	17.569	188	1800231	40.317	ng/ul	0.00
81) Pyrene-d10	19.863	212	1965622	46.727	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.015	264	1653800	45.794	ng/ul	0.00
Target Compounds						
48) 2,6-Dinitrotoluene	14.133	165	6405	1.066	ng/ul#	35


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
Data File : BN021606.D
Acq On : 06 Sep 2022 18:22
Operator : CG/JU
Sample : N4482-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW366

Quant Time: Sep 07 01:05:58 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 07 01:01:49 2022
Response via : Initial Calibration

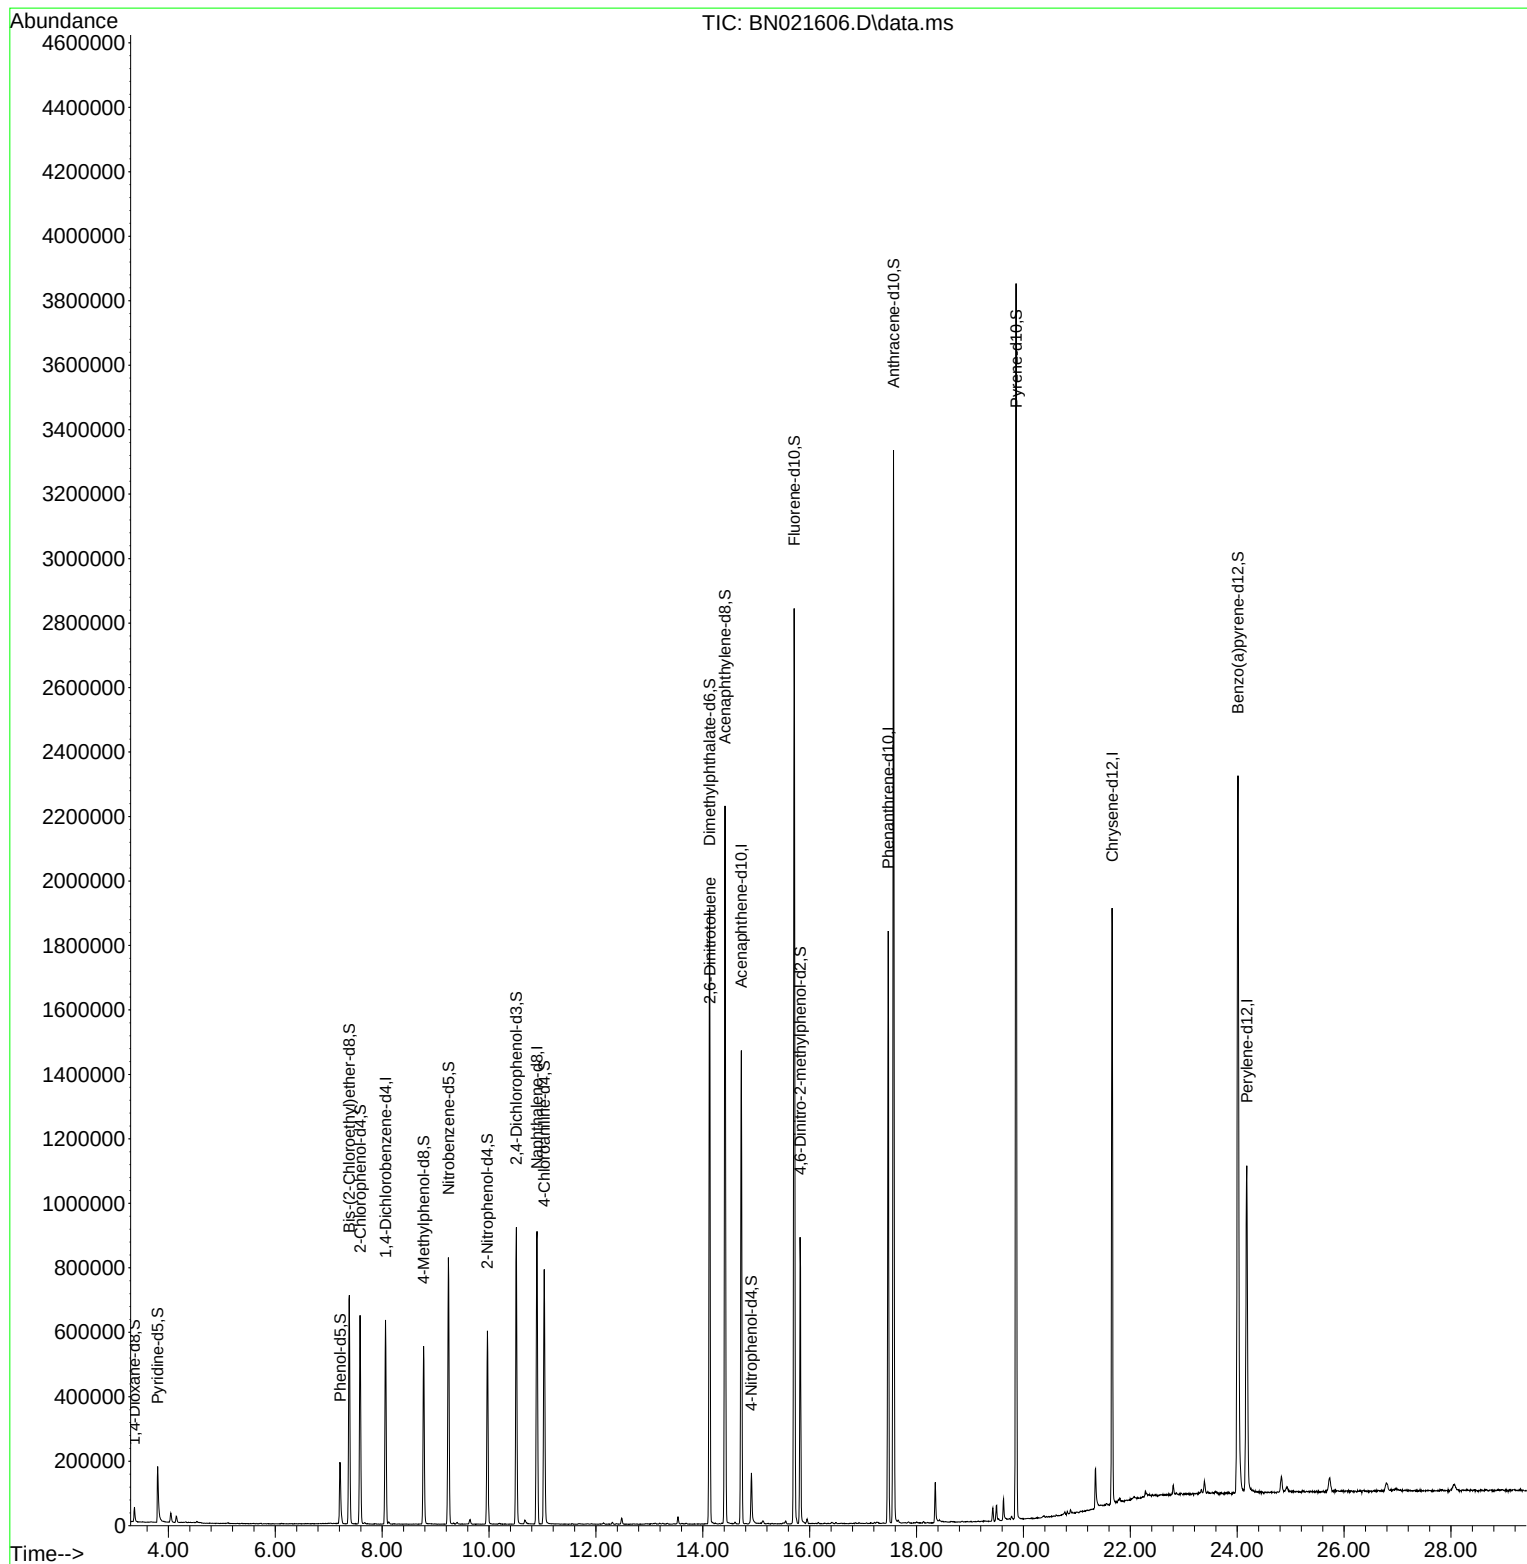

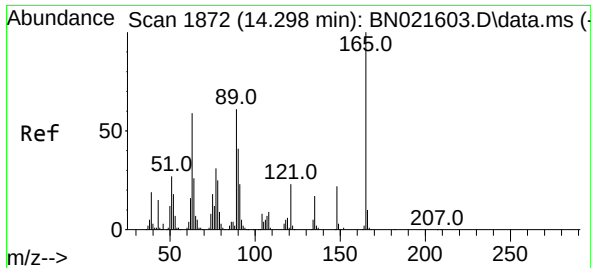

#48

2,6-Dinitrotoluene

Concen: 1.066 ng/ul

RT: 14.133 min Scan# 11

Delta R.T. -0.165 min

Lab File: BN021606.D


Acq: 06 Sep 2022 18:22

Instrument :

BNA_N

ClientSampleId :

EW366

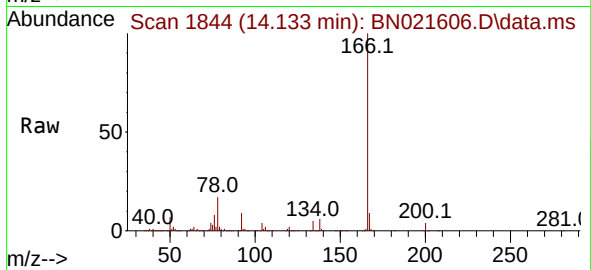

Tgt Ion:165 Resp: 6405

Ion Ratio Lower Upper

165 100

89 0.0 50.6 75.8#

121 31.5 17.9 26.9#

