

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
 Data File : BN021607.D
 Acq On : 06 Sep 2022 18:59
 Operator : CG/JU
 Sample : N4482-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW344

Quant Time: Sep 07 01:06:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 07 01:01:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.063	152	157657	20.000	ng/ul	0.00
20) Naphthalene-d8	10.898	136	711175	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.722	164	442590	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.468	188	907372	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.656	240	806784	20.000	ng/ul	0.00
88) Perylene-d12	24.180	264	740362	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	23112	5.504	ng/uL	0.00
4) Pyridine-d5	3.799	84	140789	12.302	ng/ul	0.00
7) Phenol-d5	7.216	99	127313	8.904	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.381	67	334973	38.701	ng/ul	0.00
11) 2-Chlorophenol-d4	7.587	132	318773	30.642	ng/ul	0.00
15) 4-Methylphenol-d8	8.775	113	235333	20.975	ng/ul	0.00
21) Nitrobenzene-d5	9.239	128	206369	42.591	ng/ul	0.00
24) 2-Nitrophenol-d4	9.969	143	204084	47.156	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.510	165	371021	38.710	ng/ul	0.00
31) 4-Chloroaniline-d4	11.033	131	467699	28.733	ng/ul	0.00
46) Dimethylphthalate-d6	14.127	166	1319158	43.607	ng/ul	0.00
49) Acenaphthylene-d8	14.416	160	1455298	41.266	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	39603	6.579	ng/ul	0.00
60) Fluorene-d10	15.710	176	1122269	42.636	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.821	200	165263	45.536	ng/ul	0.00
73) Anthracene-d10	17.568	188	1752131	43.818	ng/ul	0.00
81) Pyrene-d10	19.862	212	1969544	51.333	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.009	264	1642845	46.815	ng/ul	0.00
Target Compounds						
48) 2,6-Dinitrotoluene	14.133	165	7037	1.326	ng/ul#	Qvalue 32


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
Data File : BN021607.D
Acq On : 06 Sep 2022 18:59
Operator : CG/JU
Sample : N4482-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW344


Quant Time: Sep 07 01:06:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 07 01:01:49 2022
Response via : Initial Calibration

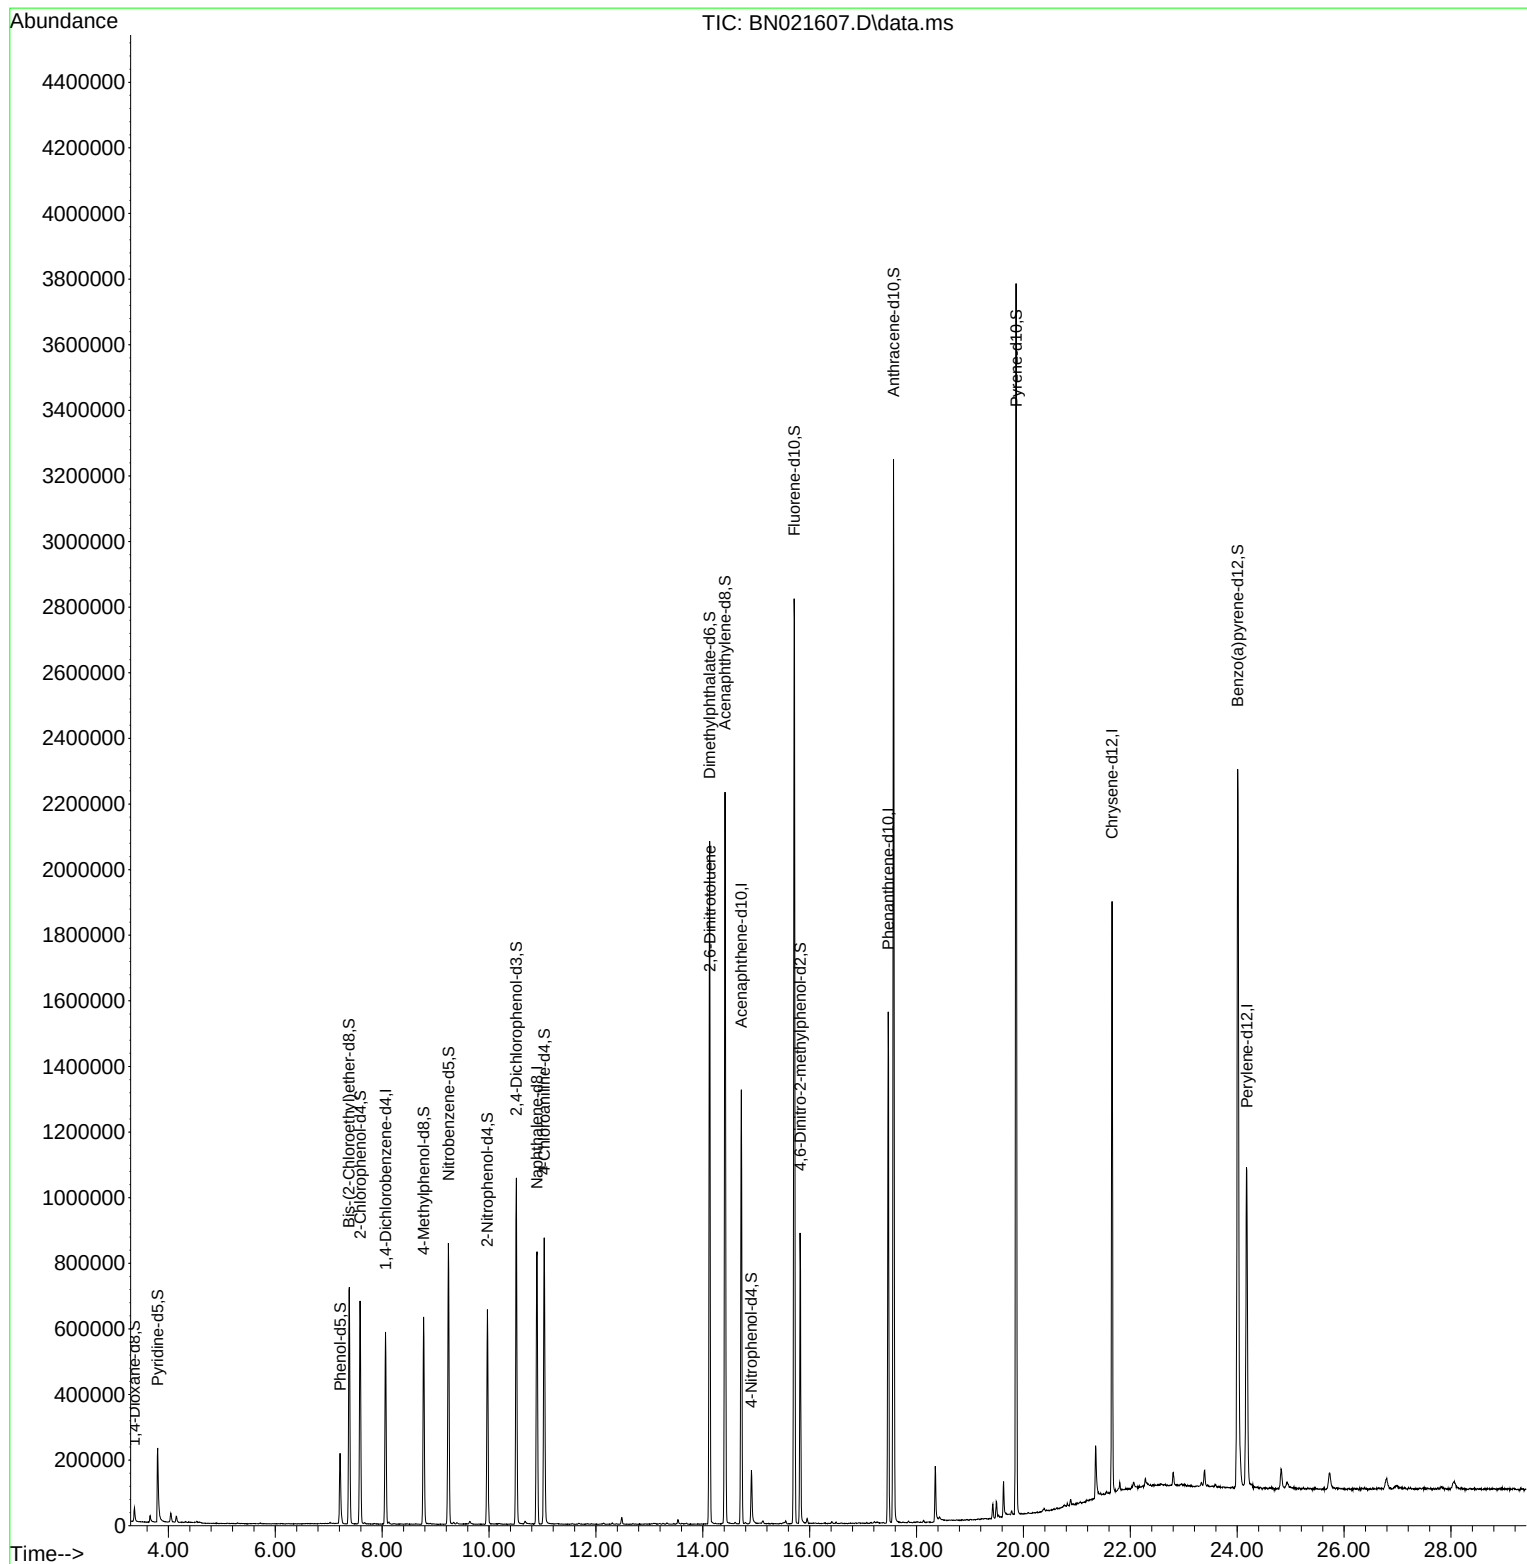

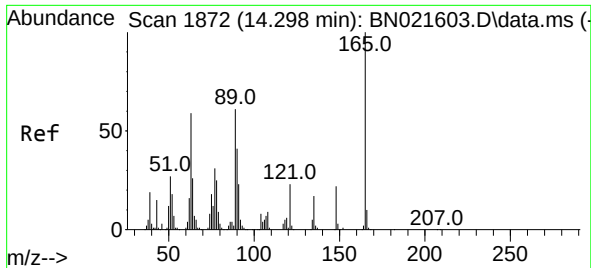

#48
 2,6-Dinitrotoluene
 Concen: 1.326 ng/ul
 RT: 14.133 min Scan# 11
 Delta R.T. -0.165 min
 Lab File: BN021607.D
 Acq: 06 Sep 2022 18:59

Instrument :
 BNA_N
 ClientSampleId :
 EW344

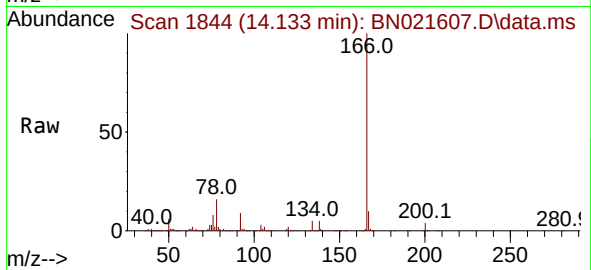

Tgt Ion:165 Resp: 7037
 Ion Ratio Lower Upper
 165 100
 89 0.0 50.6 75.8#
 121 37.2 17.9 26.9#

