

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
 Data File : BN021610.D
 Acq On : 06 Sep 2022 20:52
 Operator : CG/JU
 Sample : N4482-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW346

Quant Time: Sep 07 01:07:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 07 01:01:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.063	152	151886	20.000	ng/ul	0.00
20) Naphthalene-d8	10.898	136	680906	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.722	164	443576	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.468	188	916009	20.000	ng/ul	0.00
79) Chrysene-d12	21.656	240	858166	20.000	ng/ul	0.00
88) Perylene-d12	24.174	264	732092	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	19857	4.909	ng/uL	0.00
4) Pyridine-d5	3.799	84	114338	10.370	ng/ul	0.00
7) Phenol-d5	7.210	99	108461	7.873	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.381	67	301802	36.194	ng/ul	0.00
11) 2-Chlorophenol-d4	7.587	132	285852	28.521	ng/ul	0.00
15) 4-Methylphenol-d8	8.775	113	196688	18.197	ng/ul	0.00
21) Nitrobenzene-d5	9.239	128	189277	40.800	ng/ul	0.00
24) 2-Nitrophenol-d4	9.969	143	183857	44.371	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.510	165	311020	33.892	ng/ul	0.00
31) 4-Chloroaniline-d4	11.033	131	352408	22.612	ng/ul	0.00
46) Dimethylphthalate-d6	14.127	166	1204365	39.724	ng/ul	0.00
49) Acenaphthylene-d8	14.416	160	1319473	37.331	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	40747	6.754	ng/ul	0.00
60) Fluorene-d10	15.710	176	1036425	39.287	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.821	200	174582	47.650	ng/ul	0.00
73) Anthracene-d10	17.568	188	1825540	45.224	ng/ul	0.00
81) Pyrene-d10	19.862	212	2070026	50.722	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.009	264	1808491	52.118	ng/ul	0.00
Target Compounds						
48) 2,6-Dinitrotoluene	14.133	165	6166	1.159	ng/ul#	34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
Data File : BN021610.D
Acq On : 06 Sep 2022 20:52
Operator : CG/JU
Sample : N4482-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW346

Quant Time: Sep 07 01:07:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 07 01:01:49 2022
Response via : Initial Calibration

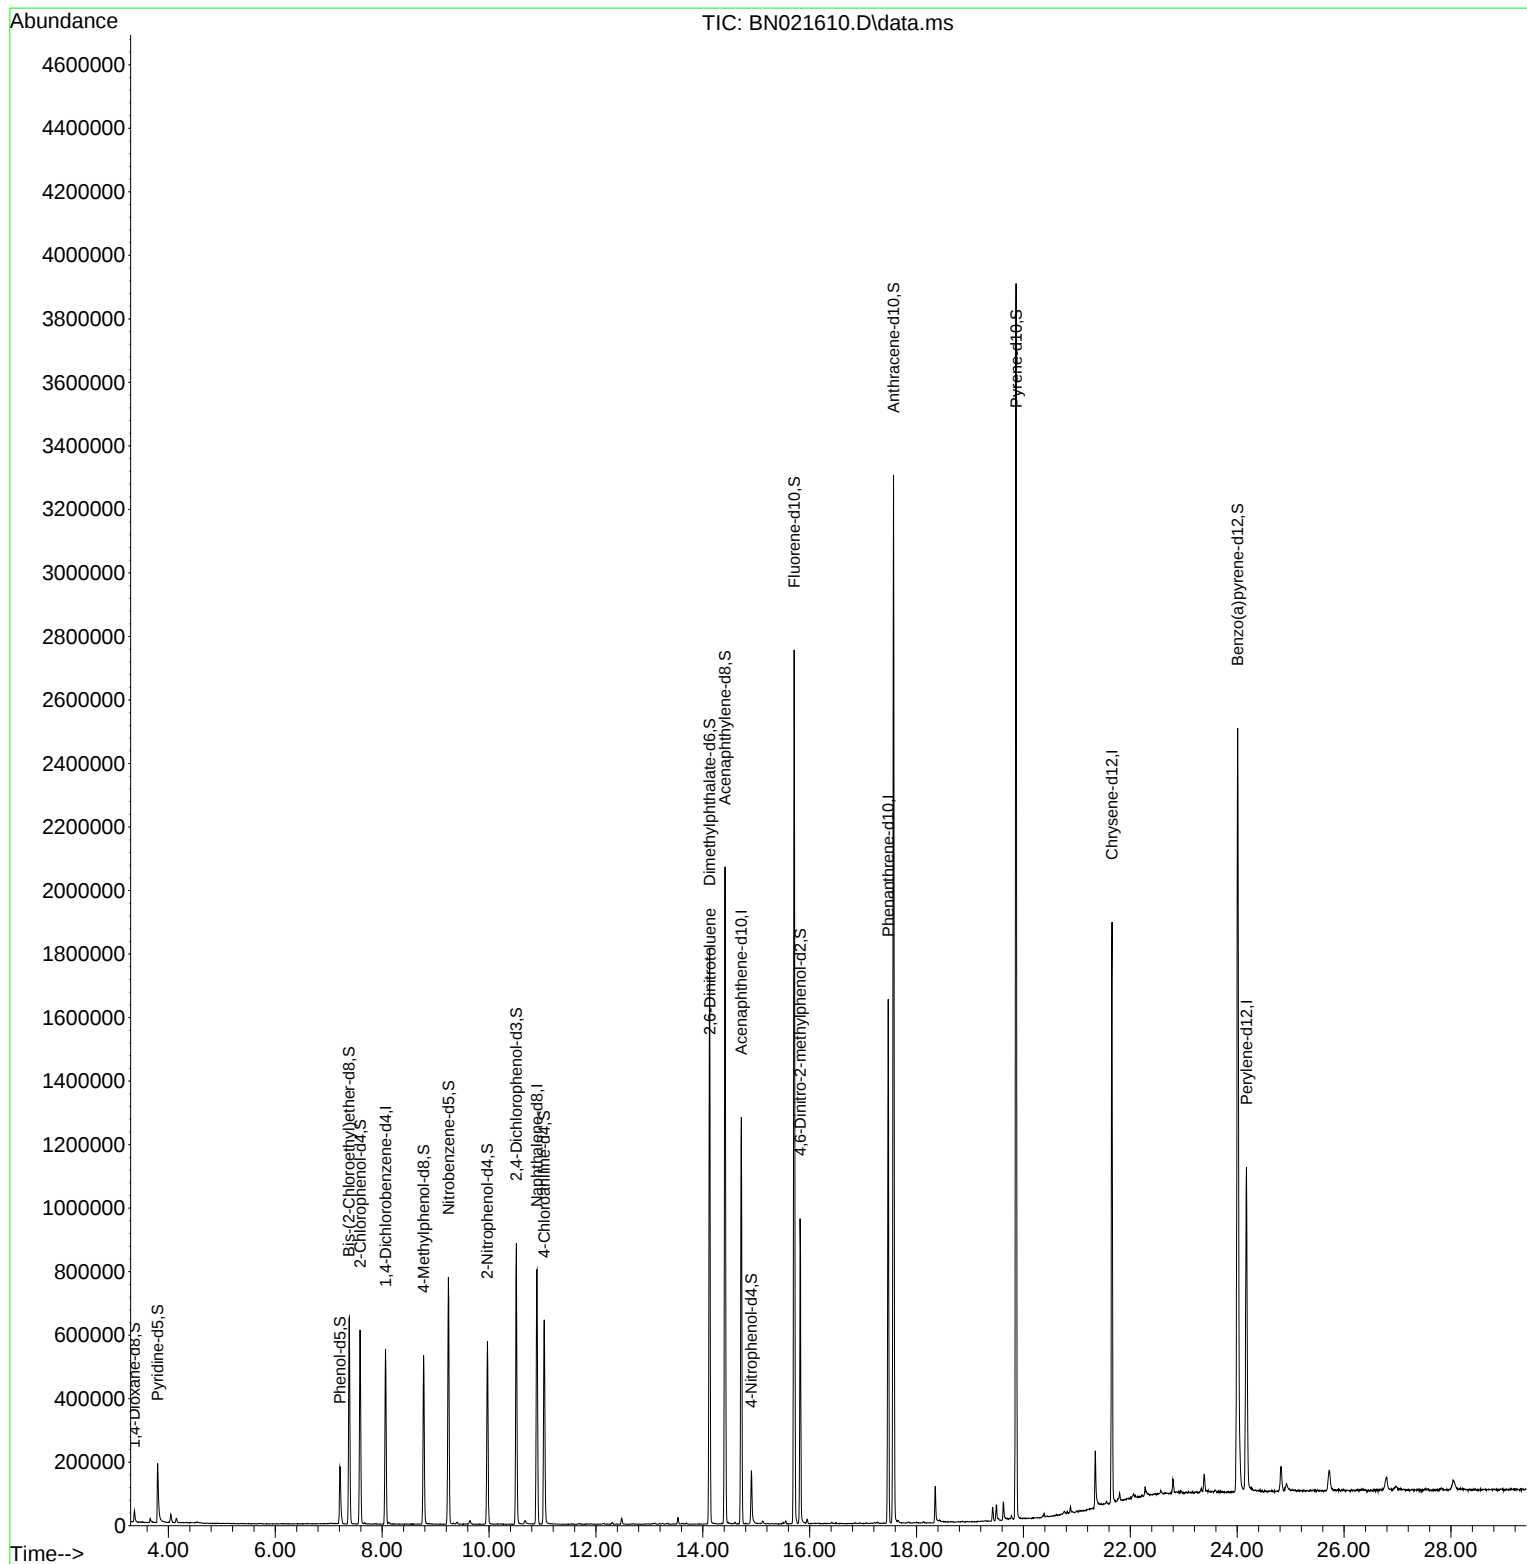

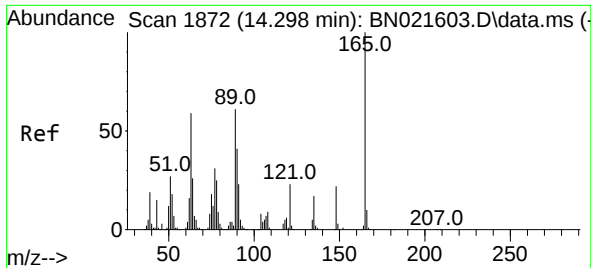

#48

2,6-Dinitrotoluene

Concen: 1.159 ng/ul

RT: 14.133 min Scan# 11

Delta R.T. -0.165 min

Lab File: BN021610.D


Acq: 06 Sep 2022 20:52

Instrument :

BNA_N

ClientSampleId :

EW346

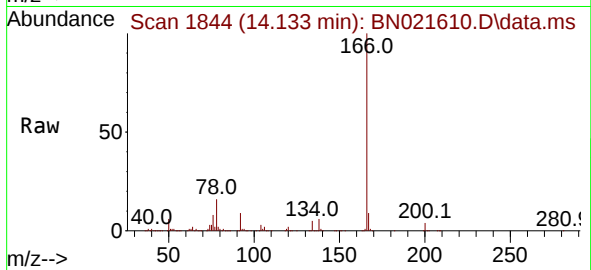

Tgt Ion:165 Resp: 6166

Ion Ratio Lower Upper

165 100

89 0.0 50.6 75.8#

121 34.1 17.9 26.9#

