

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
 Data File : BN021612.D
 Acq On : 06 Sep 2022 22:08
 Operator : CG/JU
 Sample : N4484-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0KR2

Quant Time: Sep 07 01:08:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 07 01:01:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.063	152	182061	20.000	ng/u1	0.00
20) Naphthalene-d8	10.899	136	838519	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.722	164	542562	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.469	188	1149896	20.000	ng/u1	0.00
79) Chrysene-d12	21.657	240	1032735	20.000	ng/u1	0.00
88) Perylene-d12	24.174	264	878903	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	22580	4.657	ng/uL	0.00
4) Pyridine-d5	3.799	84	81259	6.149	ng/u1	0.00
7) Phenol-d5	7.216	99	130183	7.884	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.381	67	323477	32.363	ng/u1	0.00
11) 2-Chlorophenol-d4	7.587	132	315508	26.263	ng/u1	0.00
15) 4-Methylphenol-d8	8.775	113	230570	17.796	ng/u1	0.00
21) Nitrobenzene-d5	9.240	128	204056	35.718	ng/u1	0.00
24) 2-Nitrophenol-d4	9.969	143	201432	39.475	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.510	165	345711	30.591	ng/u1	0.00
31) 4-Chloroaniline-d4	11.034	131	380939	19.849	ng/u1	0.00
46) Dimethylphthalate-d6	14.128	166	1360404	36.685	ng/u1	0.00
49) Acenaphthylene-d8	14.416	160	1470929	34.024	ng/u1	0.00
54) 4-Nitrophenol-d4	14.910	143	47204	6.397	ng/u1	0.00
60) Fluorene-d10	15.710	176	1137978	35.267	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.822	200	184048	40.016	ng/u1	0.00
73) Anthracene-d10	17.569	188	1871793	36.938	ng/u1	0.00
81) Pyrene-d10	19.863	212	2092134	42.598	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.010	264	1749291	41.991	ng/u1	0.00
Target Compounds						
48) 2,6-Dinitrotoluene	14.134	165	6854	1.053	ng/u1#	36


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
Data File : BN021612.D
Acq On : 06 Sep 2022 22:08
Operator : CG/JU
Sample : N4484-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0KR2

Quant Time: Sep 07 01:08:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 07 01:01:49 2022
Response via : Initial Calibration

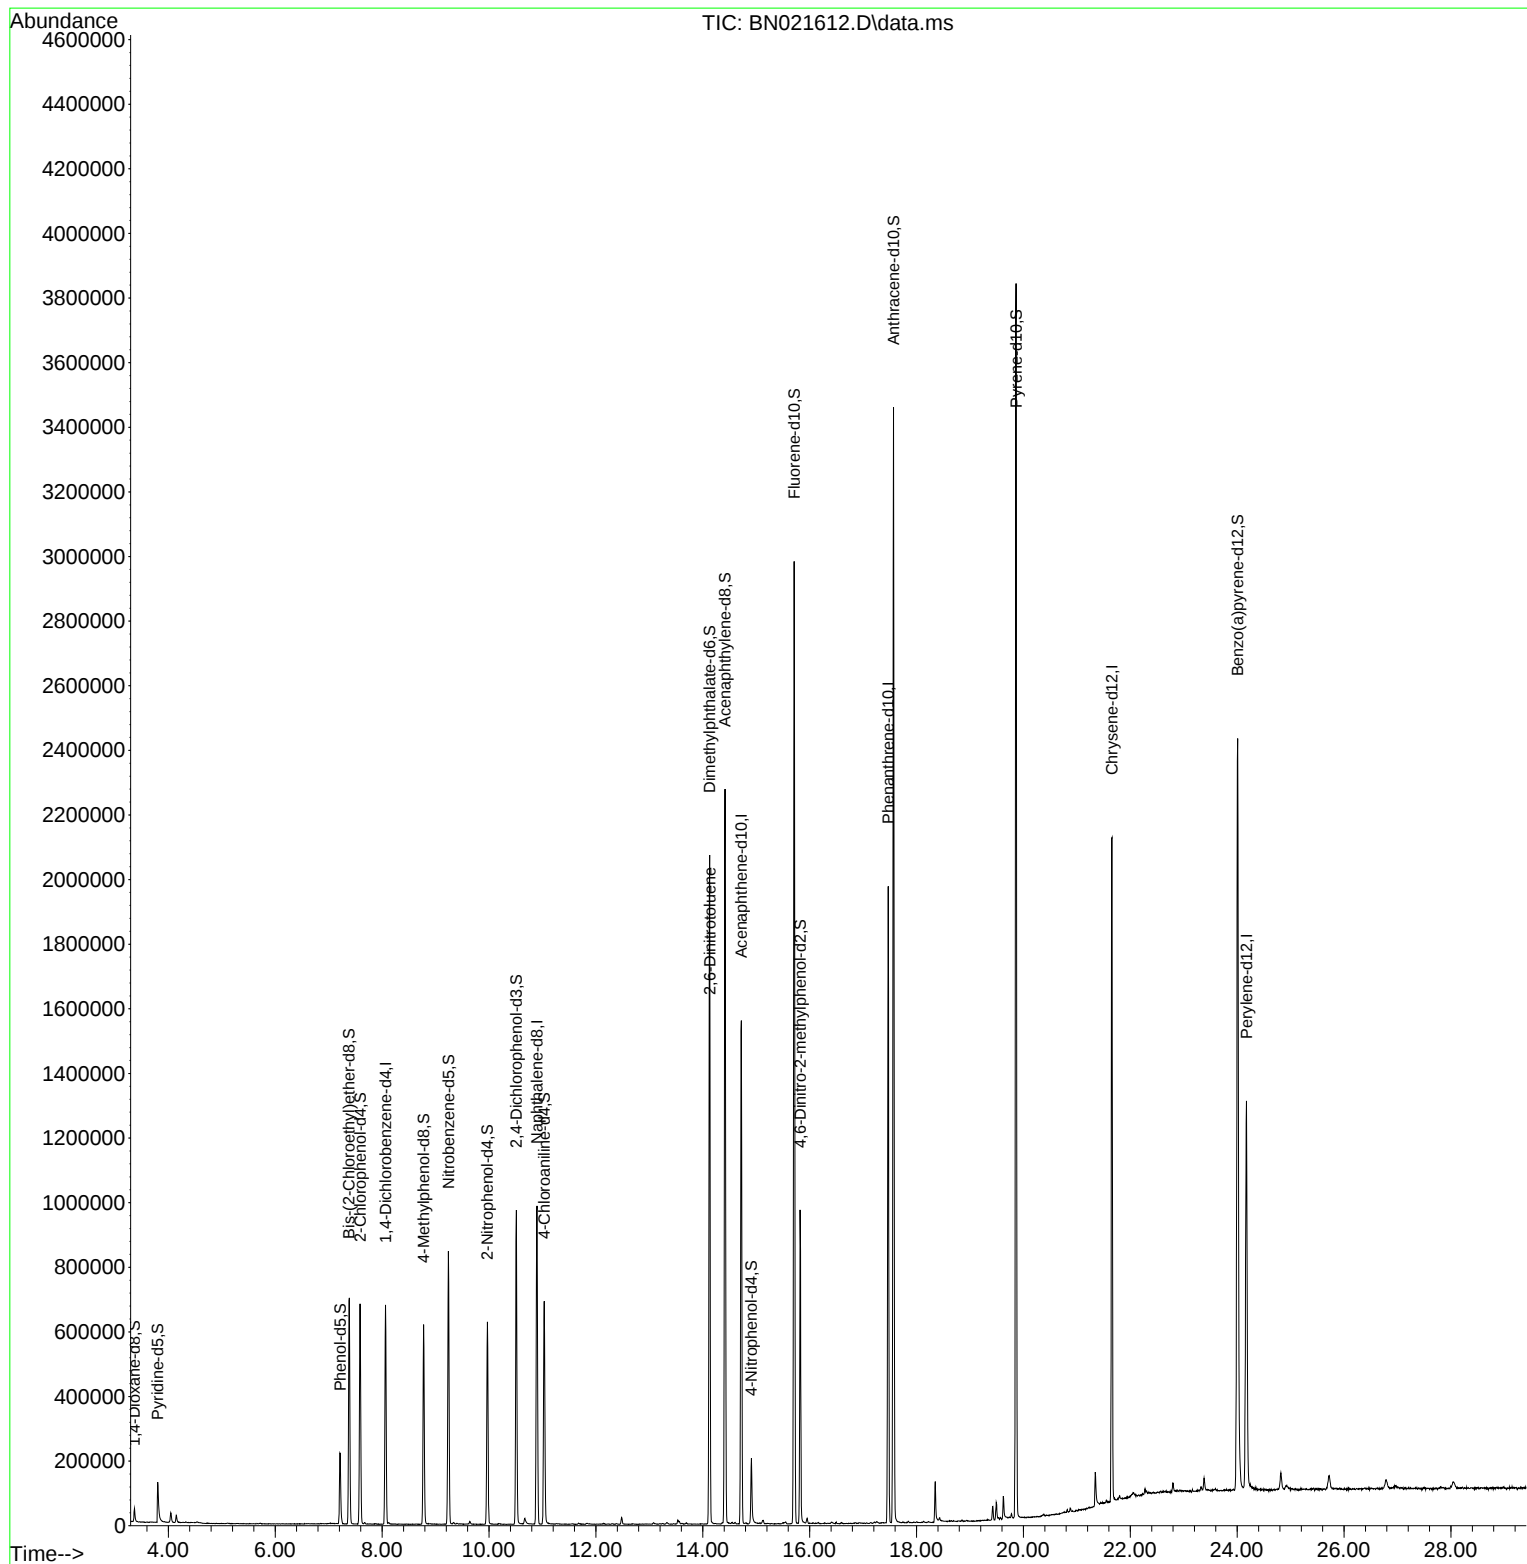

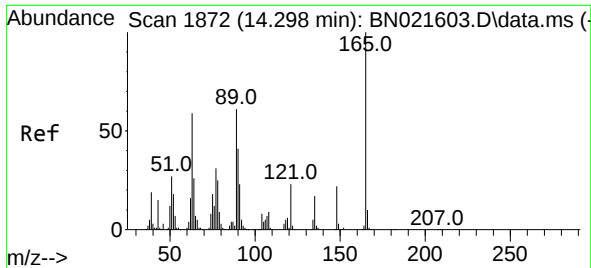

#48

2,6-Dinitrotoluene

Concen: 1.053 ng/ul

RT: 14.134 min Scan# 11

Delta R.T. -0.165 min

Lab File: BN021612.D


Acq: 06 Sep 2022 22:08

Instrument :

BNA_N

ClientSampleId :

C0KR2

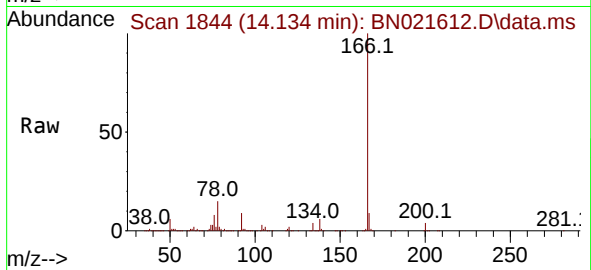

Tgt Ion:165 Resp: 6854

Ion Ratio Lower Upper

165 100

89 0.0 50.6 75.8#

121 30.3 17.9 26.9#

