

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
 Data File : BN021613.D
 Acq On : 06 Sep 2022 22:46
 Operator : CG/JU
 Sample : N4482-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW345

Quant Time: Sep 07 01:08:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 07 01:01:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.063	152	176326	20.000	ng/ul	0.00
20) Naphthalene-d8	10.899	136	807292	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.722	164	528034	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.469	188	1084648	20.000	ng/ul	0.00
79) Chrysene-d12	21.657	240	951643	20.000	ng/ul	# 0.00
88) Perylene-d12	24.168	264	822720	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	20101	4.280	ng/uL	0.00
4) Pyridine-d5	3.805	84	58854	4.598	ng/ul	0.01
7) Phenol-d5	7.216	99	104173	6.514	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.381	67	319840	33.040	ng/ul	0.00
11) 2-Chlorophenol-d4	7.587	132	288932	24.833	ng/ul	0.00
15) 4-Methylphenol-d8	8.775	113	195388	15.571	ng/ul	0.00
21) Nitrobenzene-d5	9.240	128	201526	36.640	ng/ul	0.00
24) 2-Nitrophenol-d4	9.969	143	196098	39.916	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.510	165	328627	30.204	ng/ul	0.00
31) 4-Chloroaniline-d4	11.034	131	395980	21.430	ng/ul	0.00
46) Dimethylphthalate-d6	14.128	166	1269797	35.183	ng/ul	0.00
49) Acenaphthylene-d8	14.416	160	1424805	33.863	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	37185	5.178	ng/ul	0.00
60) Fluorene-d10	15.710	176	1109778	35.339	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.822	200	173069	39.892	ng/ul	0.00
73) Anthracene-d10	17.569	188	1834141	38.372	ng/ul	0.00
81) Pyrene-d10	19.863	212	2056300	45.436	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.004	264	1684556	43.198	ng/ul	-0.01
Target Compounds						
48) 2,6-Dinitrotoluene	14.134	165	6559	1.036	ng/ul#	Qvalue 34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
Data File : BN021613.D
Acq On : 06 Sep 2022 22:46
Operator : CG/JU
Sample : N4482-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW345


Quant Time: Sep 07 01:08:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 07 01:01:49 2022
Response via : Initial Calibration

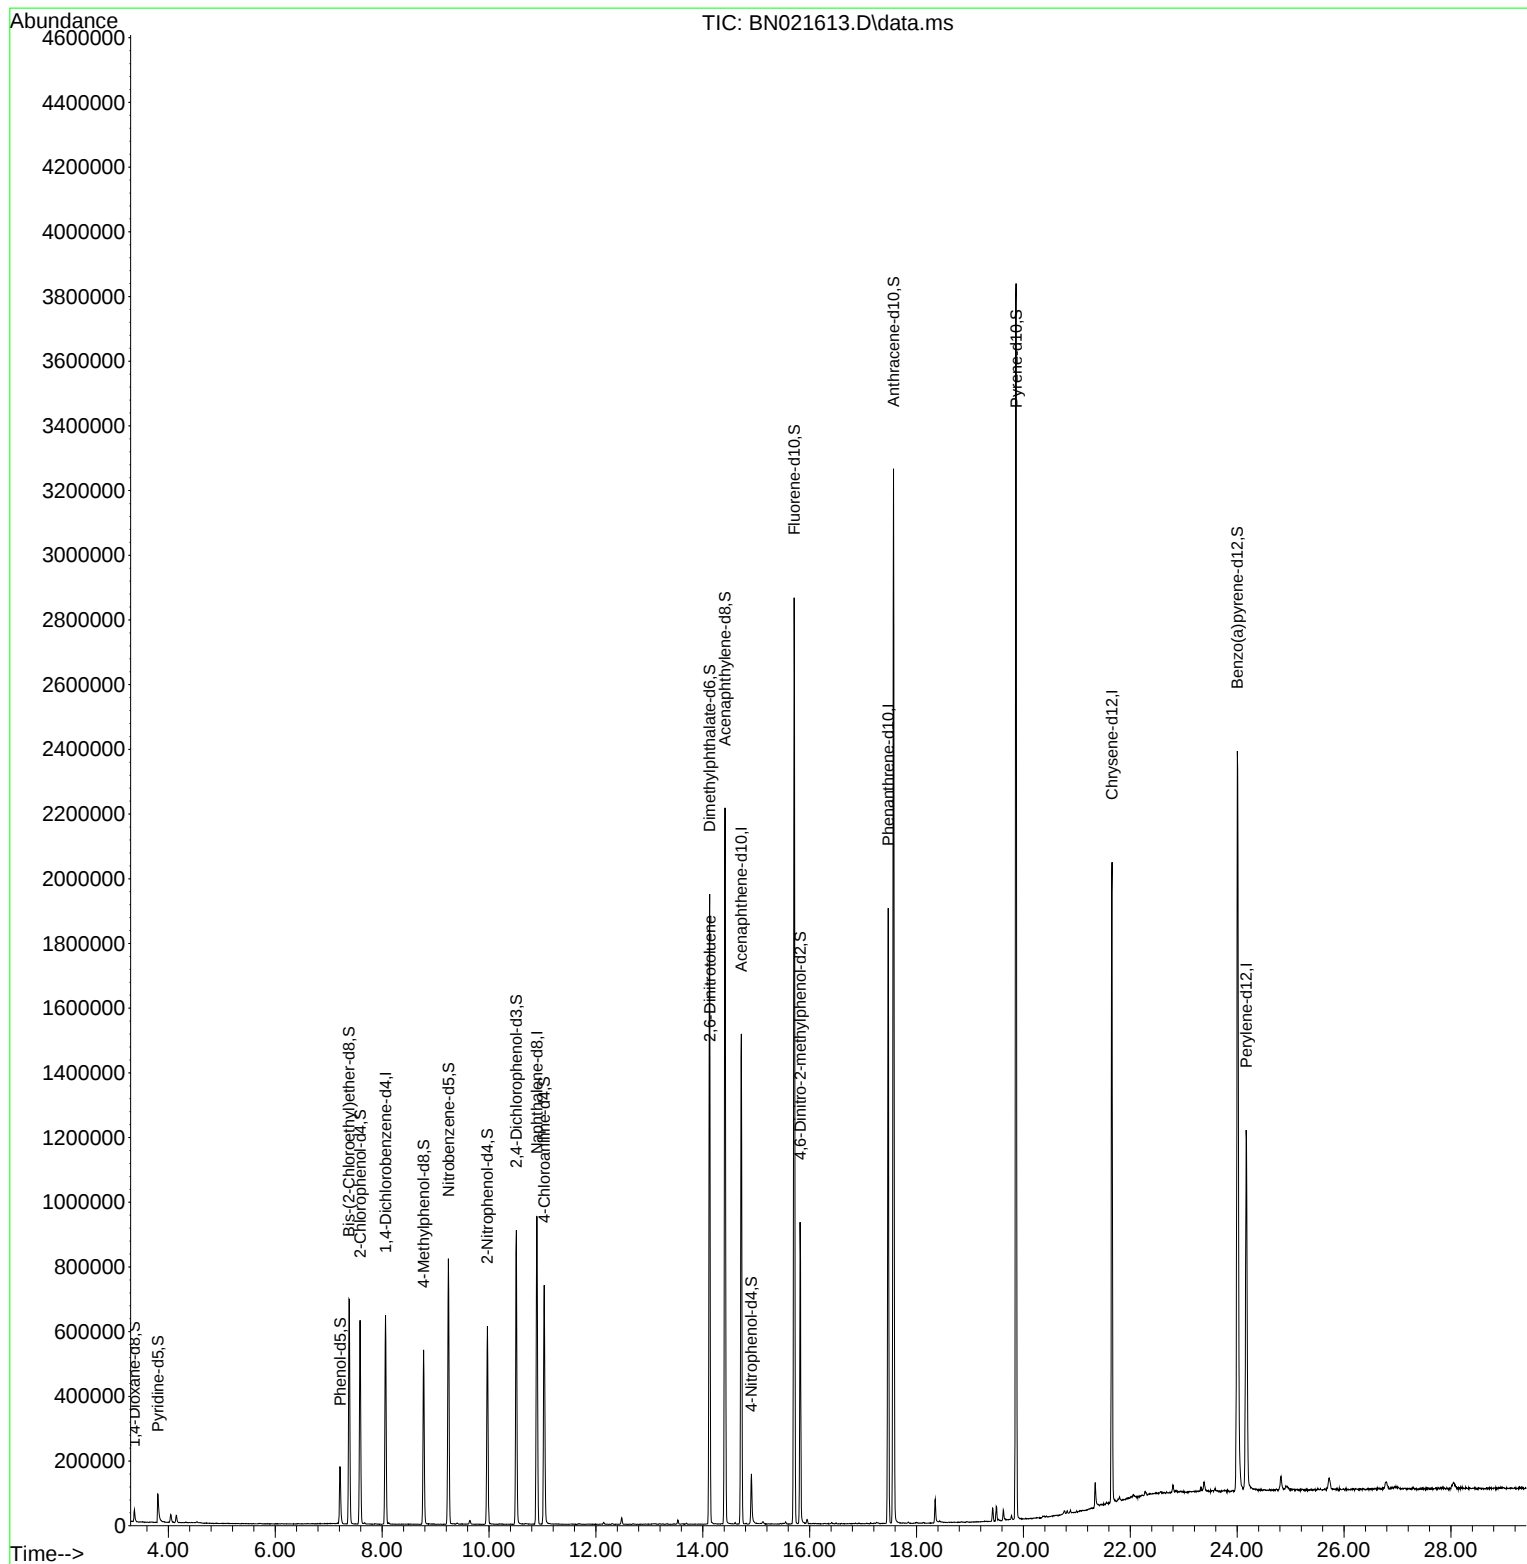

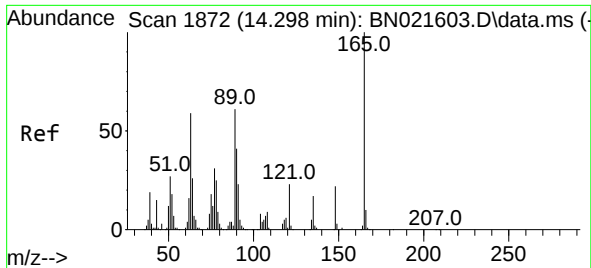

#48
 2,6-Dinitrotoluene
 Concen: 1.036 ng/ul
 RT: 14.134 min Scan# 11
 Delta R.T. -0.165 min
 Lab File: BN021613.D
 Acq: 06 Sep 2022 22:46

Instrument :
 BNA_N
 ClientSampleId :
 EW345

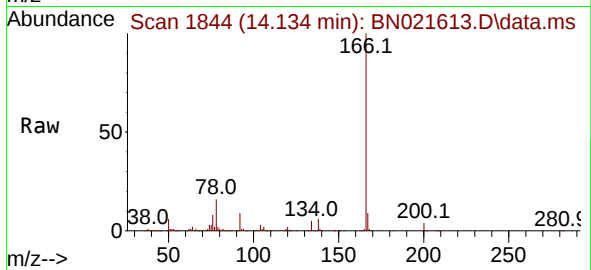

Tgt Ion:	165	Resp:	6559
Ion	Ratio	Lower	Upper
165	100		
89	0.0	50.6	75.8#
121	33.6	17.9	26.9#

