

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
 Data File : BN021615.D
 Acq On : 07 Sep 2022 00:01
 Operator : CG/JU
 Sample : N4484-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0KR3

Quant Time: Sep 07 01:09:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 07 01:01:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.063	152	171307	20.000	ng/ul	0.00
20) Naphthalene-d8	10.893	136	779527	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.722	164	515230	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.469	188	1045811	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.651	240	947309	20.000	ng/ul	#-0.01
88) Perylene-d12	24.169	264	831578	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	25004	5.480	ng/uL	0.00
4) Pyridine-d5	3.799	84	146485	11.780	ng/ul	0.00
7) Phenol-d5	7.211	99	121776	7.838	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.381	67	329656	35.052	ng/ul	0.00
11) 2-Chlorophenol-d4	7.587	132	319030	28.223	ng/ul	0.00
15) 4-Methylphenol-d8	8.775	113	224163	18.388	ng/ul	0.00
21) Nitrobenzene-d5	9.240	128	212785	40.065	ng/ul	0.00
24) 2-Nitrophenol-d4	9.969	143	213728	45.054	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.510	165	360268	34.292	ng/ul	0.00
31) 4-Chloroaniline-d4	11.034	131	412676	23.129	ng/ul	0.00
46) Dimethylphthalate-d6	14.128	166	1386624	39.375	ng/ul	0.00
49) Acenaphthylene-d8	14.416	160	1574535	38.352	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	46707	6.665	ng/ul	0.00
60) Fluorene-d10	15.710	176	1203463	39.274	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.822	200	197353	47.179	ng/ul	0.00
73) Anthracene-d10	17.569	188	1977503	42.908	ng/ul	0.00
81) Pyrene-d10	19.863	212	2172994	48.235	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.010	264	1776365	45.067	ng/ul	0.00
Target Compounds						
48) 2,6-Dinitrotoluene	14.128	165	7365	1.192	ng/ul#	Qvalue 31


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
Data File : BN021615.D
Acq On : 07 Sep 2022 00:01
Operator : CG/JU
Sample : N4484-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0KR3


Quant Time: Sep 07 01:09:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 07 01:01:49 2022
Response via : Initial Calibration

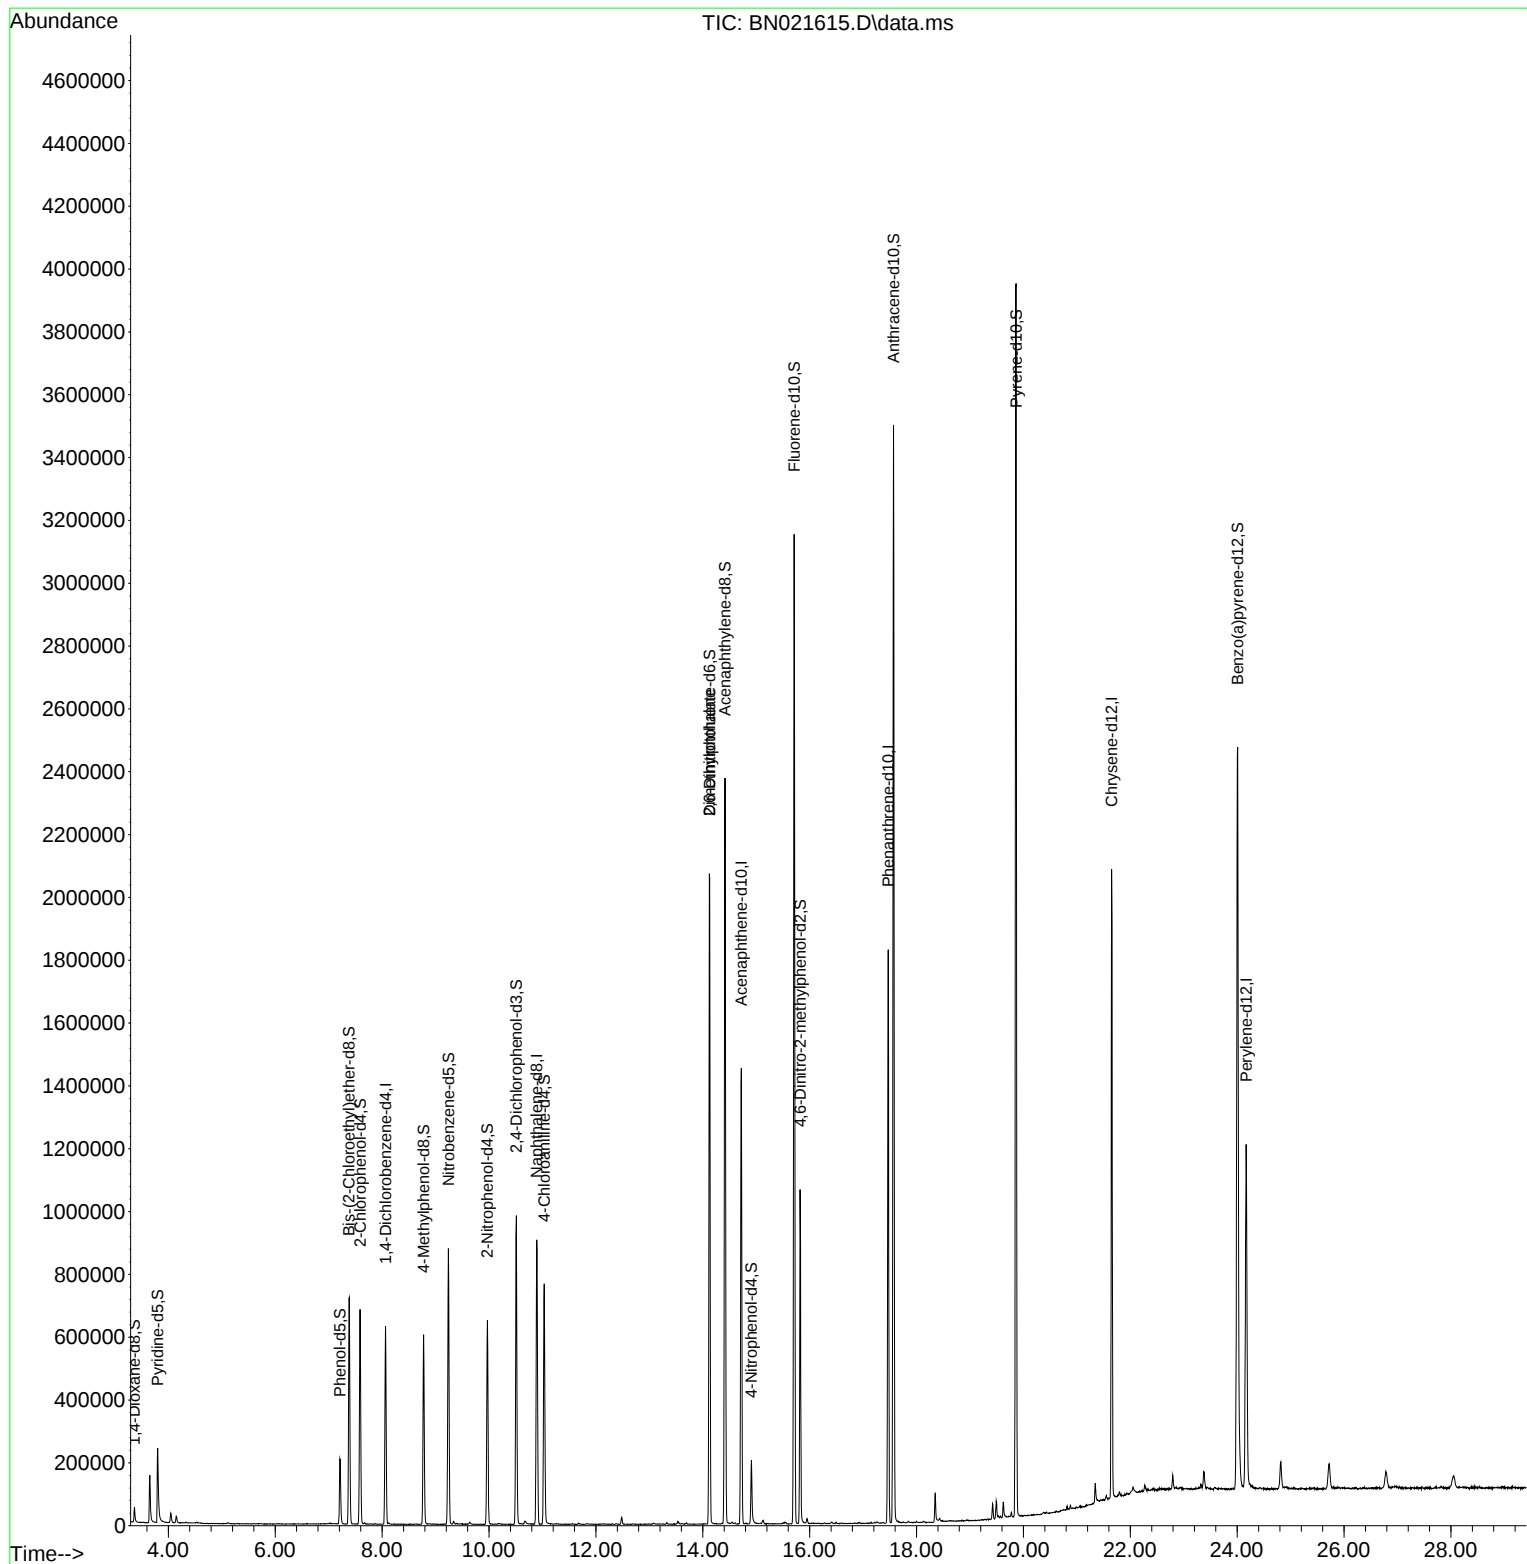

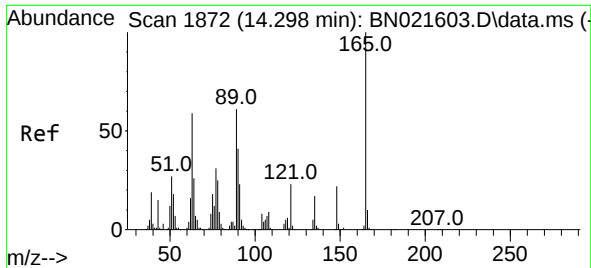

#48
 2,6-Dinitrotoluene
 Concen: 1.192 ng/ul
 RT: 14.128 min Scan# 11
 Delta R.T. -0.170 min
 Lab File: BN021615.D
 Acq: 07 Sep 2022 00:01

Instrument :
 BNA_N
 ClientSampleId :
 C0KR3

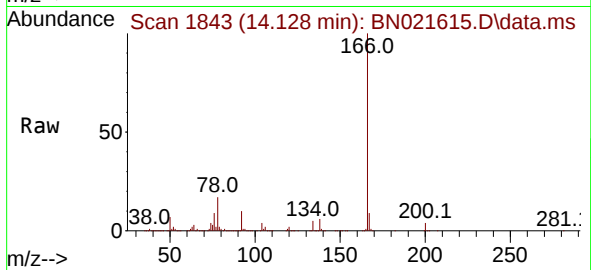

Tgt Ion	Ratio	Lower	Upper
165	100		
89	3.2	50.6	75.8#
121	43.8	17.9	26.9#

