

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
 Data File : BN021597.D
 Acq On : 06 Sep 2022 12:25
 Operator : CG/JU
 Sample : PB146656BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK656

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
 Title : SVOA CALIBRATION

Signal : TIC: BN021597.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	9	13	22	rVB	49760	70594	1.51%	0.147%
2	3.793	83	86	106	rBV	538192	893556	19.10%	1.856%
3	4.146	142	146	153	rVB	10662	17255	0.37%	0.036%
4	7.210	660	667	679	rVB	786924	1268048	27.10%	2.634%
5	7.381	690	696	706	rBV	650406	1074000	22.95%	2.231%
6	7.587	724	731	738	rBV	786236	1261370	26.96%	2.620%
7	8.063	805	812	819	rBV	568963	919214	19.64%	1.910%
8	8.775	926	933	945	rBV	1011653	1616649	34.55%	3.358%
9	9.240	1004	1012	1021	rBV	773749	1258039	26.89%	2.614%
10	9.334	1025	1028	1033	rVB5	3869	5591	0.12%	0.012%
11	9.969	1128	1136	1149	rVB	606312	986530	21.08%	2.049%
12	10.510	1220	1228	1238	rBV	962850	1614203	34.50%	3.353%
13	10.893	1286	1293	1302	rVB	847179	1453183	31.06%	3.019%
14	11.034	1309	1317	1331	rBV	1023436	1791522	38.29%	3.722%
15	12.140	1495	1505	1509	rBV7	2128	5443	0.12%	0.011%
16	12.481	1557	1563	1570	rVB2	17552	29090	0.62%	0.060%
17	13.692	1763	1769	1776	rBV9	3040	5810	0.12%	0.012%
18	14.128	1836	1843	1855	rBV	1736164	2509884	53.64%	5.214%
19	14.416	1884	1892	1904	rBV	2102146	3038478	64.93%	6.312%
20	14.722	1936	1944	1954	rBV	1328562	1985834	42.44%	4.125%
21	14.910	1969	1976	1996	rBV	827621	1193588	25.51%	2.480%
22	15.710	2105	2112	2119	rBV	2597024	3722895	79.56%	7.734%
23	15.822	2125	2131	2146	rVV	778742	1045477	22.34%	2.172%
24	15.951	2148	2153	2158	rVB	24790	35608	0.76%	0.074%
25	16.492	2239	2245	2252	rVB7	6693	9911	0.21%	0.021%
26	17.145	2351	2356	2359	rBV4	4116	4947	0.11%	0.010%
27	17.469	2405	2411	2419	rBV	1646942	2344670	50.11%	4.871%
28	17.569	2421	2428	2447	rVV2	2793325	4051405	86.58%	8.417%
29	18.133	2521	2524	2529	rVB6	7468	9781	0.21%	0.020%
30	19.427	2738	2744	2749	rBV	32013	47036	1.01%	0.098%
31	19.498	2750	2756	2762	rBV	32269	44302	0.95%	0.092%
32	19.863	2812	2818	2827	rBV	3407695	4679305	100.00%	9.721%
33	21.657	3118	3123	3135	rBV	1795981	2405544	51.41%	4.997%
34	23.392	3414	3418	3425	rVB2	33110	57551	1.23%	0.120%
35	24.010	3515	3523	3539	rBV2	2003782	4287609	91.63%	8.907%
36	24.174	3544	3551	3563	rVB2	1027511	2152116	45.99%	4.471%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
Data File : BN021597.D
Acq On : 06 Sep 2022 12:25
Operator : CG/JU
Sample : PB146656BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK656

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Title : SVOA CALIBRATION

37	24.827	3657	3662	3669	rVB2	53353	119007	2.54%	0.247%
38	25.727	3811	3815	3823	rVB3	54290	121116	2.59%	0.252%




Sum of corrected areas: 48136161

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
Data File : BN021597.D
Acq On : 06 Sep 2022 12:25
Operator : CG/JU
Sample : PB146656BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK656

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

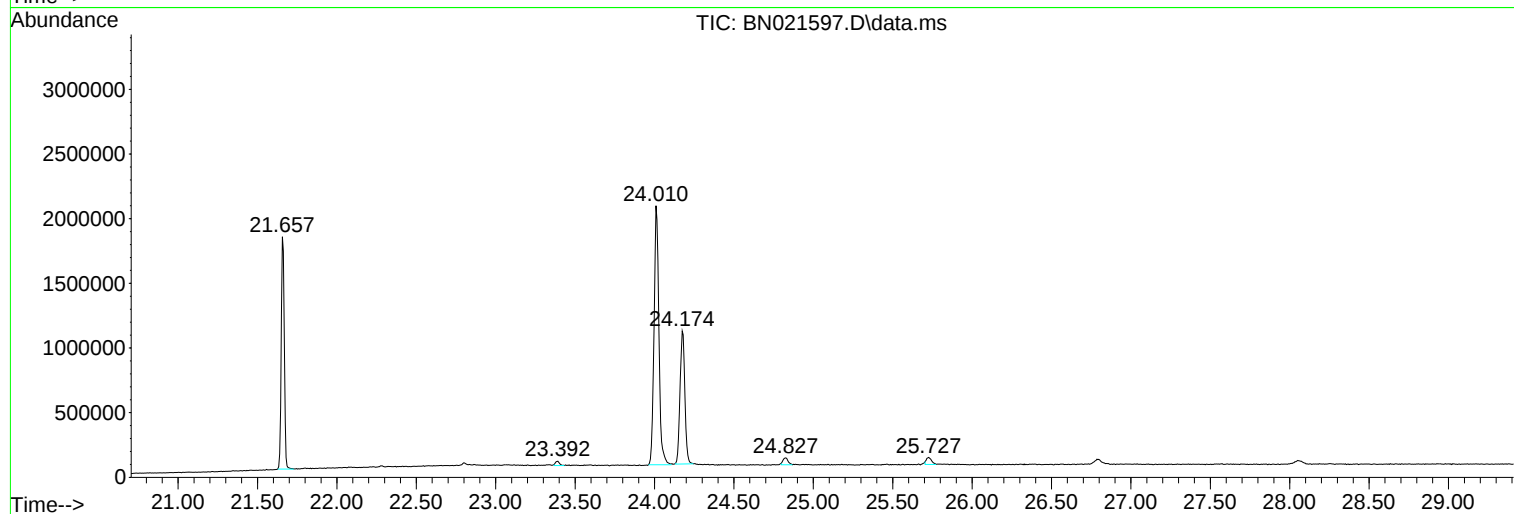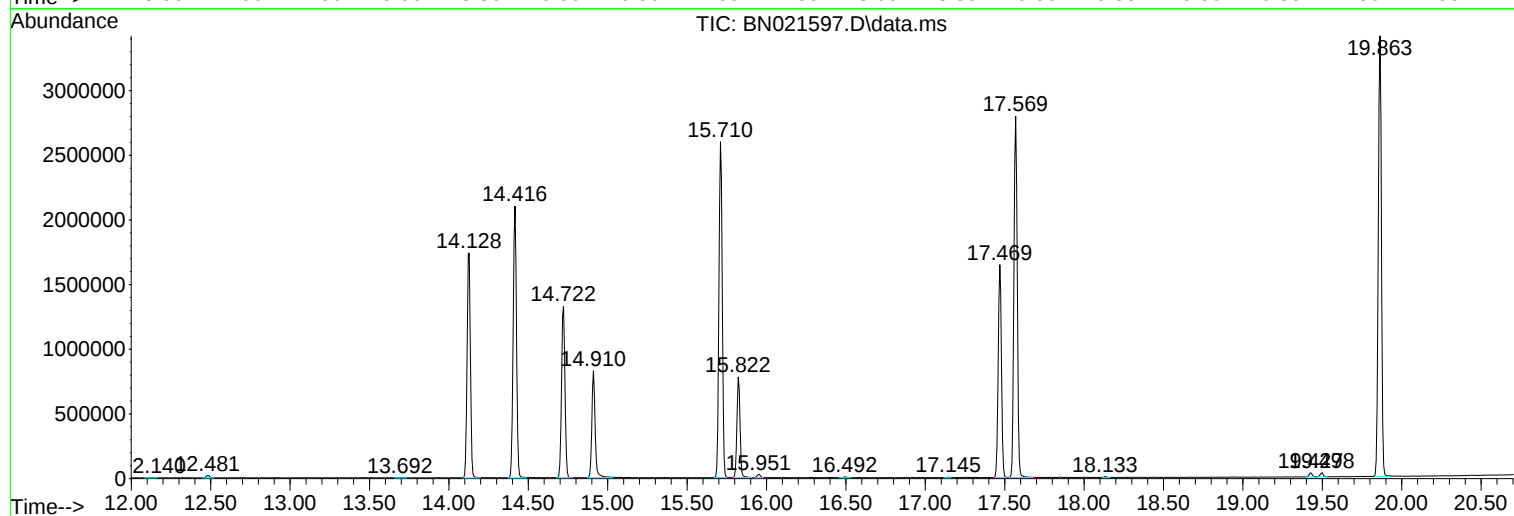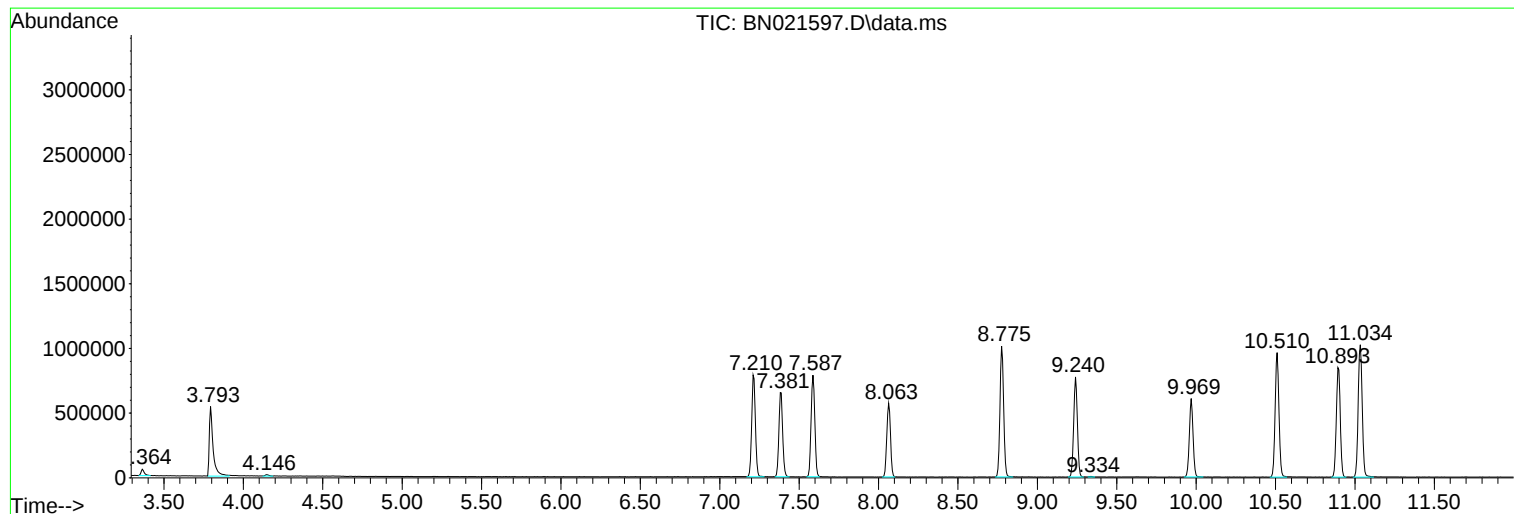

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
Data File : BN021597.D
Acq On : 06 Sep 2022 12:25
Operator : CG/JU
Sample : PB146656BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK656

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
Data File : BN021597.D
Acq On : 06 Sep 2022 12:25
Operator : CG/JU
Sample : PB146656BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK656

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
