

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
 Data File : BN021604.D
 Acq On : 06 Sep 2022 17:07
 Operator : CG/JU
 Sample : PB147443BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK443

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
 Title : SVOA CALIBRATION

Signal : TIC: BN021604.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	9	13	21	rVB	56267	78346	1.62%	0.148%
2	3.793	83	86	109	rBV	634506	1027338	21.27%	1.944%
3	4.146	142	146	154	rVB	14610	21847	0.45%	0.041%
4	7.210	661	667	676	rBV	882697	1388928	28.75%	2.628%
5	7.381	689	696	708	rVB	739572	1193449	24.71%	2.258%
6	7.587	723	731	743	rBV	869939	1382188	28.61%	2.615%
7	8.063	804	812	822	rVB	750165	1206855	24.98%	2.283%
8	8.775	925	933	950	rBV	1092095	1766426	36.57%	3.342%
9	9.240	1003	1012	1021	rBV	844462	1394277	28.86%	2.638%
10	9.334	1024	1028	1034	rVB5	3618	5823	0.12%	0.011%
11	9.969	1127	1136	1149	rBV	679965	1108575	22.95%	2.097%
12	10.510	1220	1228	1244	rBV	1059919	1781676	36.88%	3.371%
13	10.893	1284	1293	1303	rBV	1101960	1905244	39.44%	3.604%
14	11.034	1309	1317	1333	rBV	962478	1671523	34.60%	3.162%
15	12.481	1557	1563	1570	rVB	21413	34569	0.72%	0.065%
16	14.128	1836	1843	1852	rBV	1828090	2665049	55.17%	5.042%
17	14.416	1885	1892	1905	rBV	2237050	3316401	68.65%	6.274%
18	14.722	1937	1944	1952	rBV	1769443	2585896	53.53%	4.892%
19	14.910	1969	1976	1989	rBV	872299	1281675	26.53%	2.425%
20	15.128	2009	2013	2018	rVB5	3166	4943	0.10%	0.009%
21	15.710	2104	2112	2123	rBV	2765574	4012858	83.07%	7.592%
22	15.822	2125	2131	2140	rBV	828694	1107707	22.93%	2.096%
23	15.951	2148	2153	2158	rVB	13331	17576	0.36%	0.033%
24	17.257	2369	2375	2379	rBV2	4321	7201	0.15%	0.014%
25	17.469	2404	2411	2421	rVB	2125964	2978294	61.65%	5.634%
26	17.569	2421	2428	2441	rBV2	2941907	4281975	88.64%	8.101%
27	17.845	2473	2475	2481	rVB3	3847	4983	0.10%	0.009%
28	19.427	2739	2744	2749	rVB2	32946	44261	0.92%	0.084%
29	19.498	2750	2756	2762	rBV	34544	48856	1.01%	0.092%
30	19.863	2811	2818	2828	rBV2	3473547	4830640	100.00%	9.139%
31	21.657	3118	3123	3134	rBV2	2272286	2997558	62.05%	5.671%
32	24.015	3515	3524	3541	rBV2	1944327	4076967	84.40%	7.713%
33	24.180	3543	3552	3564	rBV	1284400	2628310	54.41%	4.972%




Sum of corrected areas: 52858214

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
Data File : BN021604.D
Acq On : 06 Sep 2022 17:07
Operator : CG/JU
Sample : PB147443BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK443

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

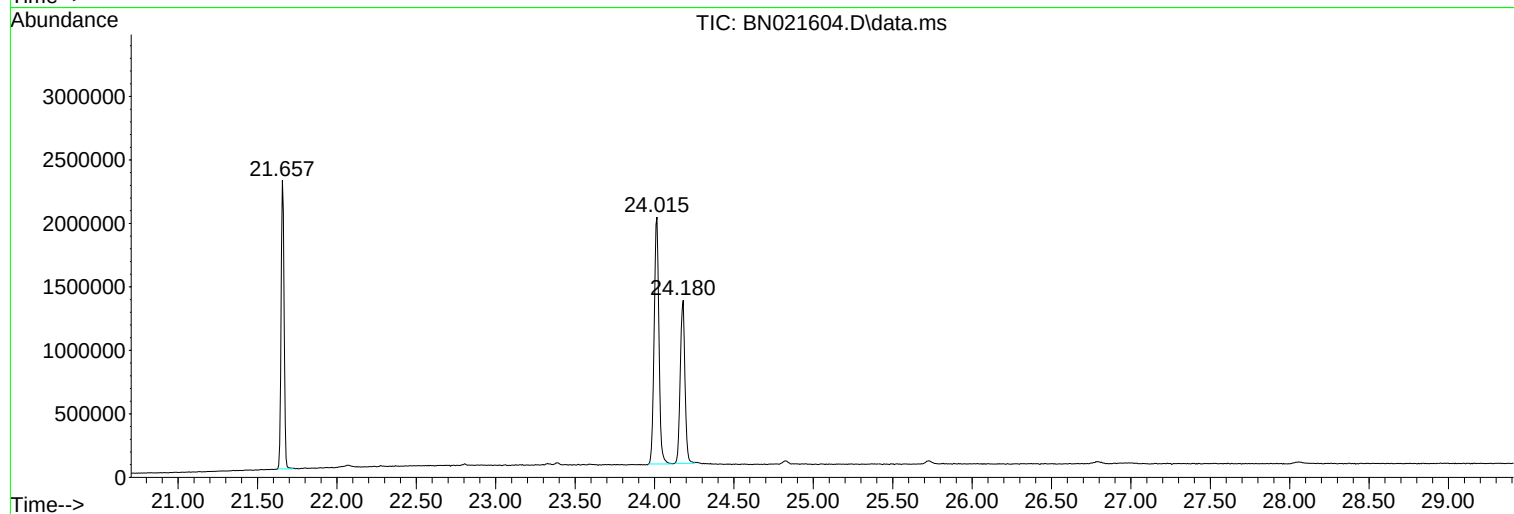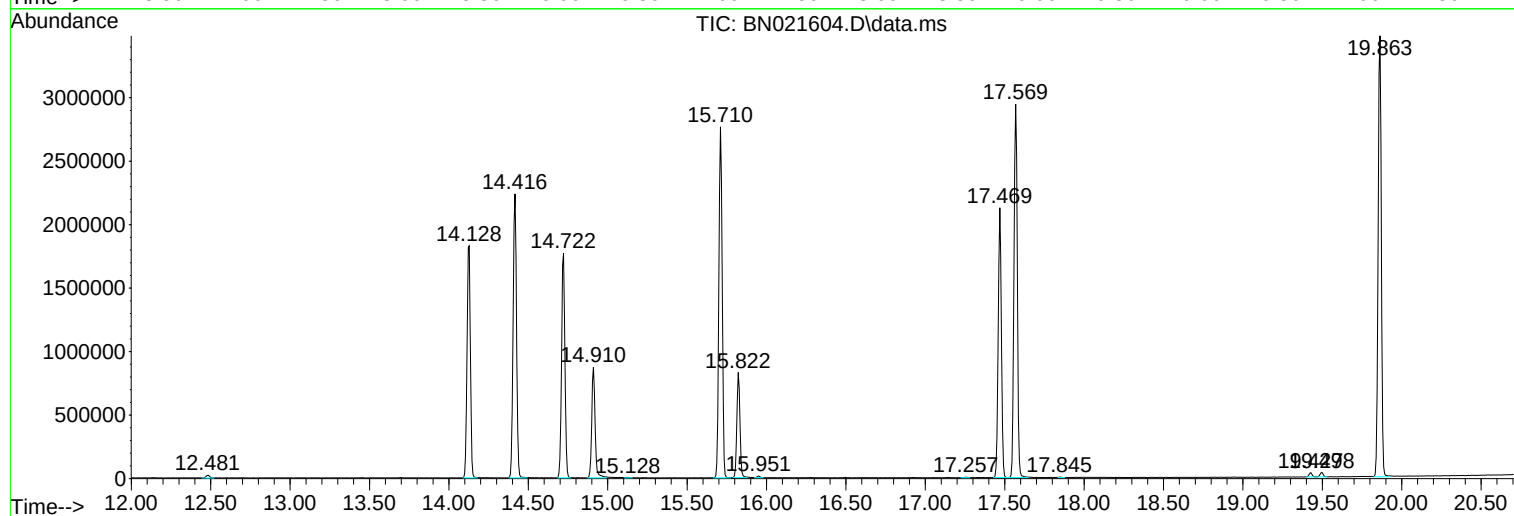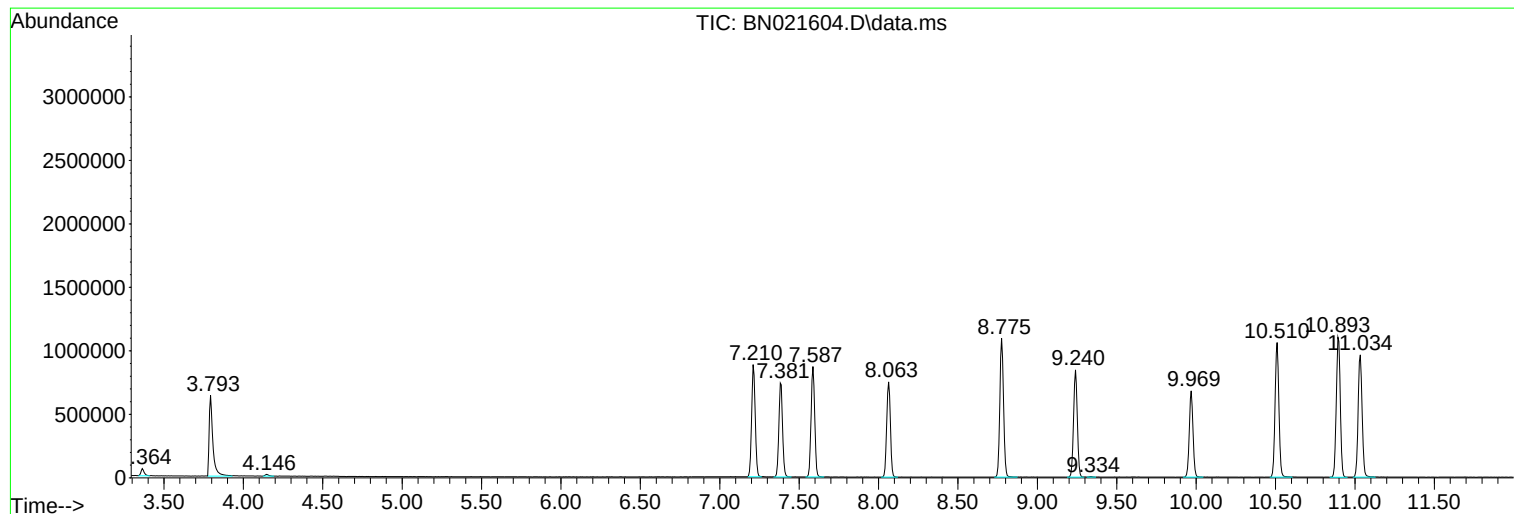

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
Data File : BN021604.D
Acq On : 06 Sep 2022 17:07
Operator : CG/JU
Sample : PB147443BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK443

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
Data File : BN021604.D
Acq On : 06 Sep 2022 17:07
Operator : CG/JU
Sample : PB147443BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK443

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc