

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
 Data File : BN021606.D
 Acq On : 06 Sep 2022 18:22
 Operator : CG/JU
 Sample : N4482-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW366

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
 Title : SVOA CALIBRATION

Signal : TIC: BN021606.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	9	13	20	rBV	44934	60810	1.13%	0.125%
2	3.799	84	87	106	rBV	172940	288418	5.36%	0.591%
3	4.046	124	129	138	rVB	29210	49785	0.92%	0.102%
4	4.146	142	146	153	rBV	19927	30573	0.57%	0.063%
5	7.210	661	667	677	rVB	190217	327273	6.08%	0.671%
6	7.387	689	697	706	rBV	709163	1152115	21.40%	2.361%
7	7.587	723	731	739	rBV	647473	1014480	18.84%	2.079%
8	7.669	742	745	752	rVB6	3892	7478	0.14%	0.015%
9	8.063	805	812	819	rBV	633239	1010273	18.76%	2.070%
10	8.122	819	822	829	rVB3	7179	11732	0.22%	0.024%
11	8.775	925	933	944	rBV	552198	886083	16.46%	1.816%
12	9.240	1005	1012	1024	rBV	826574	1355276	25.17%	2.777%
13	9.340	1025	1029	1033	rVB6	3590	5437	0.10%	0.011%
14	9.404	1035	1040	1045	rBV6	5159	8943	0.17%	0.018%
15	9.645	1073	1081	1089	rVB2	14518	27114	0.50%	0.056%
16	9.969	1128	1136	1152	rVB	599853	974217	18.09%	1.996%
17	10.198	1168	1175	1176	rBV5	2991	5453	0.10%	0.011%
18	10.510	1221	1228	1243	rBV	920509	1523373	28.29%	3.122%
19	10.669	1250	1255	1262	rBV3	11422	24334	0.45%	0.050%
20	10.898	1286	1294	1301	rBV	907794	1577718	29.30%	3.233%
21	11.034	1309	1317	1333	rBV	789681	1355035	25.17%	2.777%
22	12.139	1499	1505	1512	rVB4	4300	9461	0.18%	0.019%
23	12.310	1529	1534	1539	rVB3	5974	9529	0.18%	0.020%
24	12.481	1558	1563	1570	rVB2	19306	31341	0.58%	0.064%
25	13.104	1667	1669	1675	rVB5	3673	5953	0.11%	0.012%
26	13.533	1736	1742	1750	rVB	22295	35219	0.65%	0.072%
27	13.692	1764	1769	1775	rVB5	2863	5936	0.11%	0.012%
28	14.128	1835	1843	1849	rBV	1910990	2734877	50.79%	5.605%
29	14.416	1885	1892	1902	rVV2	2226410	3278347	60.88%	6.718%
30	14.604	1918	1924	1929	rVB5	5239	8844	0.16%	0.018%
31	14.722	1936	1944	1954	rBV	1468764	2197931	40.82%	4.504%
32	14.910	1966	1976	1992	rBV	158314	269904	5.01%	0.553%
33	15.127	2007	2013	2017	rVB5	8353	16418	0.30%	0.034%
34	15.551	2082	2085	2091	rVB3	9671	13223	0.25%	0.027%
35	15.710	2101	2112	2125	rBV	2839856	4247831	78.89%	8.705%
36	15.822	2125	2131	2147	rVV	888423	1216320	22.59%	2.493%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
 Data File : BN021606.D
 Acq On : 06 Sep 2022 18:22
 Operator : CG/JU
 Sample : N4482-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW366

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
 Title : SVOA CALIBRATION

37	15.951	2147	2153	2157	rVB2	14584	22035	0.41%	0.045%
38	16.163	2185	2189	2194	rVB7	4060	6686	0.12%	0.014%
39	16.416	2228	2232	2240	rVB7	4423	10018	0.19%	0.021%
40	16.492	2240	2245	2250	rBV8	4154	7706	0.14%	0.016%
41	17.469	2404	2411	2421	rBV	1836601	2545081	47.27%	5.216%
42	17.569	2421	2428	2440	rVV2	3328100	4808510	89.30%	9.854%
43	17.657	2440	2443	2453	rVB8	9351	18011	0.33%	0.037%
44	18.004	2497	2502	2506	rBV4	3958	6625	0.12%	0.014%
45	18.127	2520	2523	2527	rVB3	5108	7253	0.13%	0.015%
46	18.351	2556	2561	2569	rBV	125219	179452	3.33%	0.368%
47	18.427	2572	2574	2581	rVB4	5761	9582	0.18%	0.020%
48	19.427	2739	2744	2750	rBV2	41642	58823	1.09%	0.121%
49	19.498	2750	2756	2761	rBV	49428	76947	1.43%	0.158%
50	19.627	2773	2778	2788	rBV	66236	99776	1.85%	0.204%
51	19.780	2800	2804	2810	rBV5	9692	15406	0.29%	0.032%
52	19.863	2811	2818	2832	rVV	3832593	5384520	100.00%	11.034%
53	20.610	2943	2945	2951	rBV6	4535	7161	0.13%	0.015%
54	20.821	2978	2981	2986	rBV6	11134	18493	0.34%	0.038%
55	20.880	2988	2991	2996	rVV4	12061	17690	0.33%	0.036%
56	21.351	3066	3071	3082	rBV	123359	219784	4.08%	0.450%
57	21.657	3118	3123	3133	rBV	1845262	2530697	47.00%	5.186%
58	22.804	3315	3318	3325	rVB2	29004	39954	0.74%	0.082%
59	24.015	3515	3524	3541	rBV2	2223213	4741025	88.05%	9.716%
60	24.180	3544	3552	3564	rVB2	1004344	2189377	40.66%	4.487%




Sum of corrected areas: 48797666

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
Data File : BN021606.D
Acq On : 06 Sep 2022 18:22
Operator : CG/JU
Sample : N4482-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW366

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

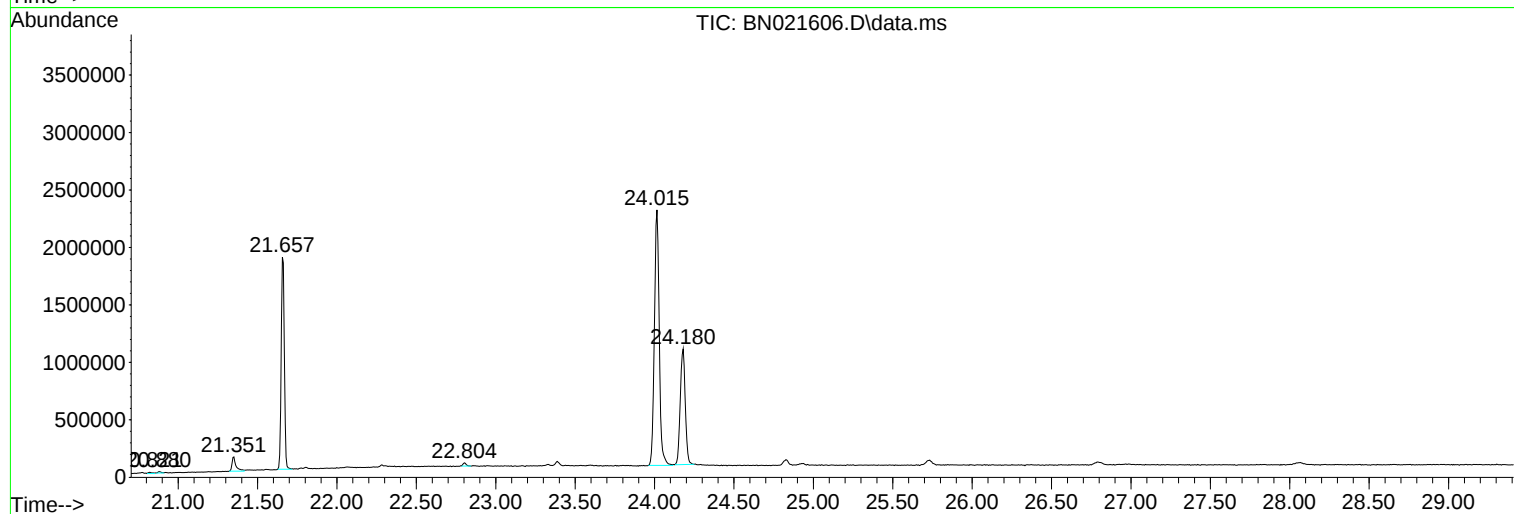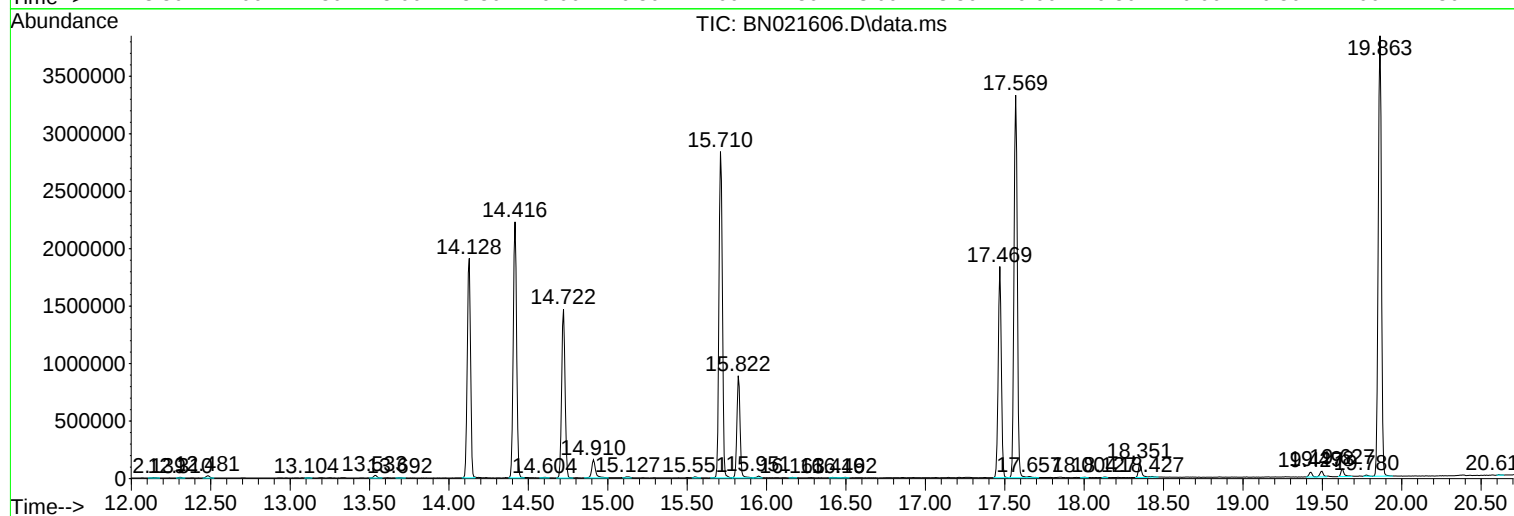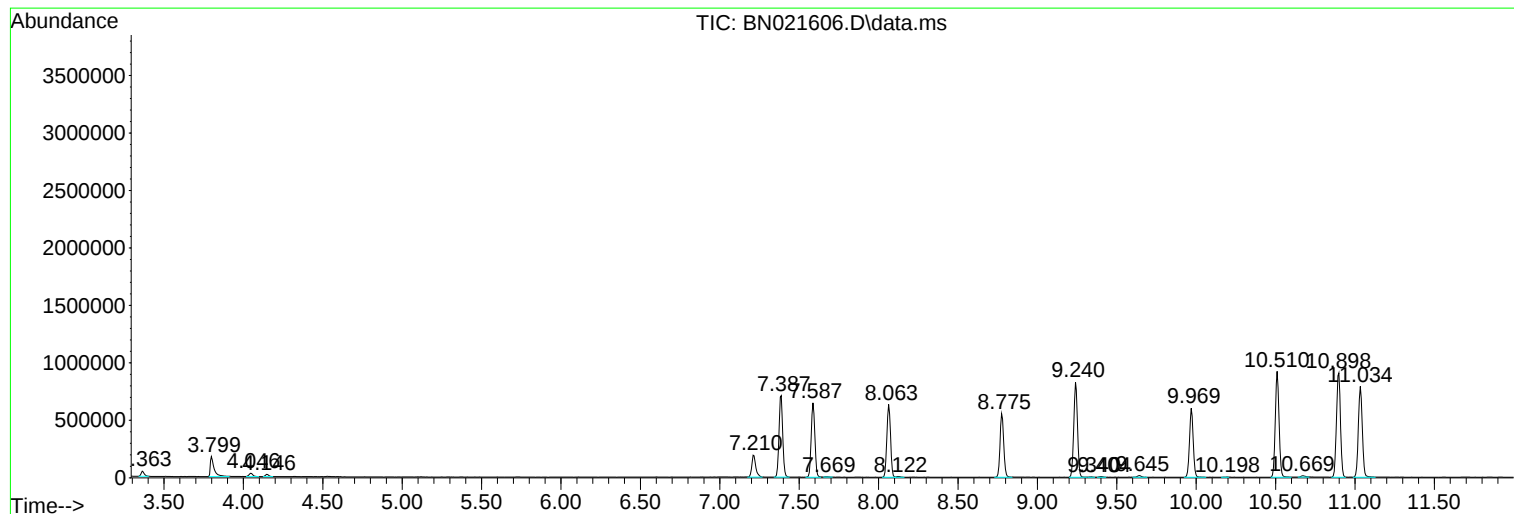

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
Data File : BN021606.D
Acq On : 06 Sep 2022 18:22
Operator : CG/JU
Sample : N4482-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW366

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
Data File : BN021606.D
Acq On : 06 Sep 2022 18:22
Operator : CG/JU
Sample : N4482-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW366

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
