

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
 Data File : BN021609.D
 Acq On : 06 Sep 2022 20:15
 Operator : CG/JU
 Sample : N4482-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW349

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
 Title : SVOA CALIBRATION

Signal : TIC: BN021609.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	9	13	19	rBV	39417	55016	0.99%	0.106%
2	3.411	19	21	26	rVB5	5376	6690	0.12%	0.013%
3	3.799	84	87	101	rBV	174721	291446	5.26%	0.560%
4	4.046	124	129	135	rBV	26709	42478	0.77%	0.082%
5	4.146	142	146	153	rBV	20089	31084	0.56%	0.060%
6	4.269	161	167	173	rBV	20917	33467	0.60%	0.064%
7	4.311	173	174	183	rVB6	3183	5891	0.11%	0.011%
8	5.516	375	379	383	rBV4	3951	6011	0.11%	0.012%
9	7.211	661	667	674	rBV	196482	316816	5.72%	0.609%
10	7.387	686	697	709	rBV	670620	1108299	20.00%	2.131%
11	7.587	723	731	741	rBV	643054	1023306	18.47%	1.967%
12	7.675	741	746	756	rVB6	4526	8970	0.16%	0.017%
13	8.063	803	812	821	rBV	710884	1145815	20.68%	2.203%
14	8.775	925	933	948	rBV	565158	921482	16.63%	1.771%
15	8.899	948	954	963	rVB	6370	12616	0.23%	0.024%
16	9.240	1004	1012	1022	rBV	794373	1319238	23.81%	2.536%
17	9.334	1024	1028	1036	rVB7	4073	9025	0.16%	0.017%
18	9.640	1075	1080	1087	rVB	5537	10554	0.19%	0.020%
19	9.969	1127	1136	1146	rBV	601874	996535	17.99%	1.916%
20	10.510	1219	1228	1240	rBV	919945	1549603	27.97%	2.979%
21	10.899	1286	1294	1304	rBV	1056405	1819060	32.83%	3.497%
22	11.034	1309	1317	1333	rBV	806441	1404891	25.36%	2.701%
23	11.557	1398	1406	1414	rVB	13260	26377	0.48%	0.051%
24	11.681	1421	1427	1433	rBV5	3359	7079	0.13%	0.014%
25	12.146	1500	1506	1511	rBV2	11699	18465	0.33%	0.035%
26	12.210	1511	1517	1526	rVB5	16839	37666	0.68%	0.072%
27	12.381	1542	1546	1554	rBV7	3112	8388	0.15%	0.016%
28	12.481	1557	1563	1569	rVB2	20110	33659	0.61%	0.065%
29	12.675	1591	1596	1603	rBV8	4825	10635	0.19%	0.020%
30	13.075	1659	1664	1668	rBV3	5524	8769	0.16%	0.017%
31	13.257	1688	1695	1702	rBV	24501	38467	0.69%	0.074%
32	13.328	1702	1707	1712	rBV4	8830	13888	0.25%	0.027%
33	13.628	1749	1758	1763	rBV	58704	90030	1.62%	0.173%
34	13.693	1765	1769	1774	rVB4	3617	5712	0.10%	0.011%
35	14.128	1835	1843	1849	rBV	1959973	2802657	50.58%	5.388%
36	14.169	1849	1850	1858	rVB2	10950	13570	0.24%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
 Data File : BN021609.D
 Acq On : 06 Sep 2022 20:15
 Operator : CG/JU
 Sample : N4482-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW349

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
 Title : SVOA CALIBRATION

37	14.357	1877	1882	1885	rBV3	4487	7256	0.13%	0.014%
38	14.416	1885	1892	1900	rBV2	2175160	3237549	58.43%	6.224%
39	14.681	1932	1937	1938	rBV4	9578	12733	0.23%	0.024%
40	14.722	1938	1944	1954	rVB	1673288	2528794	45.64%	4.861%
41	14.910	1970	1976	1988	rBV	191978	305935	5.52%	0.588%
42	15.016	1991	1994	1997	rVB4	6512	8605	0.16%	0.017%
43	15.128	2008	2013	2019	rVB5	8067	15400	0.28%	0.030%
44	15.369	2046	2054	2058	rBV5	11492	18275	0.33%	0.035%
45	15.451	2063	2068	2072	rVV	21163	30864	0.56%	0.059%
46	15.504	2073	2077	2078	rVV2	5801	6811	0.12%	0.013%
47	15.528	2078	2081	2086	rVB	21004	27428	0.50%	0.053%
48	15.710	2105	2112	2119	rBV	2955419	4231314	76.37%	8.134%
49	15.757	2119	2120	2125	rVB5	10060	7064	0.13%	0.014%
50	15.822	2125	2131	2143	rBV	960946	1290437	23.29%	2.481%
51	15.951	2147	2153	2162	rVB3	15182	27858	0.50%	0.054%
52	16.410	2222	2231	2238	rBV7	8436	19266	0.35%	0.037%
53	16.598	2259	2263	2268	rBV8	3883	5701	0.10%	0.011%
54	17.098	2345	2348	2351	rBV4	4757	6459	0.12%	0.012%
55	17.263	2371	2376	2380	rBV2	8647	13779	0.25%	0.026%
56	17.416	2398	2402	2405	rBV2	11244	14925	0.27%	0.029%
57	17.469	2405	2411	2417	rVV	2024754	3009508	54.32%	5.785%
58	17.569	2421	2428	2437	rVV2	3286849	4861186	87.74%	9.345%
59	17.745	2454	2458	2462	rBV2	14489	18675	0.34%	0.036%
60	17.939	2487	2491	2498	rBV10	3497	7625	0.14%	0.015%
61	18.328	2551	2557	2559	rBV	45728	69481	1.25%	0.134%
62	18.345	2559	2560	2563	rVV	38746	41784	0.75%	0.080%
63	18.386	2563	2567	2571	rVV	71050	98968	1.79%	0.190%
64	18.428	2571	2574	2581	rVB	49570	65160	1.18%	0.125%
65	18.616	2602	2606	2609	rBV2	10716	13364	0.24%	0.026%
66	18.657	2609	2613	2617	rVB5	11437	15418	0.28%	0.030%
67	18.869	2645	2649	2654	rBV	34657	46252	0.83%	0.089%
68	18.963	2659	2665	2669	rVB8	7846	13880	0.25%	0.027%
69	19.092	2683	2687	2690	rBV6	4379	5890	0.11%	0.011%
70	19.151	2694	2697	2699	rBV4	7793	7549	0.14%	0.015%
71	19.428	2739	2744	2750	rVB2	43587	62092	1.12%	0.119%
72	19.492	2750	2755	2760	rBV	48374	69569	1.26%	0.134%
73	19.622	2774	2777	2782	rBV3	20640	27181	0.49%	0.052%
74	19.775	2800	2803	2809	rVB6	12175	13429	0.24%	0.026%
75	19.863	2811	2818	2827	rBV	3872262	5540656	100.00%	10.651%
76	19.986	2837	2839	2843	rVB4	6746	5588	0.10%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
 Data File : BN021609.D
 Acq On : 06 Sep 2022 20:15
 Operator : CG/JU
 Sample : N4482-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW349

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
 Title : SVOA CALIBRATION

77	20.027	2843	2846	2849	rVB5	8247	8664	0.16%	0.017%
78	20.775	2971	2973	2977	rVB	14107	16185	0.29%	0.031%
79	21.657	3117	3123	3130	rBV	2404885	3123359	56.37%	6.004%
80	24.016	3515	3524	3538	rBV2	2283195	4973516	89.76%	9.561%
81	24.174	3543	3551	3564	rBV	1314433	2747360	49.59%	5.282%
82	24.827	3658	3662	3672	rVB4	51585	105950	1.91%	0.204%




Sum of corrected areas: 52018397

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
Data File : BN021609.D
Acq On : 06 Sep 2022 20:15
Operator : CG/JU
Sample : N4482-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW349

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

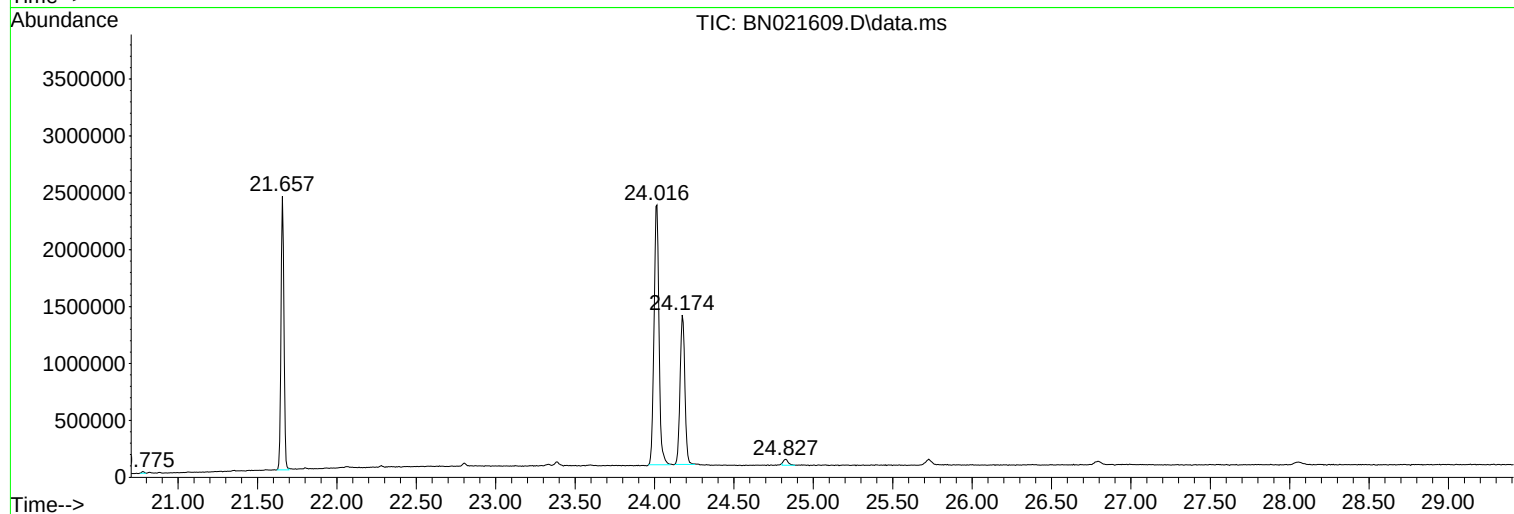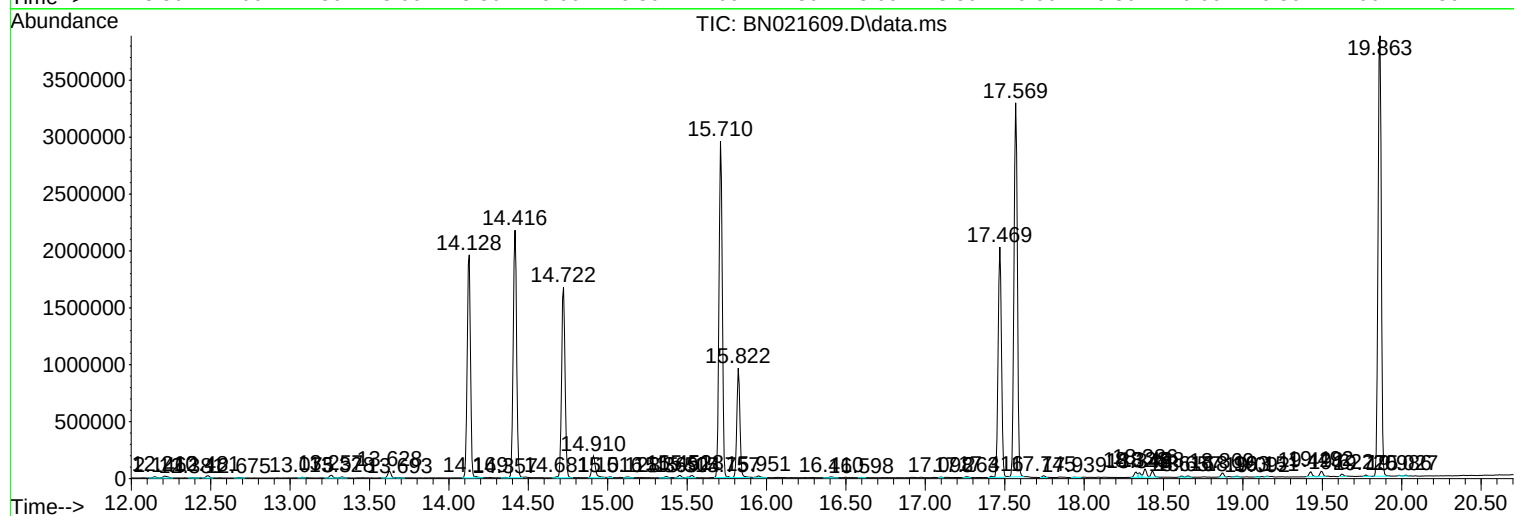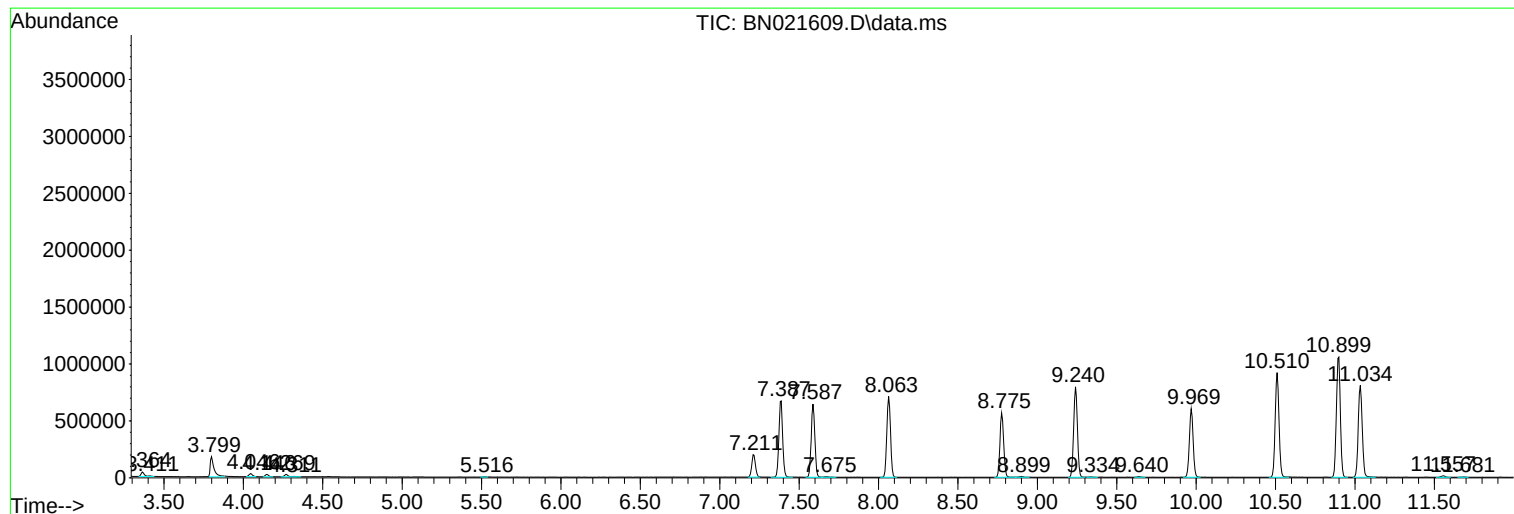

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
Data File : BN021609.D
Acq On : 06 Sep 2022 20:15
Operator : CG/JU
Sample : N4482-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW349

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
Data File : BN021609.D
Acq On : 06 Sep 2022 20:15
Operator : CG/JU
Sample : N4482-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW349

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc