

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
 Data File : BN021613.D
 Acq On : 06 Sep 2022 22:46
 Operator : CG/JU
 Sample : N4482-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW345

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
 Title : SVOA CALIBRATION

Signal : TIC: BN021613.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	9	13	20	rVB	37755	53450	0.97%	0.109%
2	3.799	85	87	103	rBV	88877	165901	3.02%	0.338%
3	4.046	124	129	135	rBV2	24327	41116	0.75%	0.084%
4	4.146	141	146	154	rBV	22532	35984	0.65%	0.073%
5	7.210	661	667	680	rVB	177408	297154	5.40%	0.606%
6	7.381	690	696	706	rBV	695157	1137152	20.68%	2.320%
7	7.587	724	731	741	rBV	629743	999989	18.18%	2.040%
8	7.669	741	745	752	rVB5	4167	7754	0.14%	0.016%
9	8.063	804	812	819	rBV	646577	1041779	18.94%	2.125%
10	8.775	926	933	945	rBV	539316	845524	15.37%	1.725%
11	9.240	1004	1012	1021	rBV	820900	1349264	24.53%	2.752%
12	9.404	1035	1040	1046	rVB6	3823	7648	0.14%	0.016%
13	9.640	1075	1080	1087	rVB	11512	18852	0.34%	0.038%
14	9.969	1126	1136	1149	rBV	612500	1004015	18.26%	2.048%
15	10.510	1220	1228	1245	rBV	909752	1539592	27.99%	3.140%
16	10.893	1286	1293	1303	rVB	951065	1648692	29.98%	3.363%
17	11.034	1309	1317	1331	rBV	739142	1262697	22.96%	2.576%
18	12.146	1502	1506	1514	rVB2	5968	9142	0.17%	0.019%
19	12.481	1556	1563	1569	rBV2	20201	31438	0.57%	0.064%
20	13.534	1736	1742	1747	rBV2	13125	18687	0.34%	0.038%
21	14.128	1836	1843	1857	rBV	1947241	2740138	49.82%	5.589%
22	14.416	1885	1892	1908	rVV2	2213853	3292826	59.87%	6.717%
23	14.604	1920	1924	1929	rVB4	4698	5513	0.10%	0.011%
24	14.722	1937	1944	1952	rBV	1514675	2279828	41.45%	4.650%
25	14.910	1967	1976	1990	rBV	155096	254276	4.62%	0.519%
26	15.122	2007	2012	2018	rVB9	6509	12104	0.22%	0.025%
27	15.551	2081	2085	2091	rVB	6744	9966	0.18%	0.020%
28	15.710	2101	2112	2120	rBV	2863504	4193362	76.25%	8.554%
29	15.822	2125	2131	2145	rVV	932988	1271315	23.12%	2.593%
30	15.951	2149	2153	2157	rVB	13676	20981	0.38%	0.043%
31	16.410	2225	2231	2235	rBV5	4186	7223	0.13%	0.015%
32	17.251	2371	2374	2383	rVB3	3777	7914	0.14%	0.016%
33	17.469	2404	2411	2421	rBV	1901569	2685640	48.83%	5.478%
34	17.569	2421	2428	2443	rBV2	3258975	4874848	88.64%	9.944%
35	18.351	2556	2561	2570	rBV	74164	108848	1.98%	0.222%
36	19.422	2739	2743	2748	rBV2	41691	57499	1.05%	0.117%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
 Data File : BN021613.D
 Acq On : 06 Sep 2022 22:46
 Operator : CG/JU
 Sample : N4482-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW345

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
 Title : SVOA CALIBRATION

37	19.492	2748	2755	2760	rBV	46204	70702	1.29%	0.144%
38	19.533	2760	2762	2766	rVB5	4797	5829	0.11%	0.012%
39	19.622	2773	2777	2782	rBV	32611	43908	0.80%	0.090%
40	19.775	2800	2803	2808	rVB3	12482	14093	0.26%	0.029%
41	19.863	2811	2818	2829	rVV	3819810	5499599	100.00%	11.218%
42	21.345	3066	3070	3079	rBV2	76486	124671	2.27%	0.254%
43	21.657	3117	3123	3132	rBV	1978506	2711063	49.30%	5.530%
44	24.004	3514	3522	3539	rBV2	2283056	4852450	88.23%	9.898%
45	24.168	3543	3550	3564	rVB2	1106695	2364594	43.00%	4.823%




Sum of corrected areas: 49025020

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
Data File : BN021613.D
Acq On : 06 Sep 2022 22:46
Operator : CG/JU
Sample : N4482-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW345

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

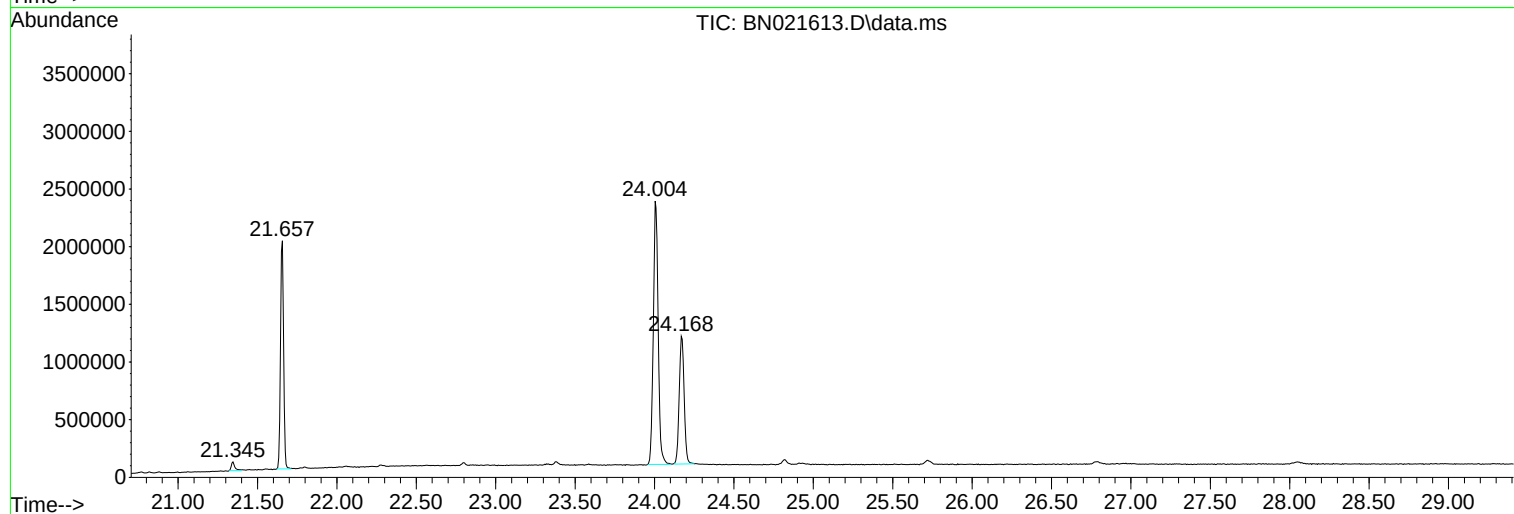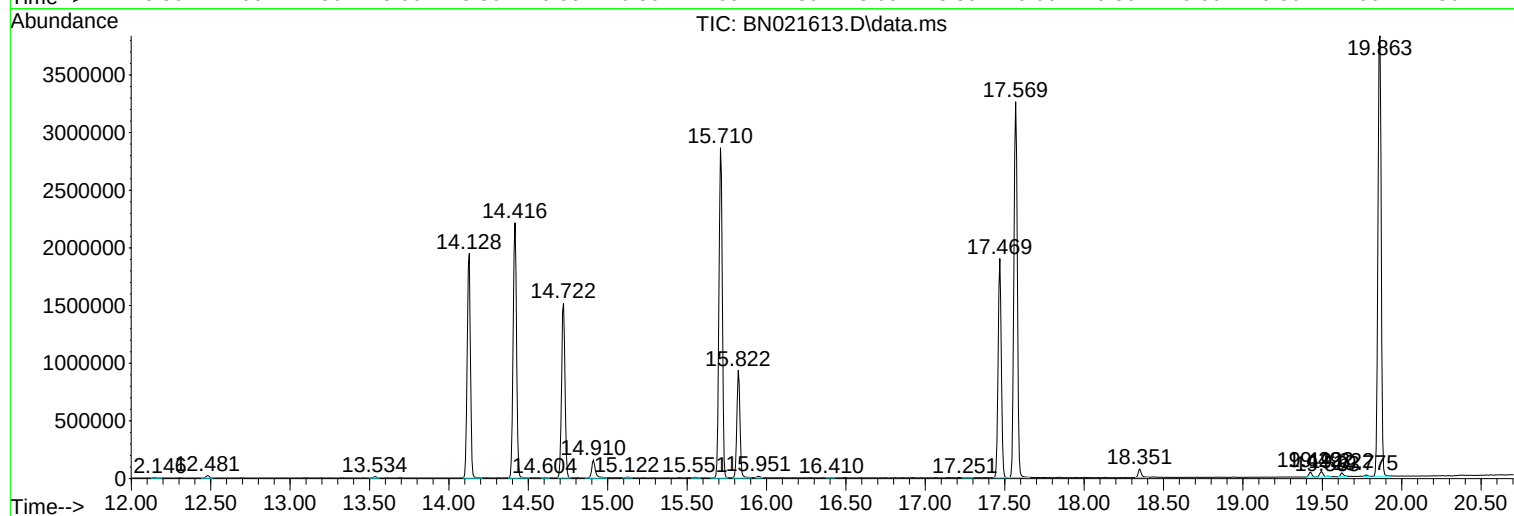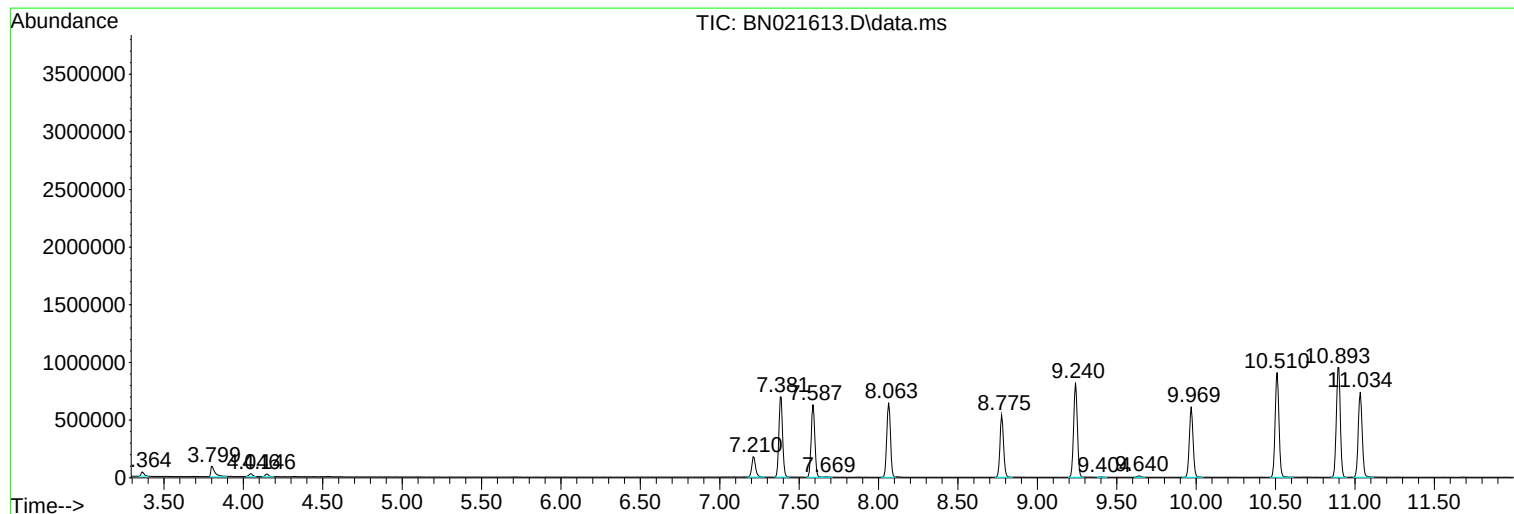

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
Data File : BN021613.D
Acq On : 06 Sep 2022 22:46
Operator : CG/JU
Sample : N4482-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW345

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090622\
Data File : BN021613.D
Acq On : 06 Sep 2022 22:46
Operator : CG/JU
Sample : N4482-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW345

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc