
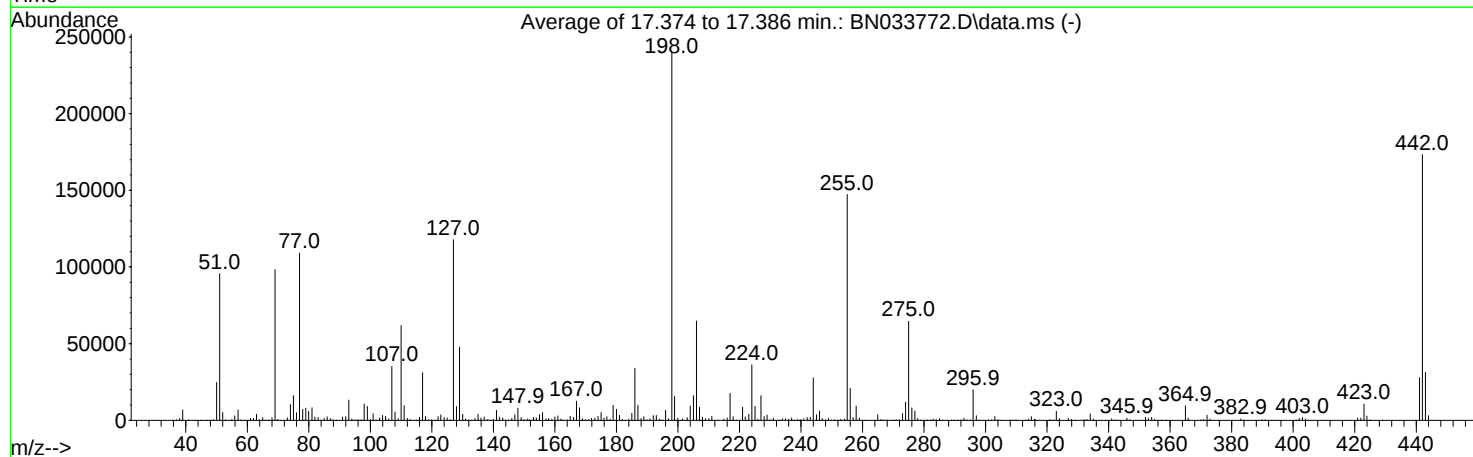


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090624\
Data File : BN033772.D
Acq On : 06 Sep 2024 08:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN090424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 04 18:36:01 2024

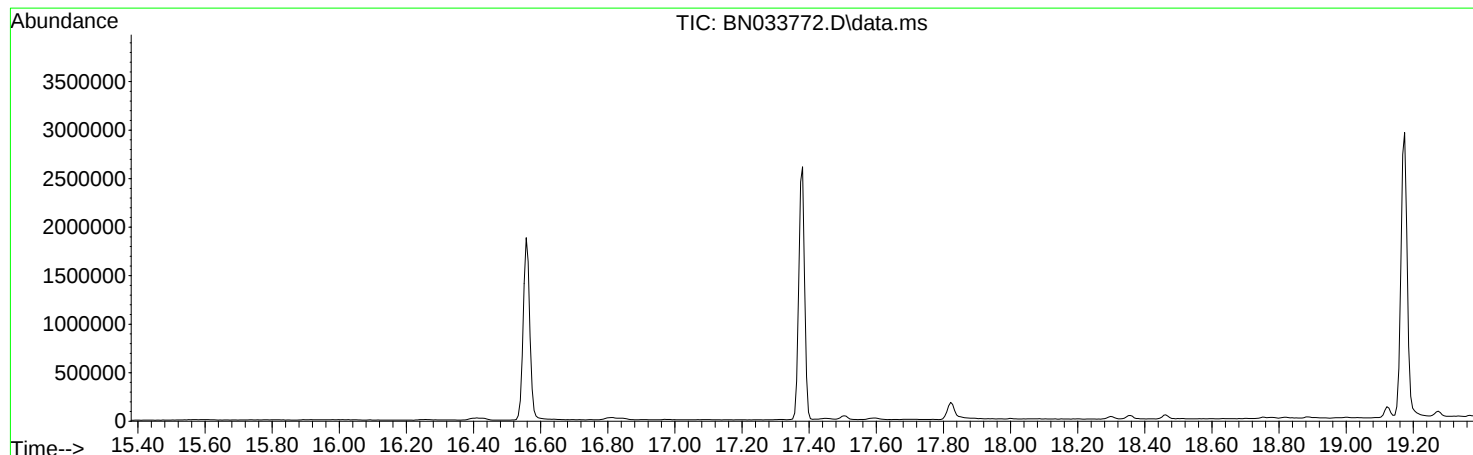

AutoFind: Scans 2446, 2447, 2448; Background Corrected with Scan 2439

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.8	95578	PASS
68	69	0.00	2	1.8	1754	PASS
69	198	0.00	100	41.0	98397	PASS
70	69	0.00	2	0.6	591	PASS
127	198	10	80	49.1	117837	PASS
197	198	0.00	2	0.4	1016	PASS
198	198	100	100	100.0	239851	PASS
199	198	5	9	6.6	15768	PASS
275	198	10	60	26.9	64616	PASS
365	198	1	100	4.0	9514	PASS
441	198	0.01	100	11.6	27763	PASS
442	442	50	100	100.0	173248	PASS
443	442	15	24	18.1	31355	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/6/2024	BNA_N	<u>BN033772.D</u>
Compound Name	Response	Retention Time
DDT	817867	20.421
DDD	15207	19.98
DDE	1076	19.468
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16283	834150	1.95

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090624\
Data File : BN033772.D
Acq On : 06 Sep 2024 08:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 06 19:11:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 04:54:27 2024
Response via : Initial Calibration

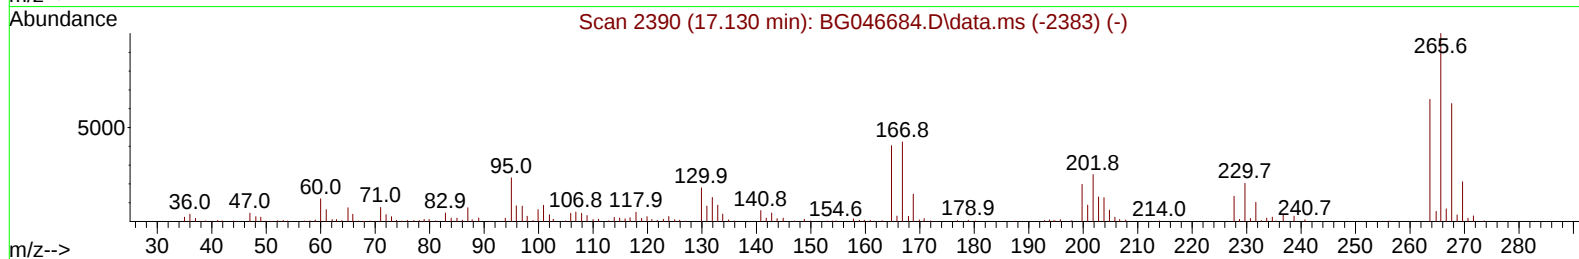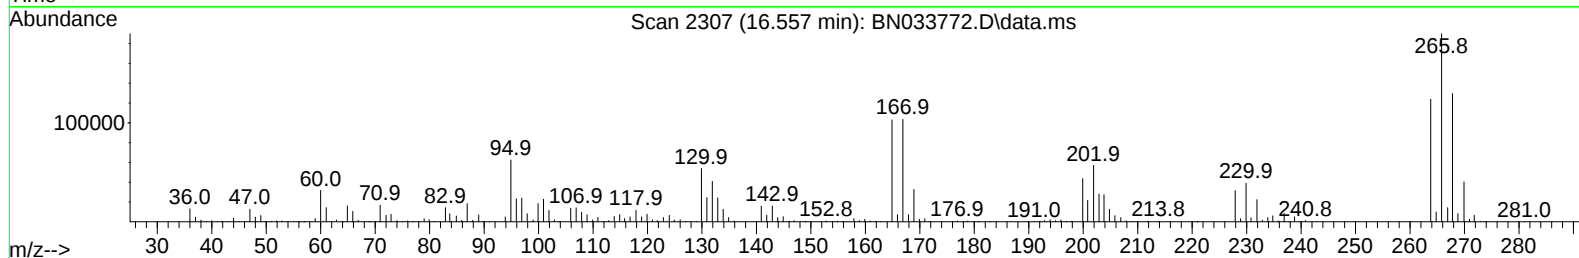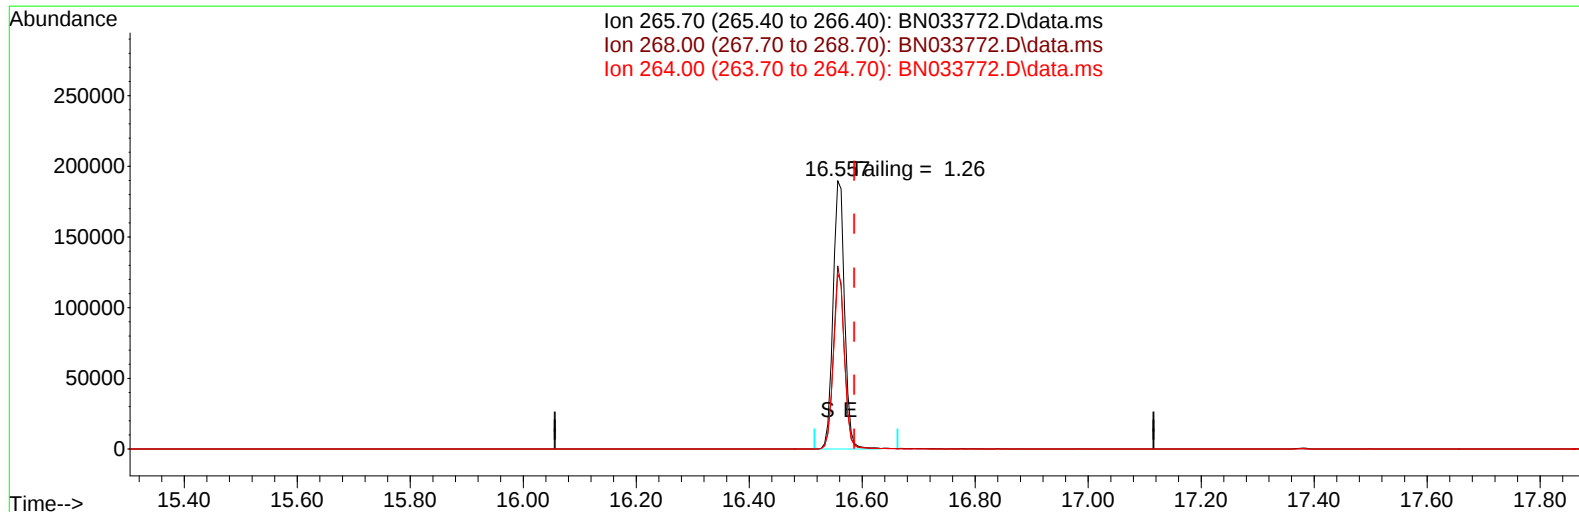

TIC: BN033772.D\data.ms

(70) Pentachlorophenol (C)

16.557min (-0.029) 21760.36 ng




response 269304

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.21
264.00	61.60	65.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090624\
Data File : BN033772.D
Acq On : 06 Sep 2024 08:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 06 19:11:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 04:54:27 2024
Response via : Initial Calibration

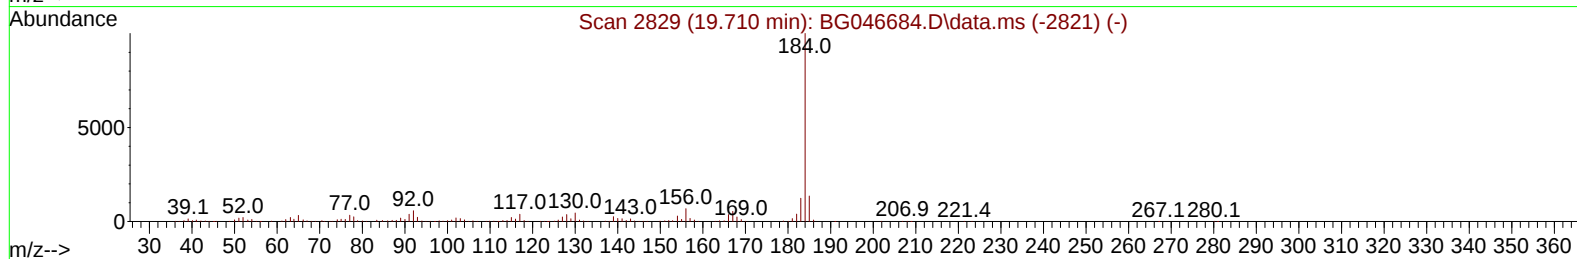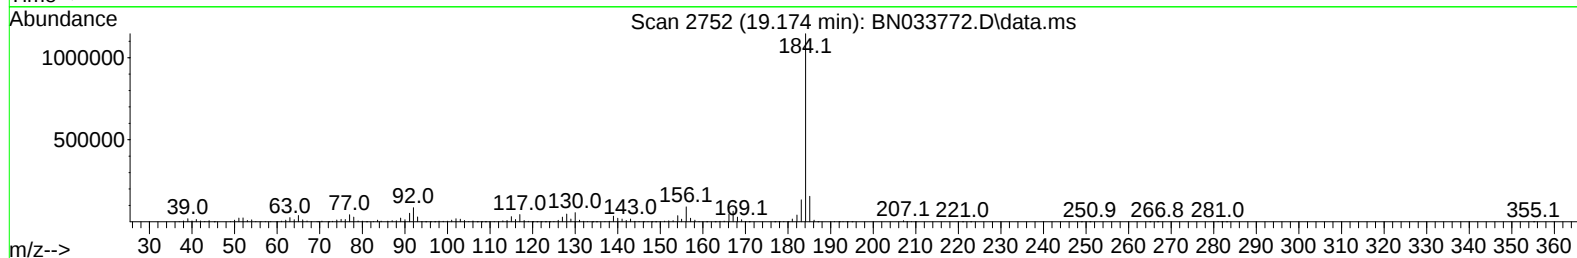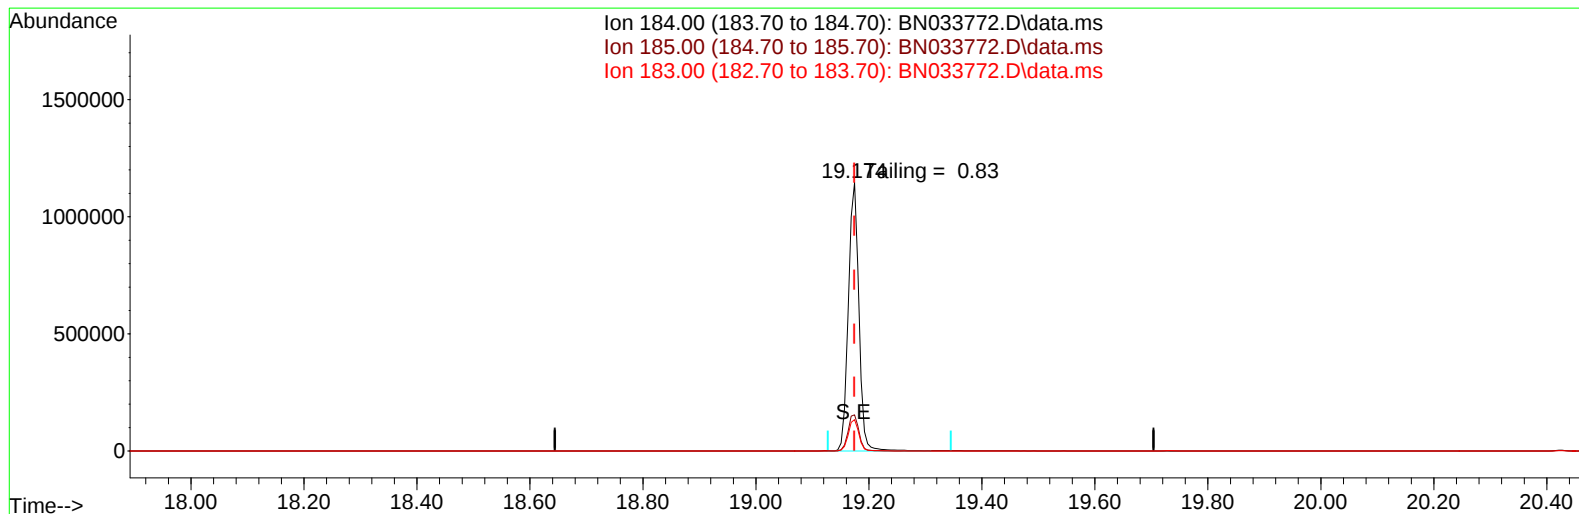

TIC: BN033772.D\data.ms

(77) Benzidine

19.174min (+ 0.000) 0.00 ng

response 1494843

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.52
183.00	13.20	11.68
0.00	0.00	0.00