


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090624\
Data File : BN033791.D
Acq On : 06 Sep 2024 21:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN090424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 04 18:36:01 2024

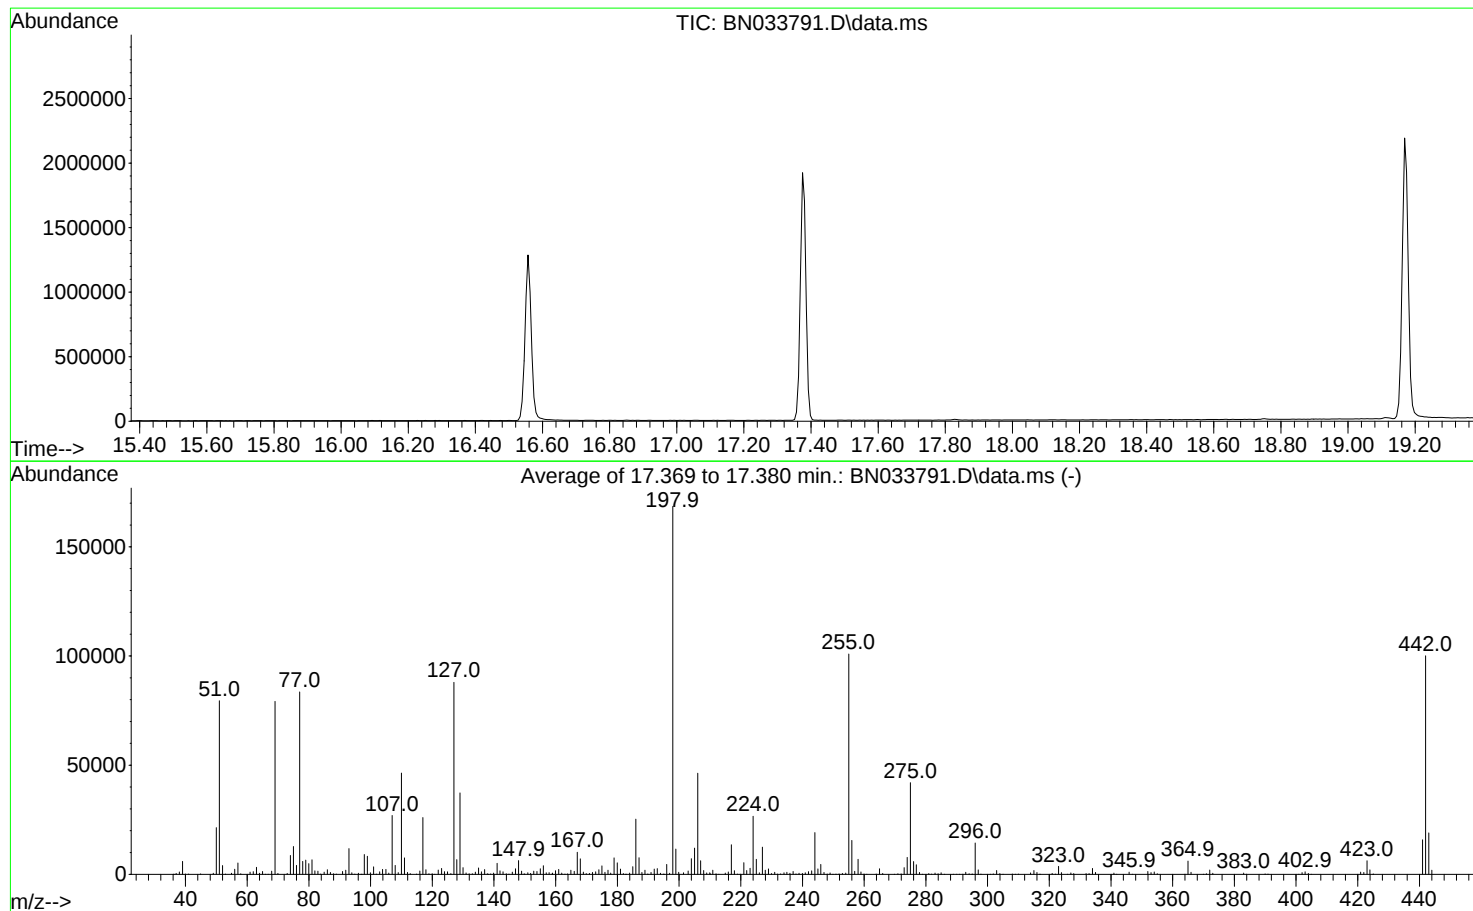

AutoFind: Scans 2445, 2446, 2447; Background Corrected with Scan 2439

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.2	79493	PASS
68	69	0.00	2	1.9	1488	PASS
69	198	0.00	100	47.0	79229	PASS
70	69	0.00	2	0.5	418	PASS
127	198	10	80	52.2	87955	PASS
197	198	0.00	2	0.3	532	PASS
198	198	100	100	100.0	168469	PASS
199	198	5	9	6.9	11600	PASS
275	198	10	60	24.9	42003	PASS
365	198	1	100	3.6	6086	PASS
441	198	0.01	100	9.4	15844	PASS
442	442	50	100	100.0	100091	PASS
443	442	15	24	19.0	18993	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/6/2024	BNA_N	<u>BN033791.D</u>
Compound Name	Response	Retention Time
DDT	560577	20.416
DDD	9063	19.974
DDE	307	19.469
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9370	569947	1.64

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090624\
Data File : BN033791.D
Acq On : 06 Sep 2024 21:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 07 02:02:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 07 02:00:52 2024
Response via : Initial Calibration

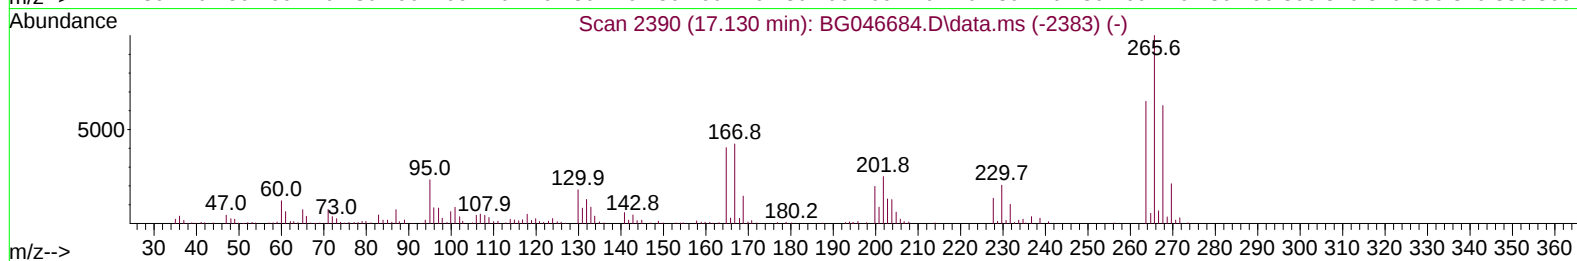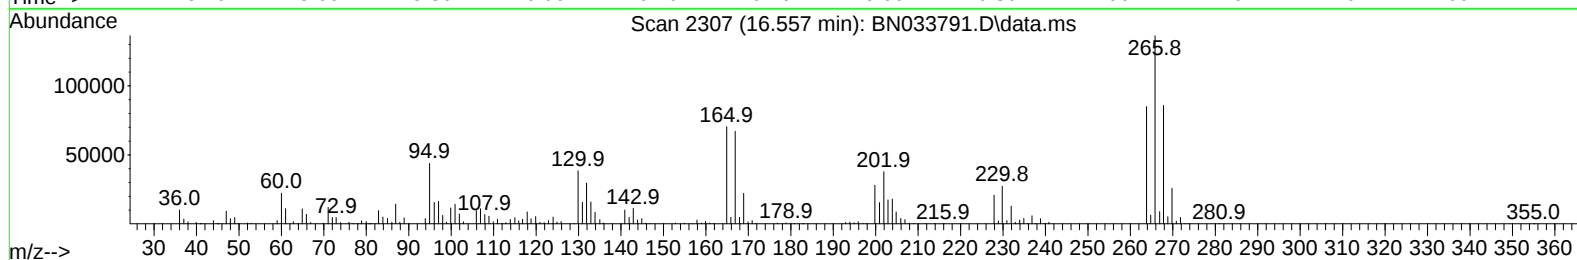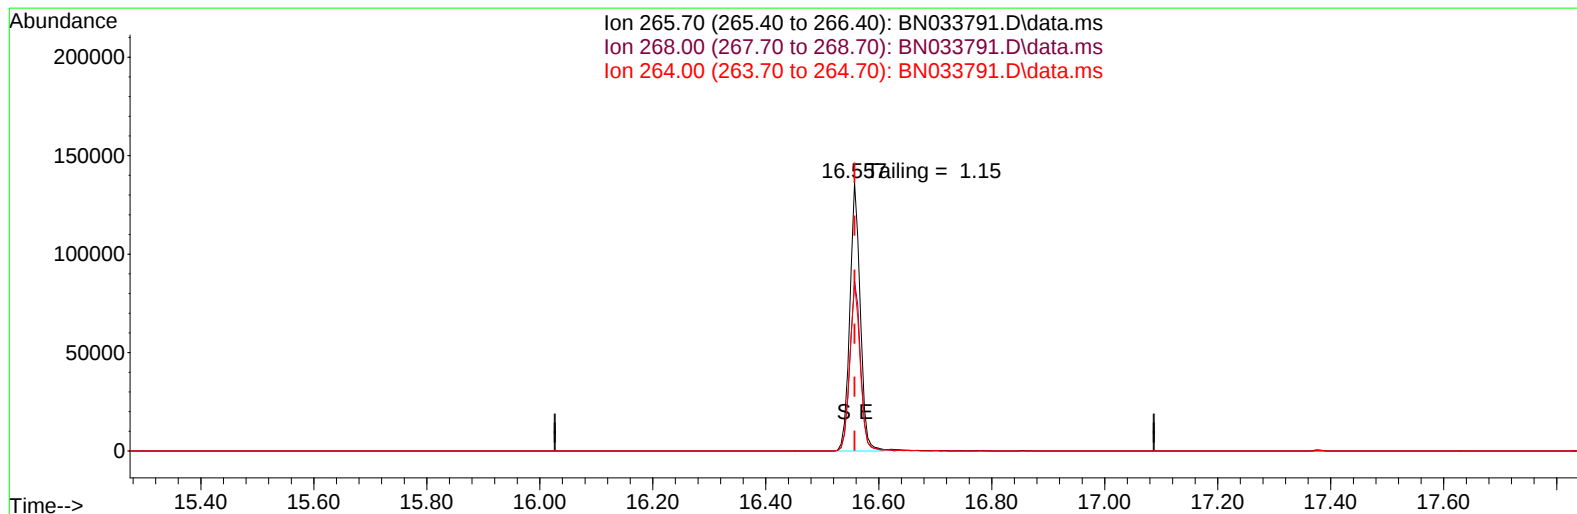

TIC: BN033791.D\data.ms

(70) Pentachlorophenol (C)

16.557min (0.000) 18862.89 ng

response 175417

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.06
264.00	61.60	62.38
0.00	0.00	0.00

