

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090722\
 Data File : BN021632.D
 Acq On : 07 Sep 2022 18:29
 Operator : CG/JU
 Sample : N4483-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW352

Quant Time: Sep 08 02:02:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 07 01:01:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.063	152	155417	20.000	ng/u1	0.00
20) Naphthalene-d8	10.893	136	684878	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.722	164	441344	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.469	188	918348	20.000	ng/u1	0.00
79) Chrysene-d12	21.657	240	819956	20.000	ng/u1	# 0.00
88) Perylene-d12	24.174	264	740536	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	18505	4.470	ng/uL	0.00
4) Pyridine-d5	3.805	84	51507	4.566	ng/u1	0.01
7) Phenol-d5	7.210	99	350019	24.831	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.381	67	215353	25.240	ng/u1	0.00
11) 2-Chlorophenol-d4	7.587	132	269542	26.283	ng/u1	0.00
15) 4-Methylphenol-d8	8.775	113	270020	24.414	ng/u1	0.00
21) Nitrobenzene-d5	9.240	128	134726	28.873	ng/u1	0.00
24) 2-Nitrophenol-d4	9.969	143	138662	33.270	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.510	165	247665	26.832	ng/u1	0.00
31) 4-Chloroaniline-d4	11.034	131	294396	18.780	ng/u1	0.00
46) Dimethylphthalate-d6	14.122	166	828671	27.471	ng/u1	0.00
49) Acenaphthylene-d8	14.416	160	972053	27.641	ng/u1	0.00
54) 4-Nitrophenol-d4	14.910	143	133780	22.286	ng/u1	0.00
60) Fluorene-d10	15.710	176	735745	28.030	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.822	200	90604	24.666	ng/u1	0.00
73) Anthracene-d10	17.569	188	1129489	27.909	ng/u1	0.00
81) Pyrene-d10	19.857	212	1317070	33.776	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.010	264	1105265	31.489	ng/u1	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.240	94	16694	1.146	ng/u1	98
80) Fluoranthene	19.527	202	52975	1.126	ng/u1	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090722\
Data File : BN021632.D
Acq On : 07 Sep 2022 18:29
Operator : CG/JU
Sample : N4483-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW352

Quant Time: Sep 08 02:02:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 07 01:01:49 2022
Response via : Initial Calibration




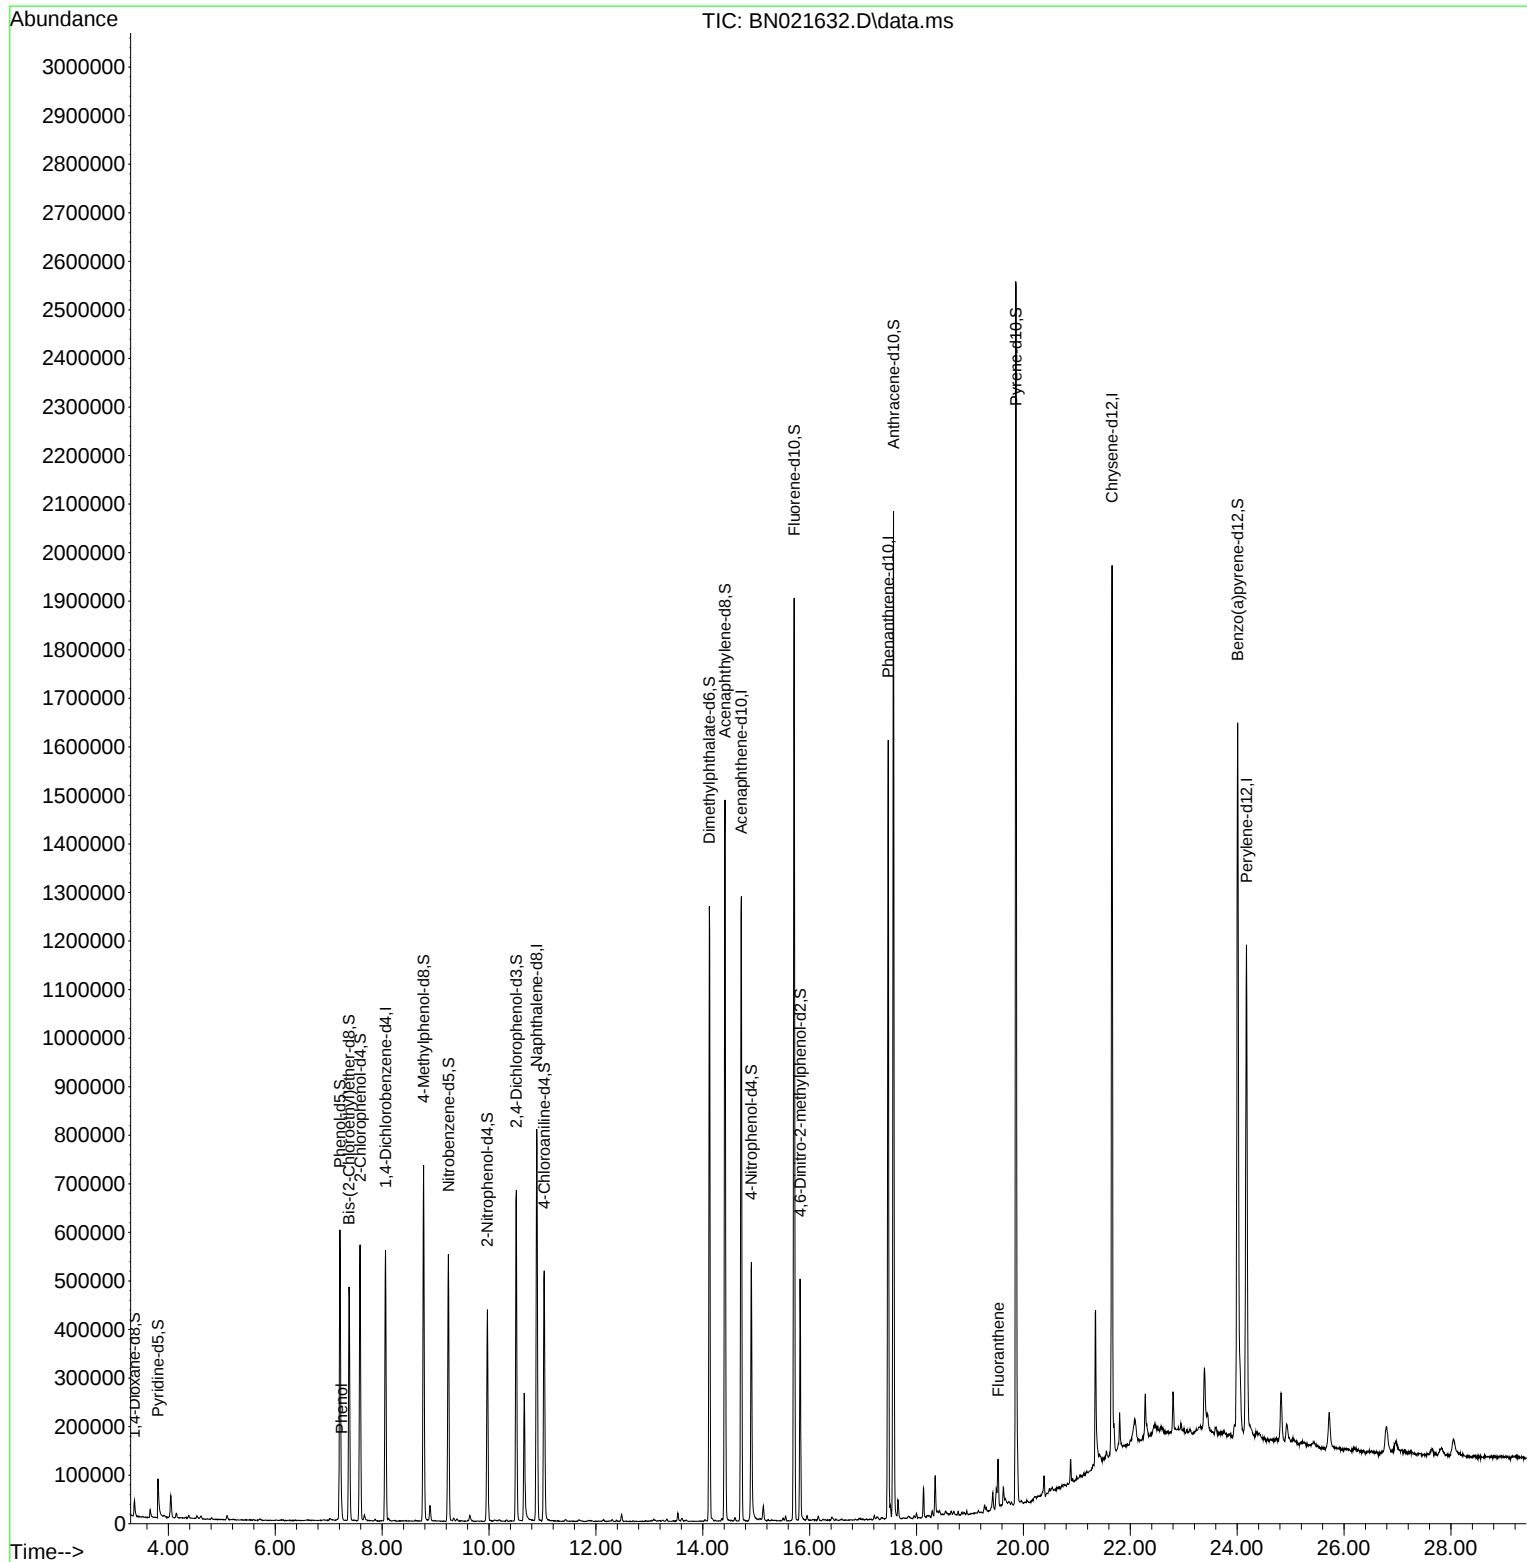


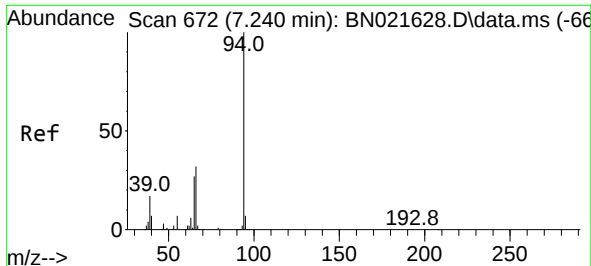

#8
Phenol
Concen: 1.146 ng/ul
RT: 7.240 min Scan# 672
Delta R.T. -0.000 min
Lab File: BN021632.D
Acq: 07 Sep 2022 18:29

Instrument :
BNA_N
ClientSampleId :
EW352

Tgt Ion: 94 Resp: 16694
Ion Ratio Lower Upper
94 100
65 28.9 23.6 35.4
66 37.2 31.2 46.8

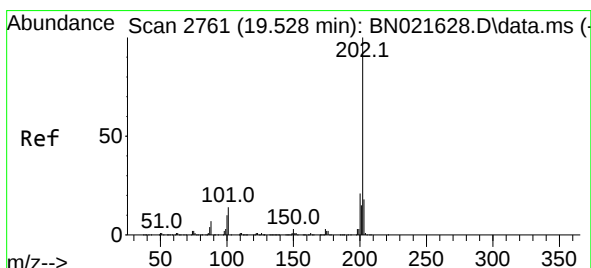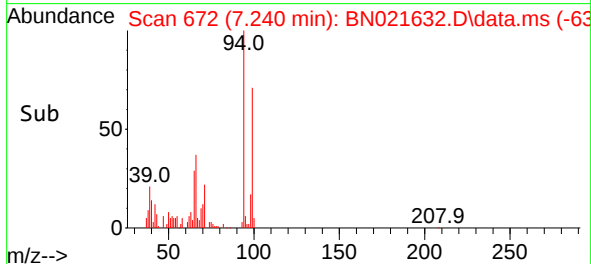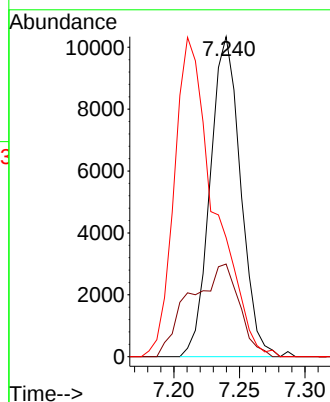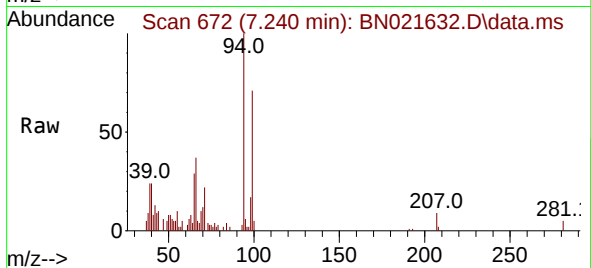

#80
Fluoranthene
Concen: 1.126 ng/ul
RT: 19.527 min Scan# 2761
Delta R.T. -0.000 min
Lab File: BN021632.D
Acq: 07 Sep 2022 18:29

Tgt Ion: 202 Resp: 52975
Ion Ratio Lower Upper
202 100
101 12.1 8.9 13.3
100 9.5 6.7 10.1

