

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090722\
 Data File : BN021633.D
 Acq On : 07 Sep 2022 19:07
 Operator : CG/JU
 Sample : N4483-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW361

Quant Time: Sep 08 02:02:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 07 01:01:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.063	152	141826	20.000	ng/ul	0.00
20) Naphthalene-d8	10.893	136	656278	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.716	164	436794	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.469	188	886206	20.000	ng/ul	0.00
79) Chrysene-d12	21.657	240	806281	20.000	ng/ul	# 0.00
88) Perylene-d12	24.174	264	748310	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	19187	5.079	ng/uL	0.00
4) Pyridine-d5	3.805	84	41672	4.048	ng/ul	0.01
7) Phenol-d5	7.211	99	355384	27.628	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.381	67	221400	28.435	ng/ul	0.00
11) 2-Chlorophenol-d4	7.587	132	273762	29.253	ng/ul	0.00
15) 4-Methylphenol-d8	8.775	113	291588	28.891	ng/ul	0.00
21) Nitrobenzene-d5	9.240	128	139755	31.256	ng/ul	0.00
24) 2-Nitrophenol-d4	9.969	143	142541	35.691	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.510	165	265947	30.068	ng/ul	0.00
31) 4-Chloroaniline-d4	11.034	131	396015	26.364	ng/ul	0.00
46) Dimethylphthalate-d6	14.122	166	896480	30.028	ng/ul	0.00
49) Acenaphthylene-d8	14.416	160	1066039	30.629	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	151636	25.524	ng/ul	0.00
60) Fluorene-d10	15.710	176	790212	30.419	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.822	200	100694	28.407	ng/ul	0.00
73) Anthracene-d10	17.569	188	1215004	31.111	ng/ul	0.00
81) Pyrene-d10	19.857	212	1483992	38.702	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.010	264	1304809	36.787	ng/ul	0.00
Target Compounds						
8) Phenol	7.240	94	18824	1.416	ng/ul	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090722\
Data File : BN021633.D
Acq On : 07 Sep 2022 19:07
Operator : CG/JU
Sample : N4483-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW361

Quant Time: Sep 08 02:02:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 07 01:01:49 2022
Response via : Initial Calibration

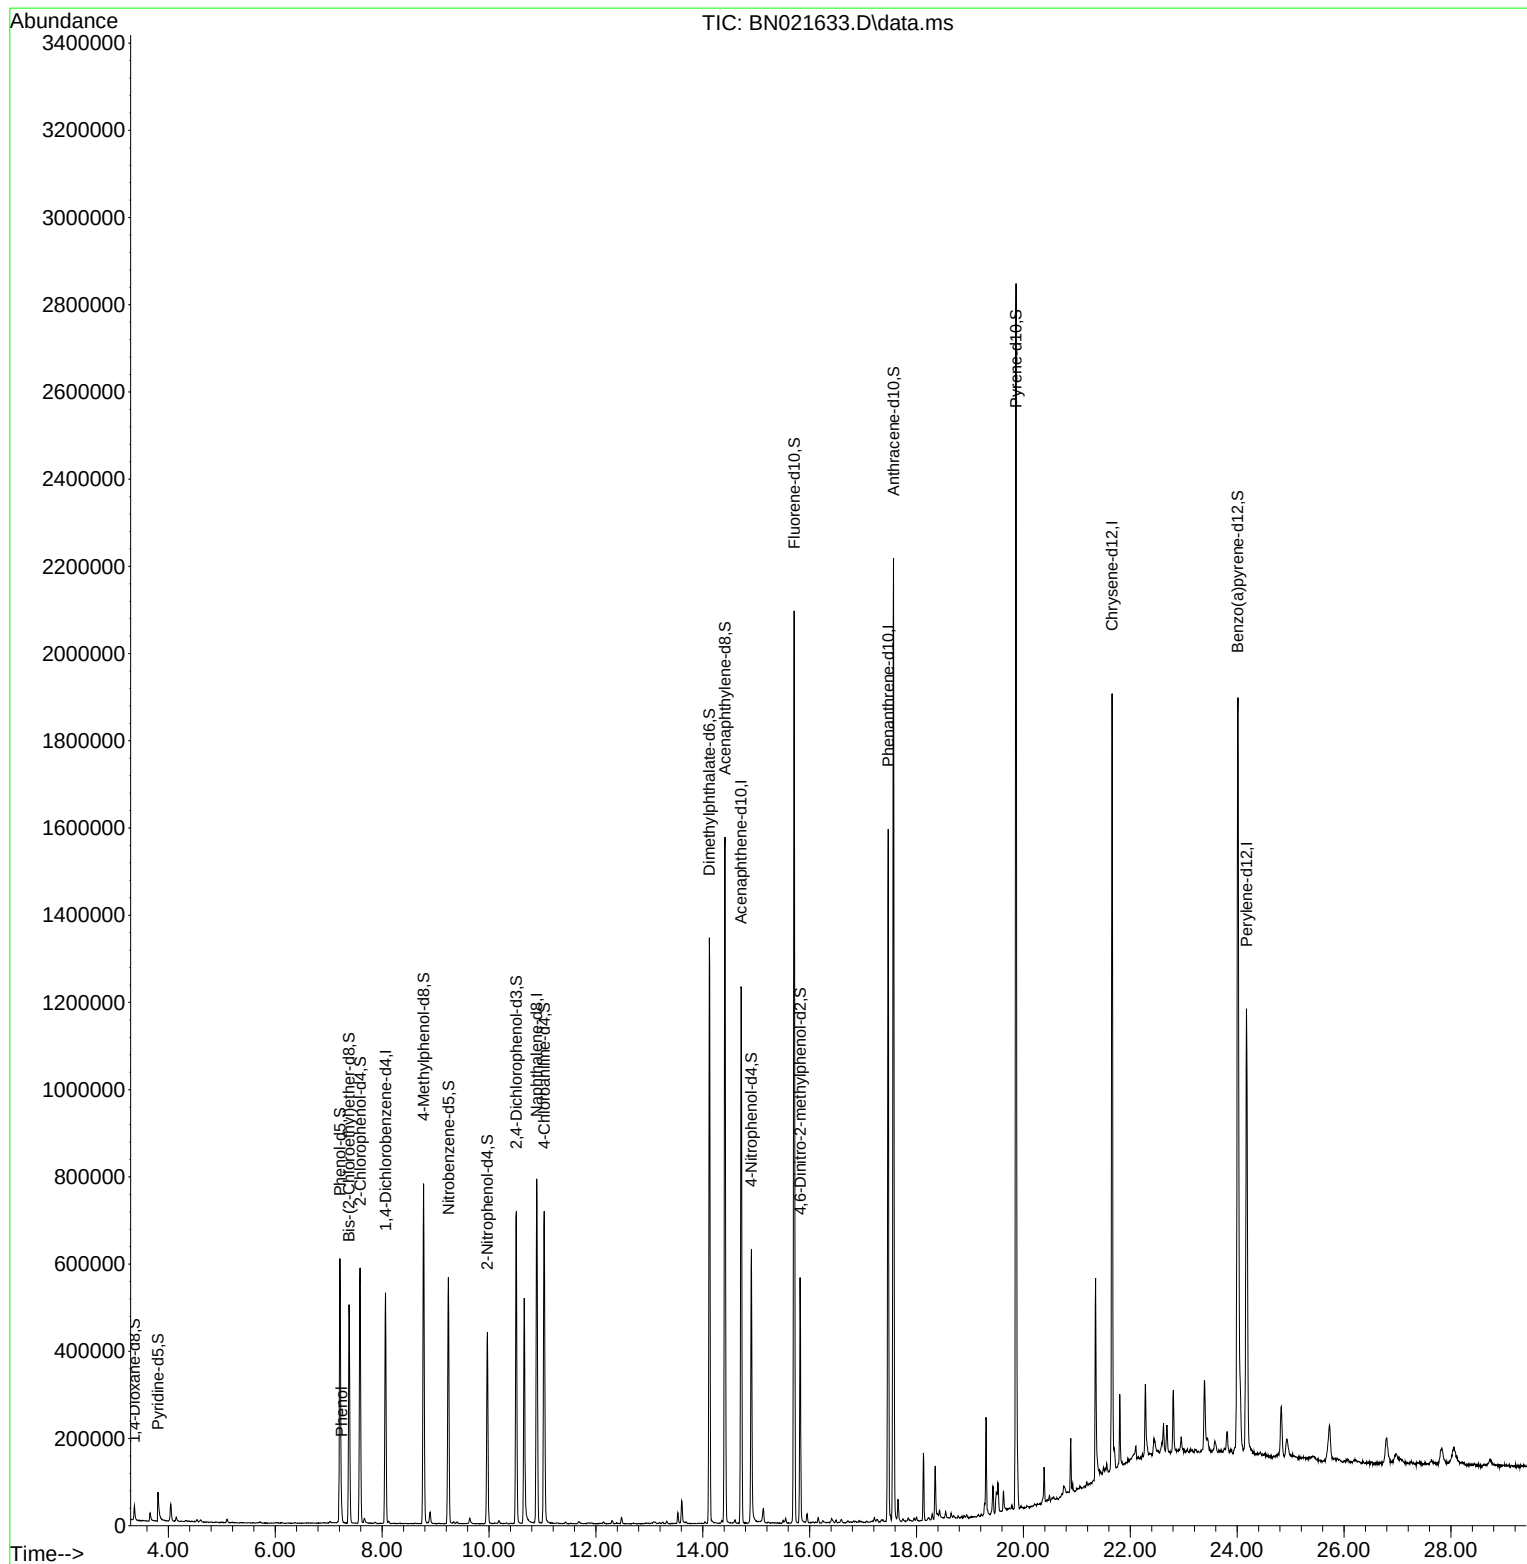

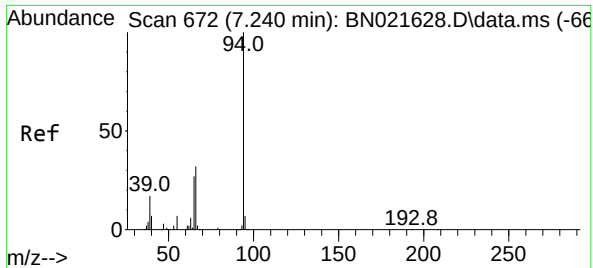

#8
Phenol
Concen: 1.416 ng/ul
RT: 7.240 min Scan# 61
Delta R.T. 0.000 min
Lab File: BN021633.D
Acq: 07 Sep 2022 19:07

Instrument :
BNA_N
ClientSampleId :
EW361

Tgt Ion:	94	Resp:	18824
Ion	Ratio	Lower	Upper
94	100		
65	27.0	23.6	35.4
66	36.9	31.2	46.8

