

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090722\
 Data File : BN021627.D
 Acq On : 07 Sep 2022 15:21
 Operator : CG/JU
 Sample : PB146669BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK669

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
 Title : SVOA CALIBRATION

Signal : TIC: BN021627.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	9	13	22	rVB	53624	72562	1.62%	0.148%
2	3.793	83	86	107	rBV	540005	861865	19.21%	1.754%
3	4.146	142	146	151	rVB	13068	18978	0.42%	0.039%
4	7.210	660	667	677	rBV	757543	1209898	26.97%	2.462%
5	7.381	690	696	707	rVB	634443	1021630	22.77%	2.079%
6	7.587	723	731	741	rBV	759194	1220658	27.21%	2.484%
7	8.063	804	812	820	rBV	658158	1057262	23.57%	2.152%
8	8.775	926	933	945	rBV	959746	1518307	33.84%	3.090%
9	9.240	1002	1012	1024	rBV	716603	1197167	26.68%	2.436%
10	9.969	1128	1136	1149	rBV	579727	950167	21.18%	1.934%
11	10.510	1221	1228	1237	rBV	887029	1510108	33.66%	3.073%
12	10.893	1285	1293	1302	rVB	920212	1612006	35.93%	3.281%
13	11.034	1306	1317	1333	rBV	1258192	2188021	48.77%	4.453%
14	12.481	1558	1563	1571	rVB2	17273	27800	0.62%	0.057%
15	14.128	1836	1843	1855	rBV	1790934	2508782	55.92%	5.106%
16	14.416	1885	1892	1900	rBV	1973439	2903119	64.71%	5.908%
17	14.722	1937	1944	1952	rBV	1527403	2256045	50.29%	4.592%
18	14.910	1969	1976	1989	rBV	844293	1218928	27.17%	2.481%
19	15.710	2102	2112	2125	rBV	2532113	3662520	81.64%	7.454%
20	15.822	2125	2131	2145	rBV	807146	1129754	25.18%	2.299%
21	15.951	2149	2153	2158	rVB	23427	32168	0.72%	0.065%
22	16.492	2239	2245	2251	rBV4	7078	10421	0.23%	0.021%
23	16.922	2314	2318	2323	rVV2	4310	6071	0.14%	0.012%
24	17.257	2370	2375	2378	rBV3	4616	7649	0.17%	0.016%
25	17.469	2405	2411	2421	rBV	1903043	2707295	60.34%	5.510%
26	17.569	2421	2428	2446	rVB2	2676988	3966069	88.40%	8.072%
27	18.004	2496	2502	2505	rBV4	3993	7982	0.18%	0.016%
28	18.133	2521	2524	2529	rVB6	9364	11211	0.25%	0.023%
29	19.427	2739	2744	2749	rBV	32588	44648	1.00%	0.091%
30	19.498	2752	2756	2761	rVB	30628	40371	0.90%	0.082%
31	19.863	2812	2818	2832	rBV	3252893	4486387	100.00%	9.131%
32	21.663	3118	3124	3141	rBV	2125831	2736956	61.01%	5.570%
33	23.392	3414	3418	3425	rBV2	51663	83501	1.86%	0.170%
34	24.015	3516	3524	3538	rBV2	1946592	4087473	91.11%	8.319%
35	24.180	3545	3552	3562	rBV	1160095	2416807	53.87%	4.919%
36	24.827	3658	3662	3669	rVB	81512	165940	3.70%	0.338%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090722\
Data File : BN021627.D
Acq On : 07 Sep 2022 15:21
Operator : CG/JU
Sample : PB146669BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK669

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Title : SVOA CALIBRATION

37	25.733	3813	3816	3826	rVB2	85898	178532	3.98%	0.363%
----	--------	------	------	------	------	-------	--------	-------	--------




Sum of corrected areas: 49135058

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090722\
Data File : BN021627.D
Acq On : 07 Sep 2022 15:21
Operator : CG/JU
Sample : PB146669BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK669

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

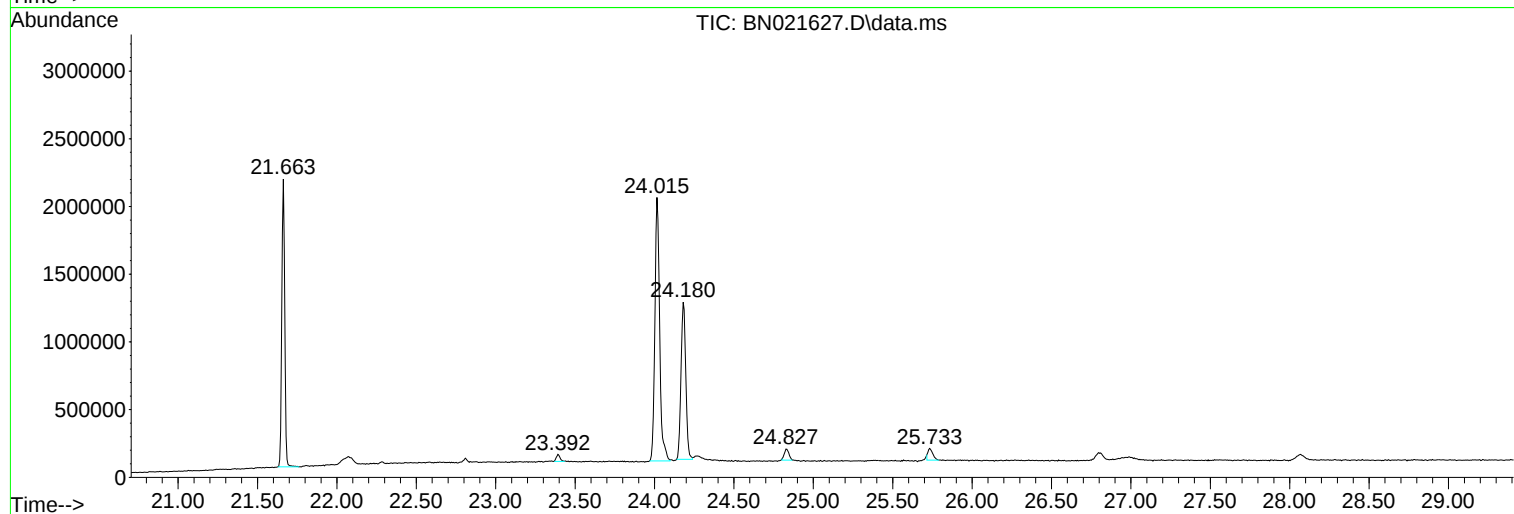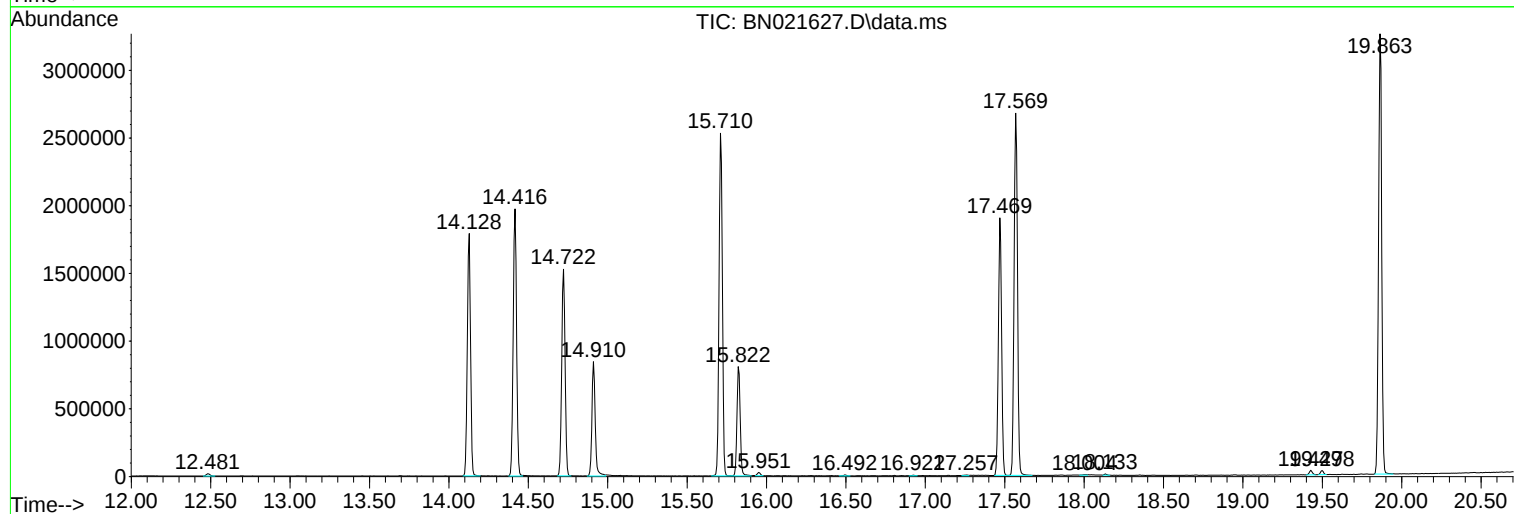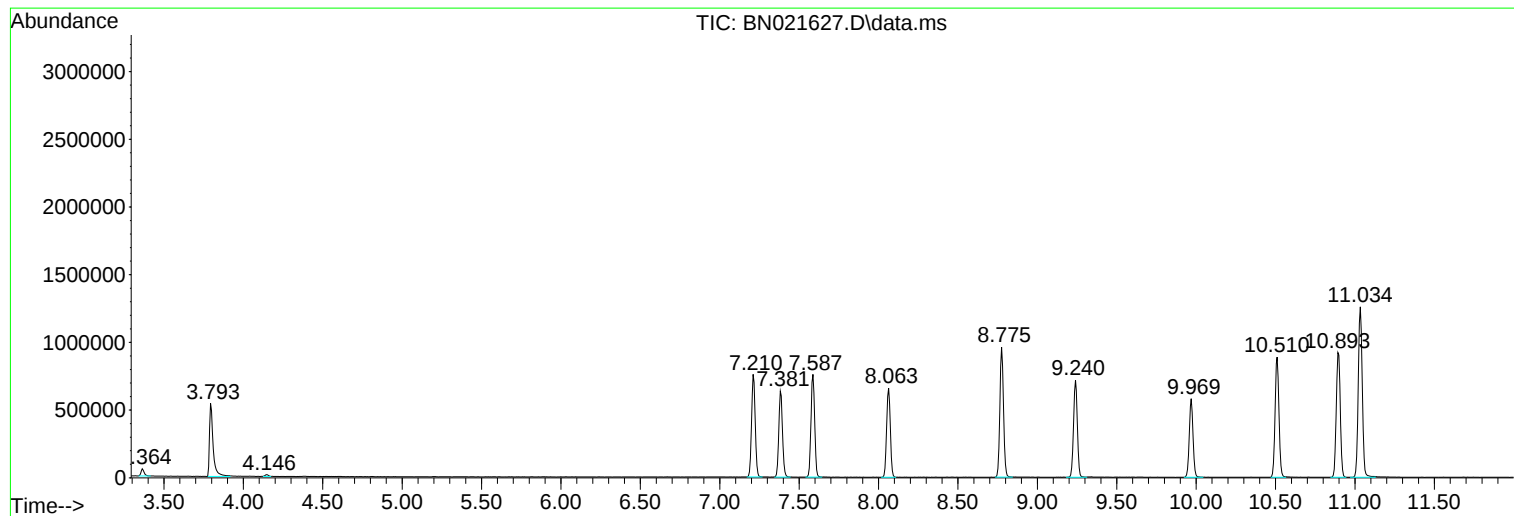

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090722\
Data File : BN021627.D
Acq On : 07 Sep 2022 15:21
Operator : CG/JU
Sample : PB146669BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK669

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090722\
Data File : BN021627.D
Acq On : 07 Sep 2022 15:21
Operator : CG/JU
Sample : PB146669BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK669

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc