


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090819\
 Data File : BN007558.D
 Acq On : 08 Sep 2019 19:12
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 17 15:50:54 2019

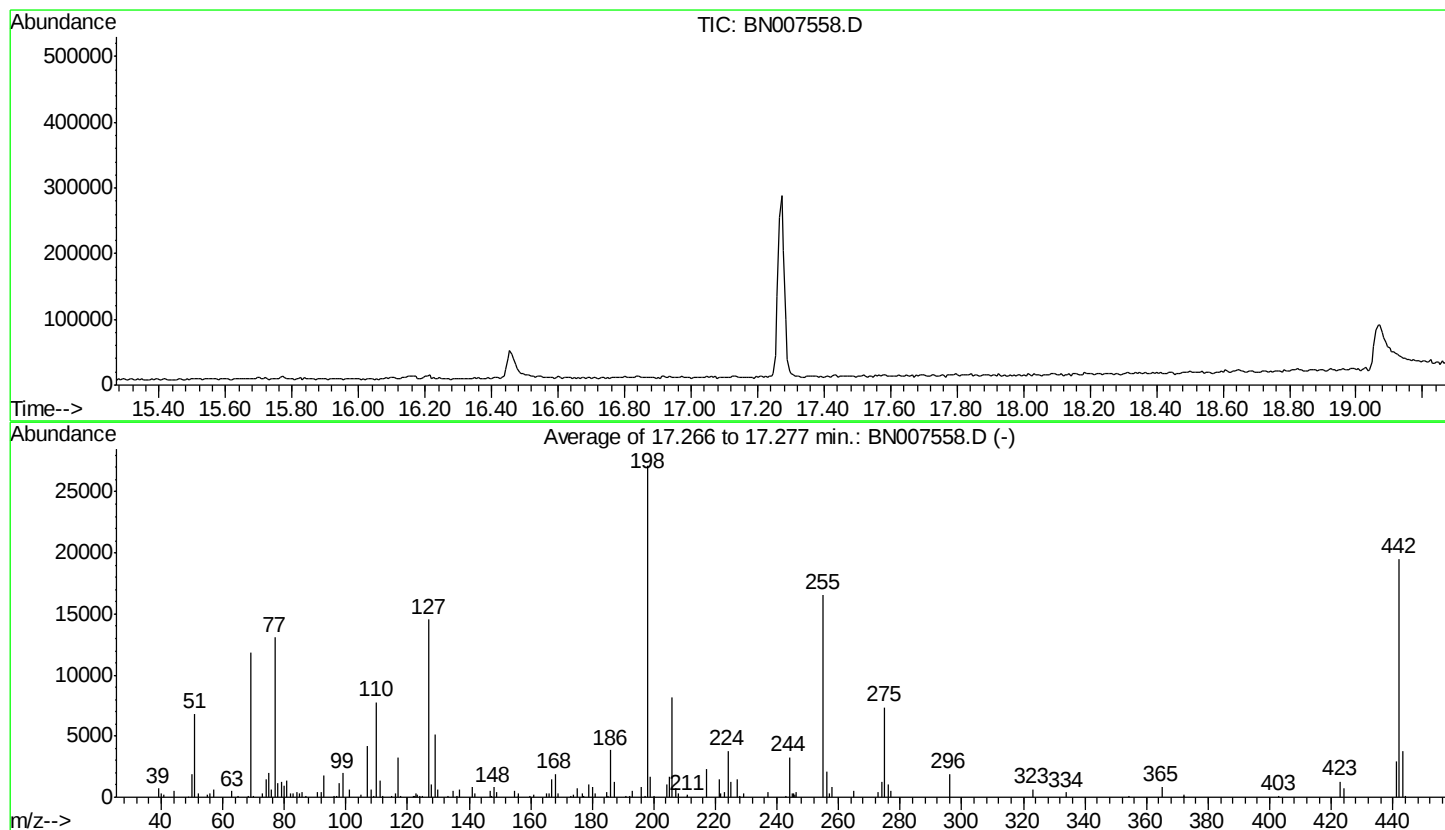

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.3	6859	PASS
68	69	0.00	2	1.0	123	PASS
69	198	0.00	100	43.6	11848	PASS
70	69	0.00	2	1.0	121	PASS
127	198	10	80	53.7	14566	PASS
197	198	0.00	2	0.5	129	PASS
198	198	100	100	100.0	27149	PASS
199	198	5	9	6.4	1729	PASS
275	198	10	60	27.2	7386	PASS
365	198	1	100	3.1	845	PASS
441	198	0.01	100	11.0	2986	PASS
442	198	50	100	71.8	19501	PASS
443	442	15	24	19.3	3769	PASS