
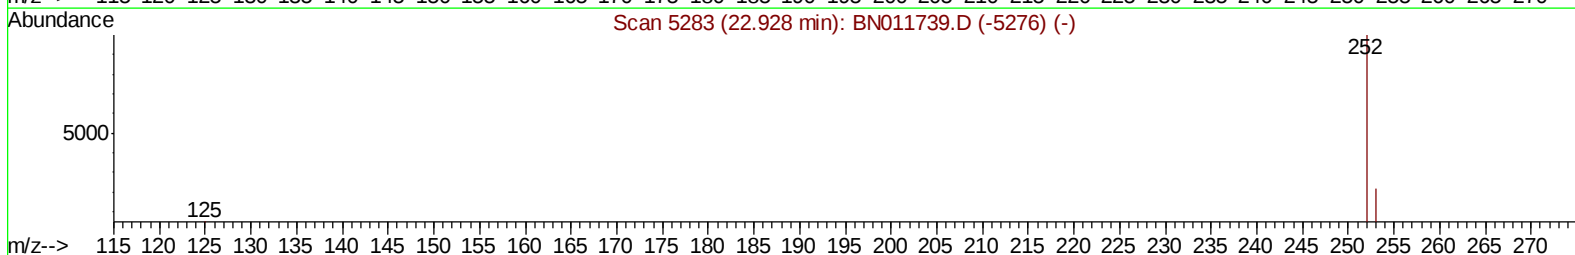
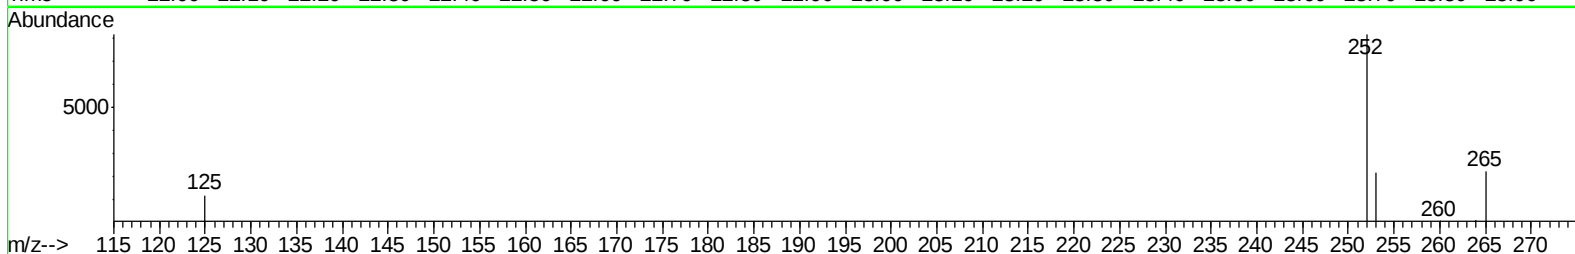


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090820\
Data File : BN011743.D
Acq On : 08 Sep 2020 18:54
Operator : CG/JU
Sample : L3840-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Sep 09 06:42:19 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN090820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 09 06:29:50 2020
Response via : Initial Calibration

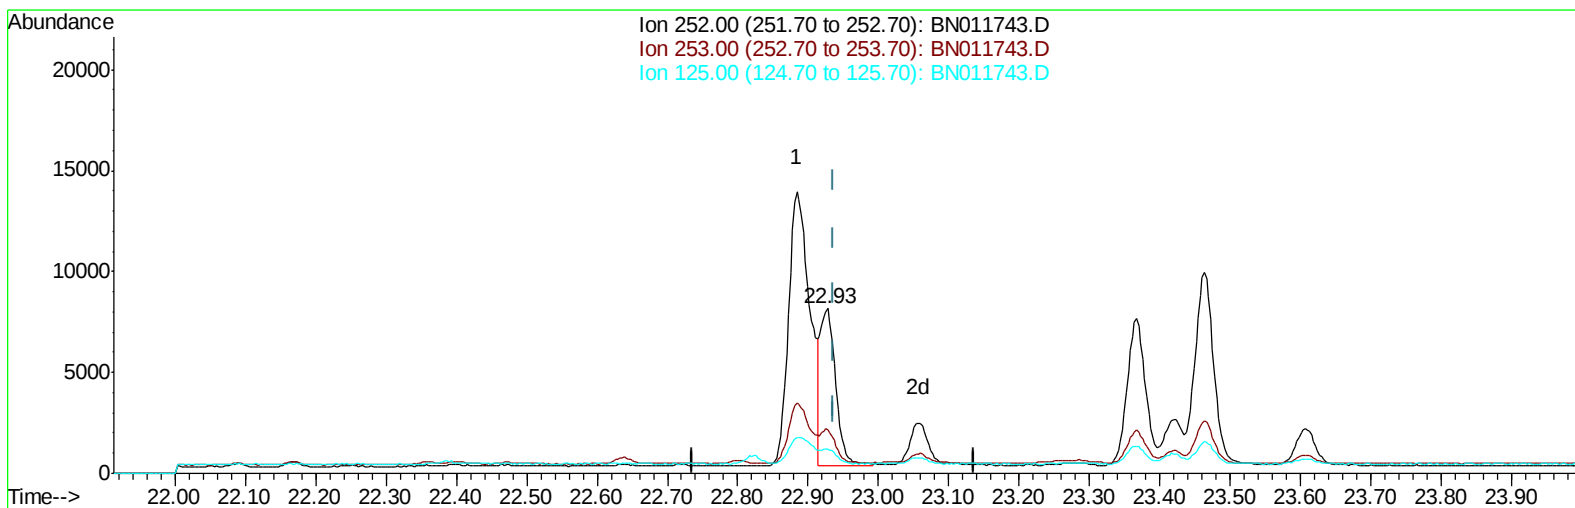

TIC: BN011743.D

(22) Benzo(k)fluoranthene

22.928min (-0.009) 0.28ng/ul m

response 12005

Ion	Exp%	Act%
252.00	100	100
253.00	25.90	26.70
125.00	12.10	14.50
0.00	0.00	0.00