
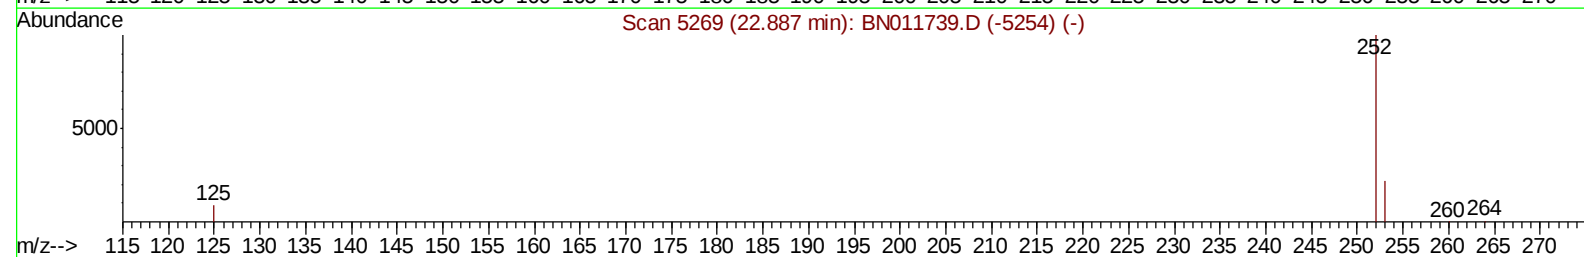
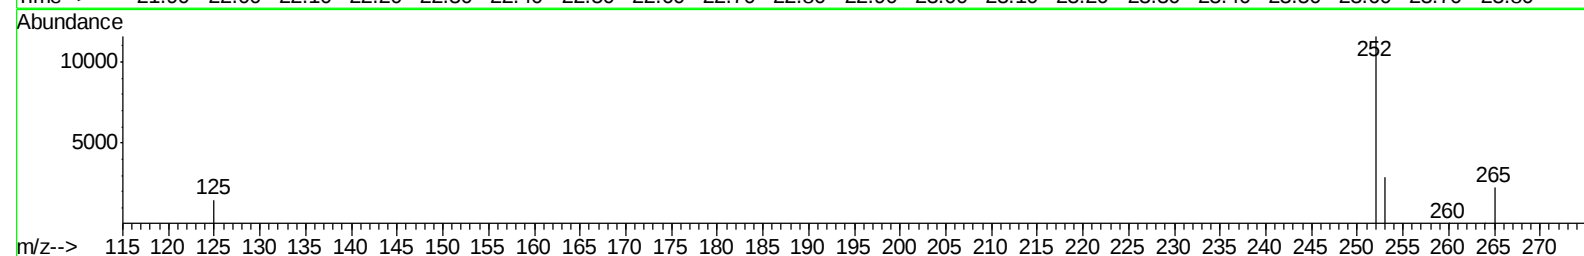


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090820\
 Data File : BN011744.D
 Acq On : 08 Sep 2020 19:30
 Operator : CG/JU
 Sample : L3840-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Sep 09 06:44:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN090820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 09 06:29:50 2020
 Response via : Initial Calibration

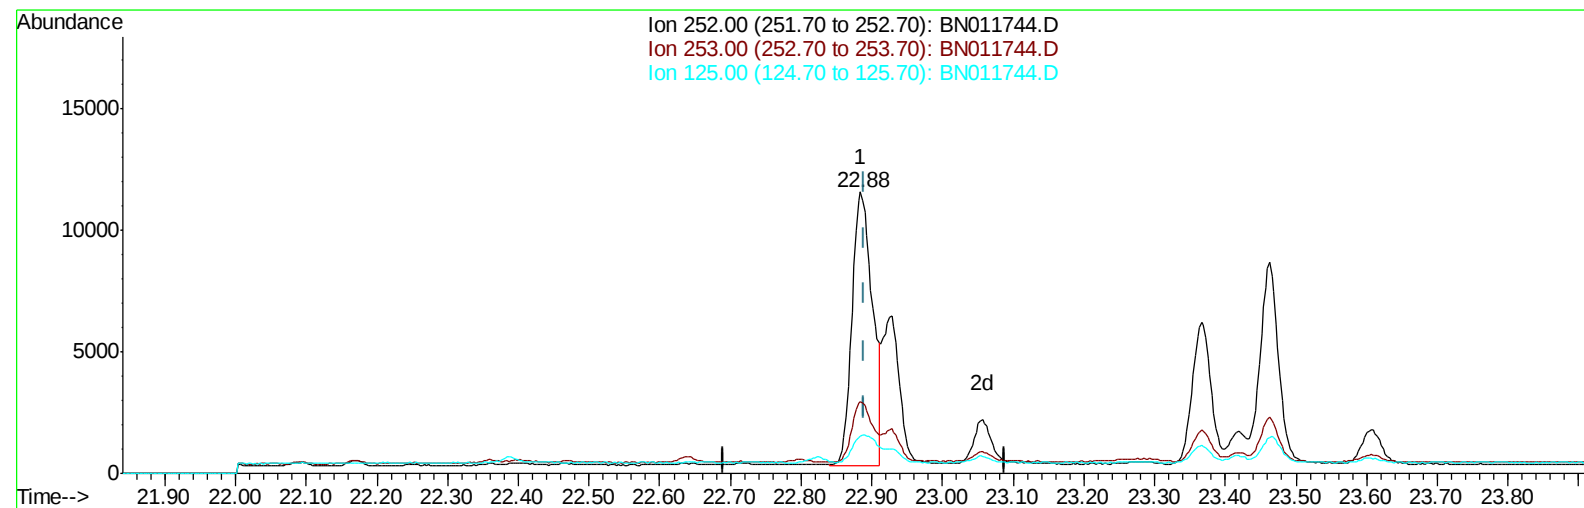

TIC: BN011744.D

(21) Benzo(b)fluoranthene

22.884min (-0.006) 0.59ng/ul m

response 22330

Ion	Exp%	Act%
252.00	100	100
253.00	25.30	25.34
125.00	11.80	13.04
0.00	0.00	0.00