
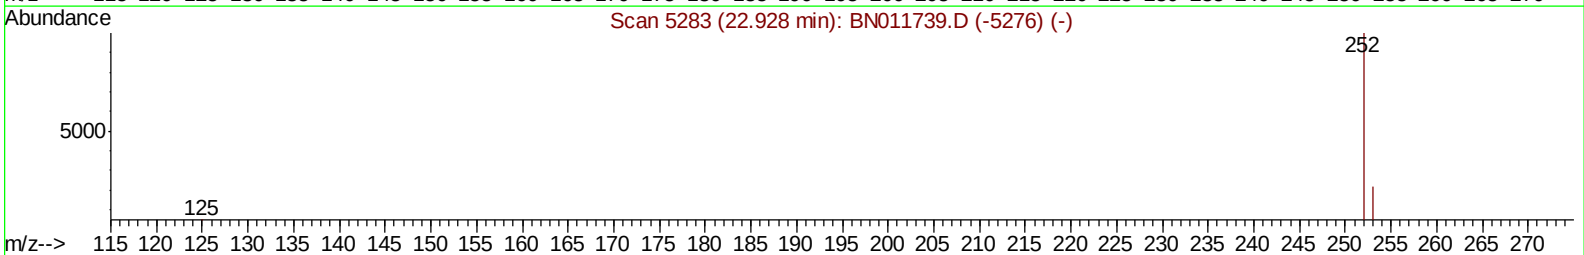
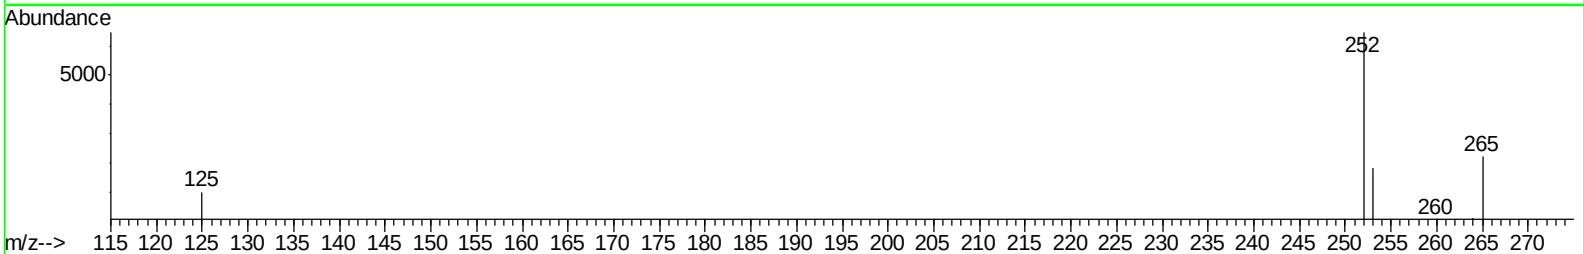


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090820\  
Data File : BN011744.D  
Acq On : 08 Sep 2020 19:30  
Operator : CG/JU  
Sample : L3840-07  
Misc :  
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Sep 09 06:44:57 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN090820.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Sep 09 06:29:50 2020  
Response via : Initial Calibration

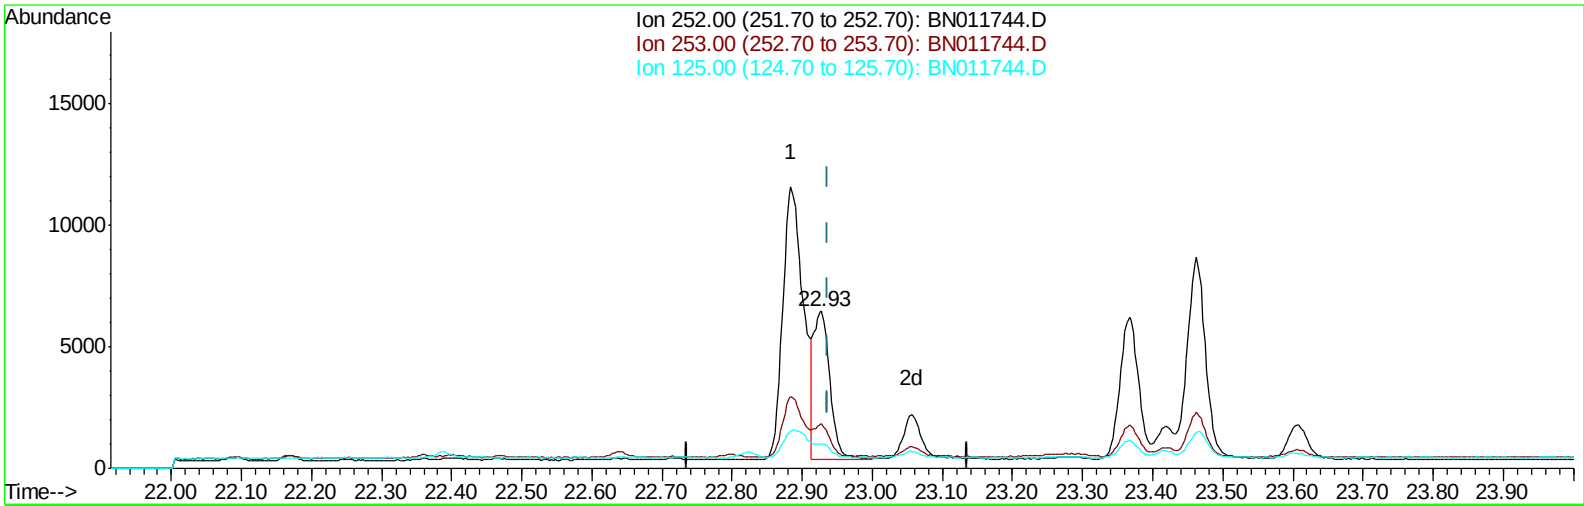

TIC: BN011744.D

(22) Benzo(k)fluoranthene

22.928min (-0.009) 0.24ng/ul m

response 9534

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 25.90 | 28.31  |
| 125.00 | 12.10 | 15.51# |
| 0.00   | 0.00  | 0.00   |