
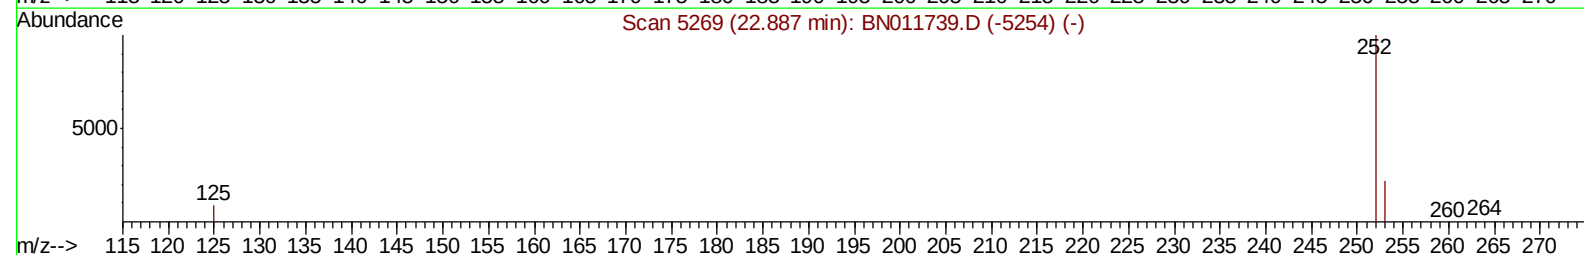
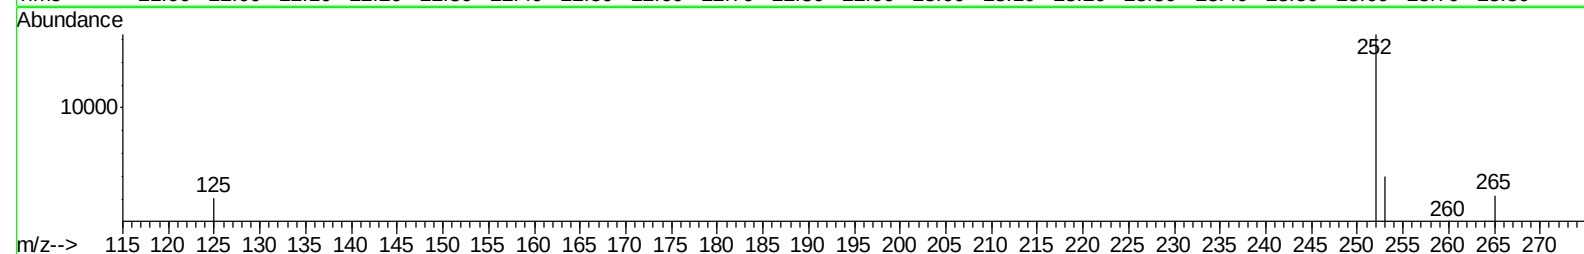


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090820\
Data File : BN011745.D
Acq On : 08 Sep 2020 20:06
Operator : CG/JU
Sample : L3840-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Sep 09 06:48:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN090820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 09 06:29:50 2020
Response via : Initial Calibration

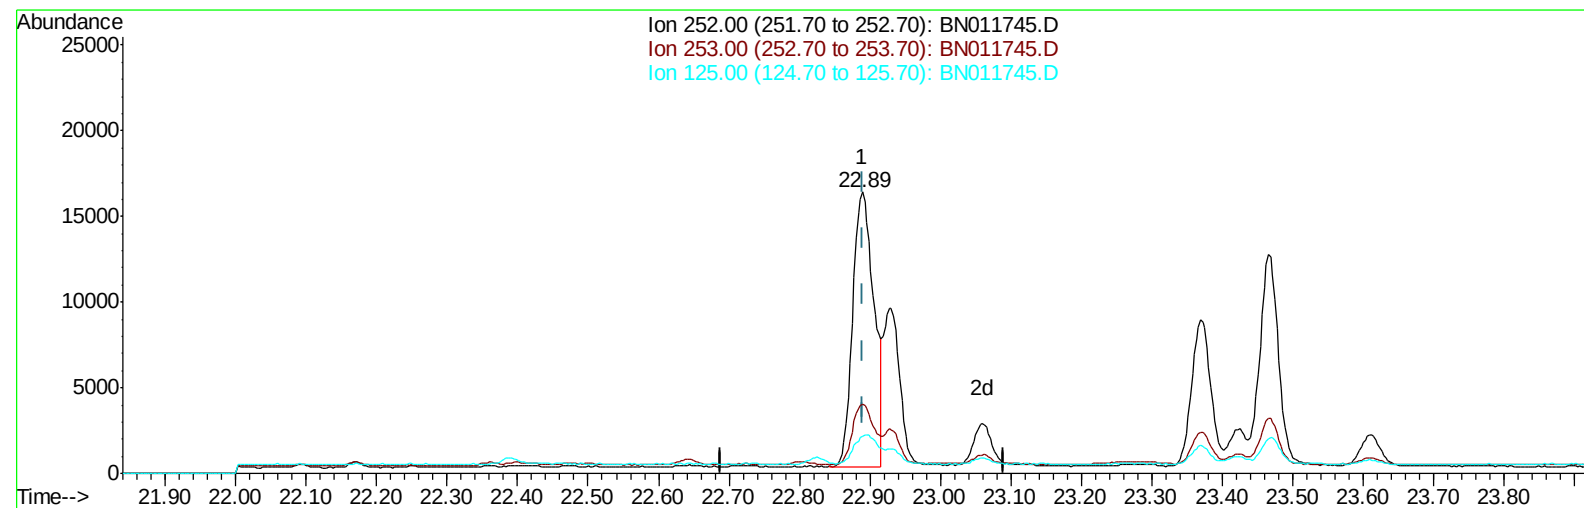

TIC: BN011745.D

(21) Benzo(b)fluoranthene

22.889min (-0.000) 0.81ng/ul m

response 33427

Ion	Exp%	Act%
252.00	100	100
253.00	25.30	24.53
125.00	11.80	12.99
0.00	0.00	0.00