
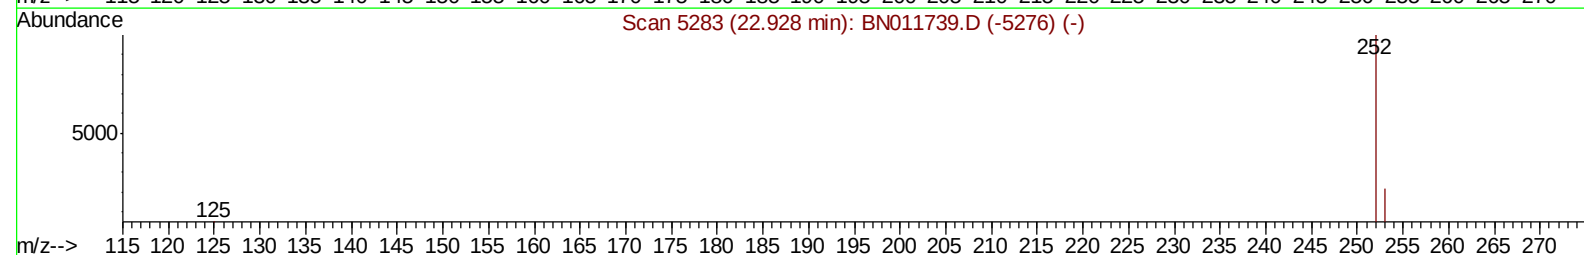
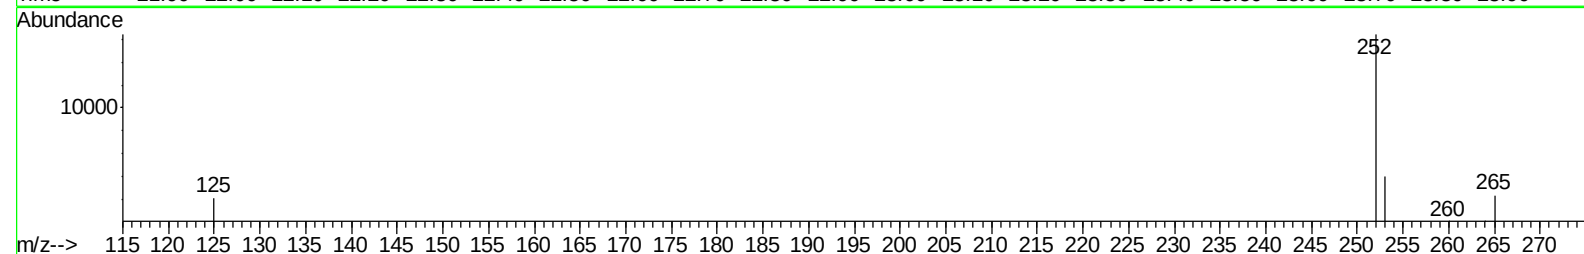


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090820\
 Data File : BN011745.D
 Acq On : 08 Sep 2020 20:06
 Operator : CG/JU
 Sample : L3840-12
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Quant Time: Sep 09 06:48:00 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN090820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 09 06:29:50 2020
 Response via : Initial Calibration

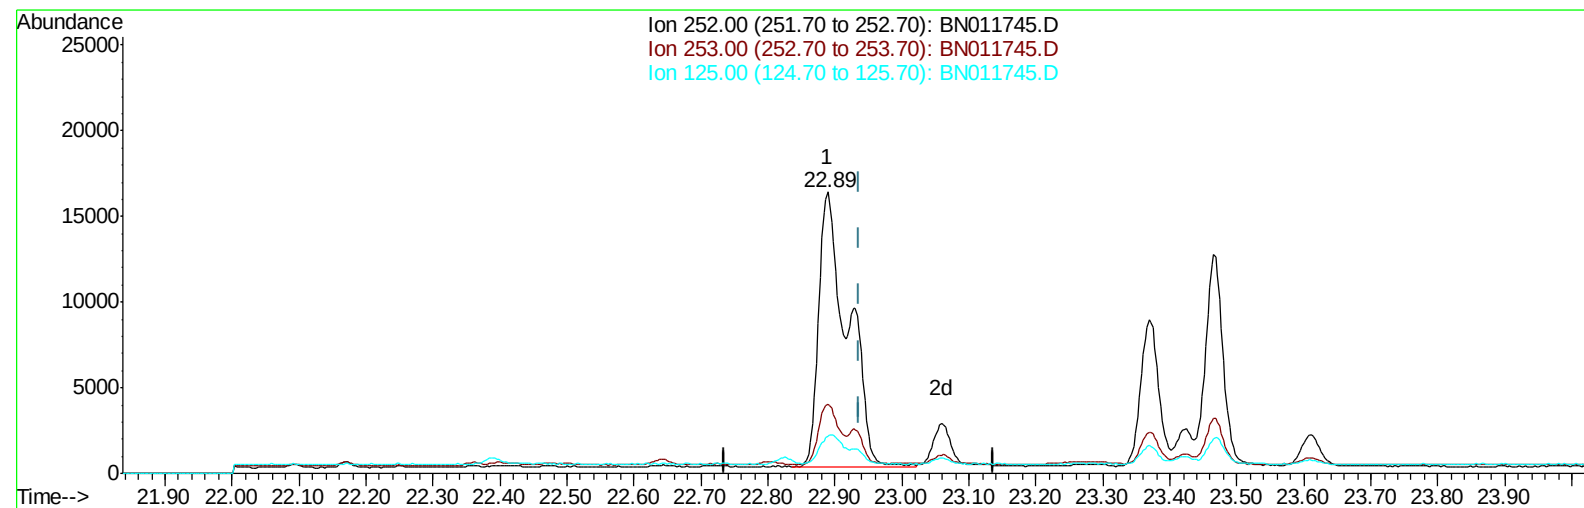

TIC: BN011745.D

(22) Benzo(k)fluoranthene

22.889min (-0.047) 1.15ng/ul

response 48497

Ion	Exp%	Act%
252.00	100	100
253.00	25.90	24.53
125.00	12.10	12.99
0.00	0.00	0.00