
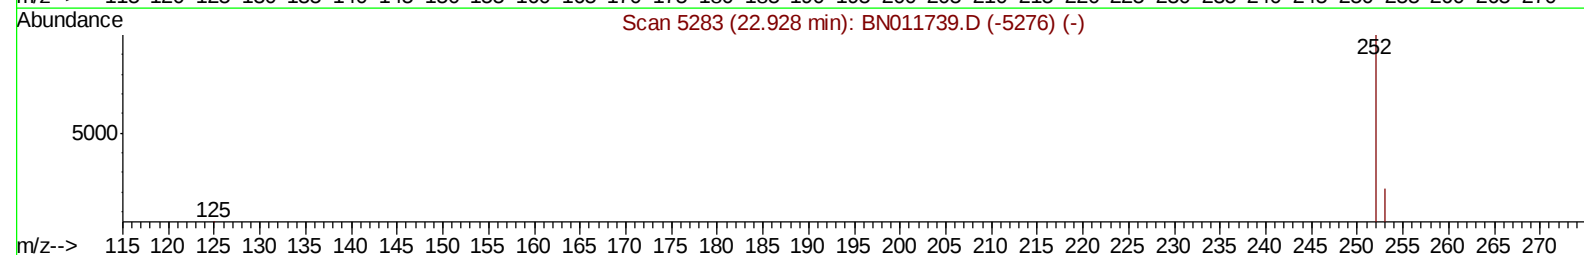
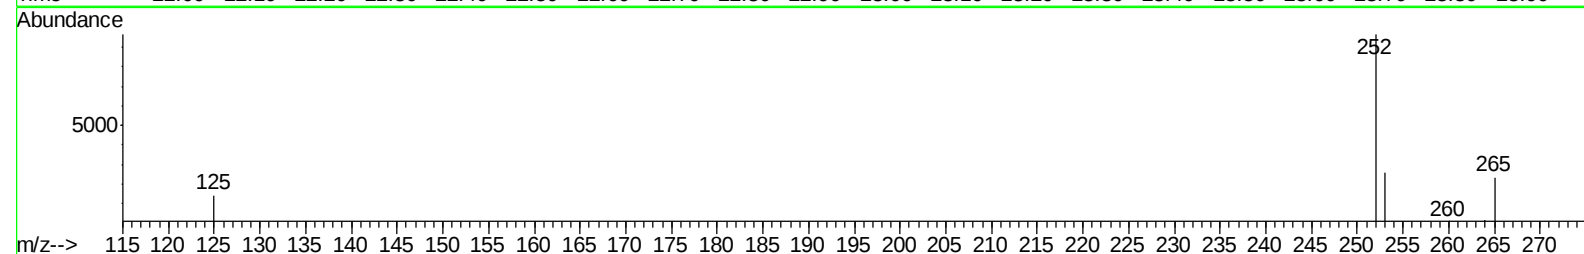


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090820\
 Data File : BN011745.D
 Acq On : 08 Sep 2020 20:06
 Operator : CG/JU
 Sample : L3840-12
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Quant Time: Sep 09 06:48:00 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN090820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 09 06:29:50 2020
 Response via : Initial Calibration

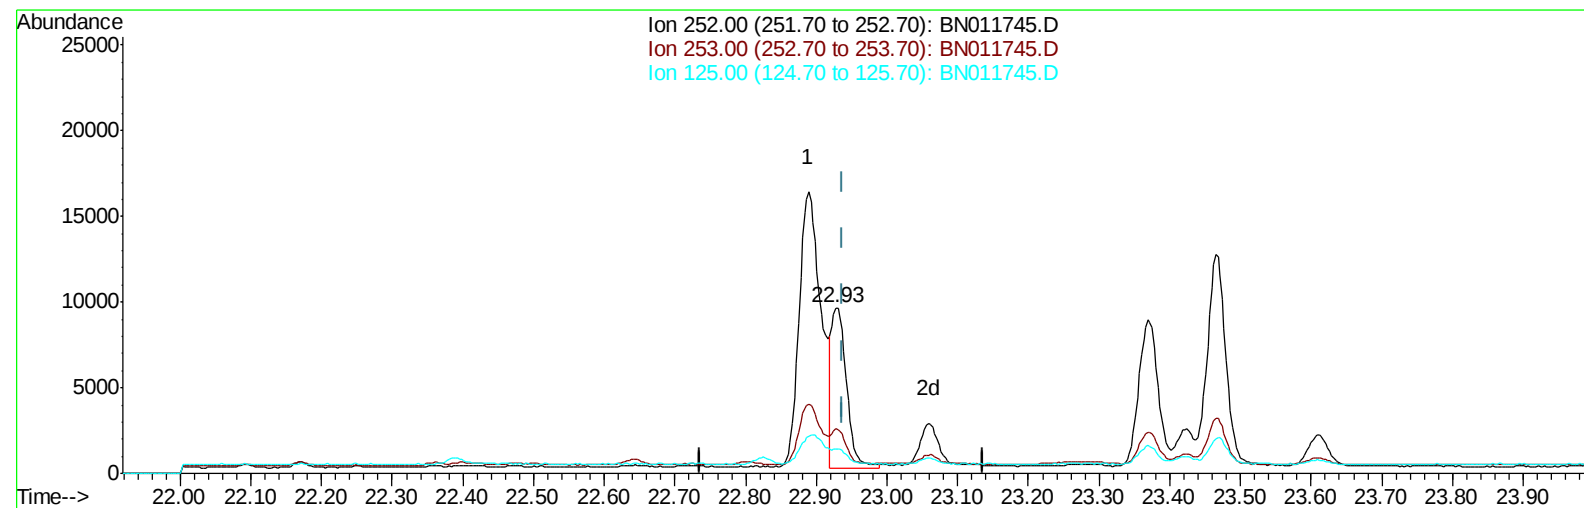

TIC: BN011745.D

(22) Benzo(k)fluoranthene

22.927min (-0.009) 0.33ng/ul m

response 13748

Ion	Exp%	Act%
252.00	100	100
253.00	25.90	26.79
125.00	12.10	14.66#
0.00	0.00	0.00