
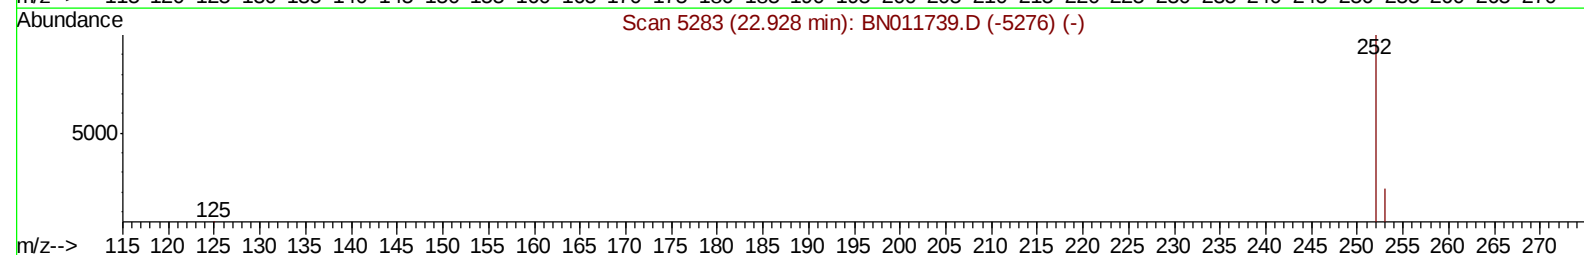
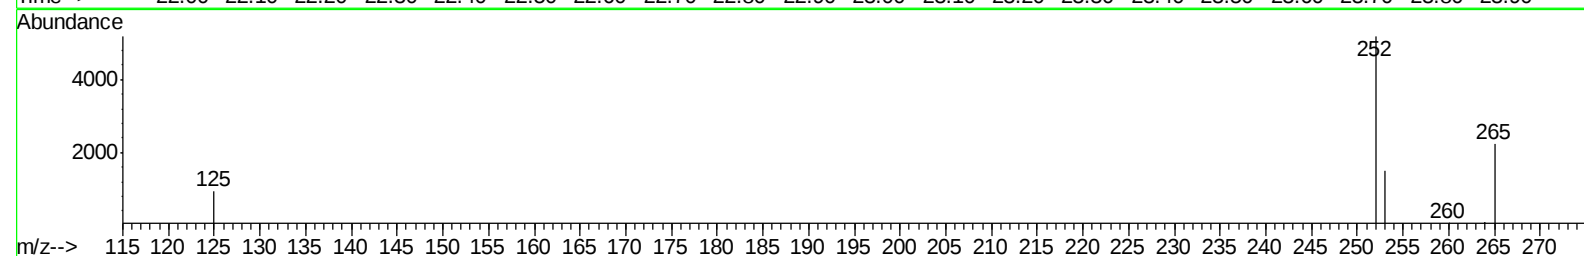


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090820\
Data File : BN011747.D
Acq On : 08 Sep 2020 21:19
Operator : CG/JU
Sample : L3840-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Sep 09 06:55:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN090820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 09 06:29:50 2020
Response via : Initial Calibration

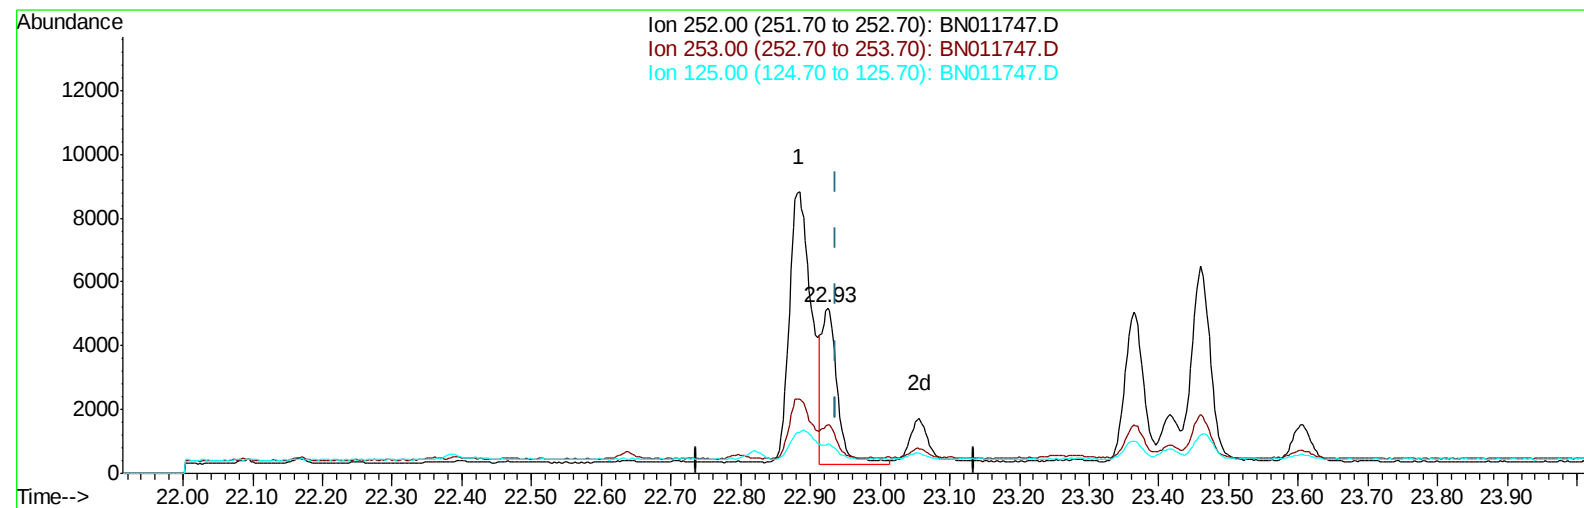

TIC: BN011747.D

(22) Benzo(k)fluoranthene

22.925min (-0.012) 0.19ng/ul m

response 7424

Ion	Exp%	Act%
252.00	100	100
253.00	25.90	29.15
125.00	12.10	18.02#
0.00	0.00	0.00