
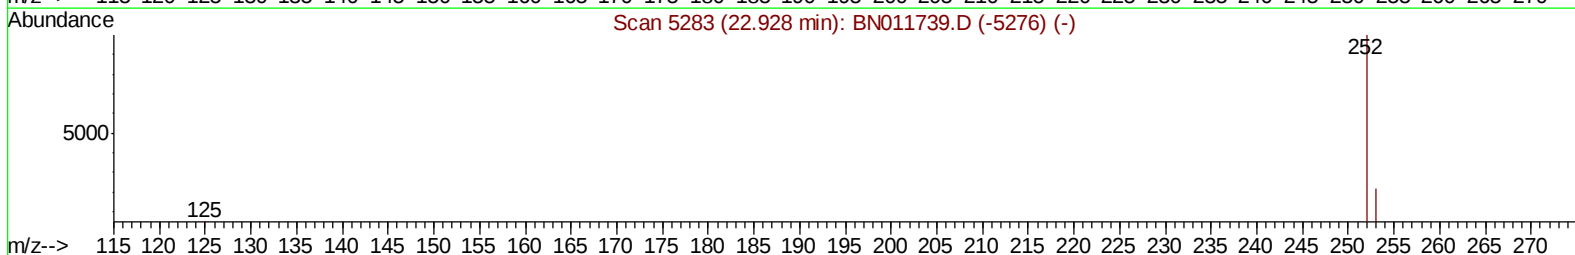
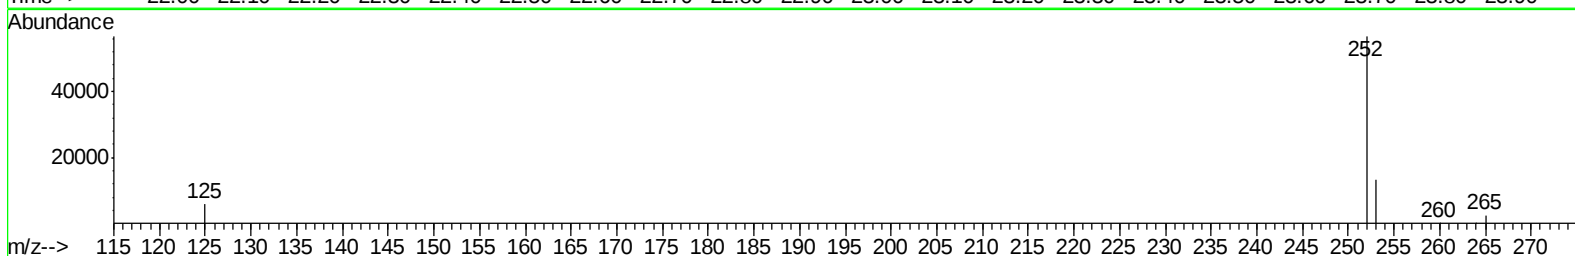


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090820\
Data File : BN011749.D
Acq On : 08 Sep 2020 22:31
Operator : CG/JU
Sample : L3840-14
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Sep 09 07:00:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN090820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 09 06:29:50 2020
Response via : Initial Calibration

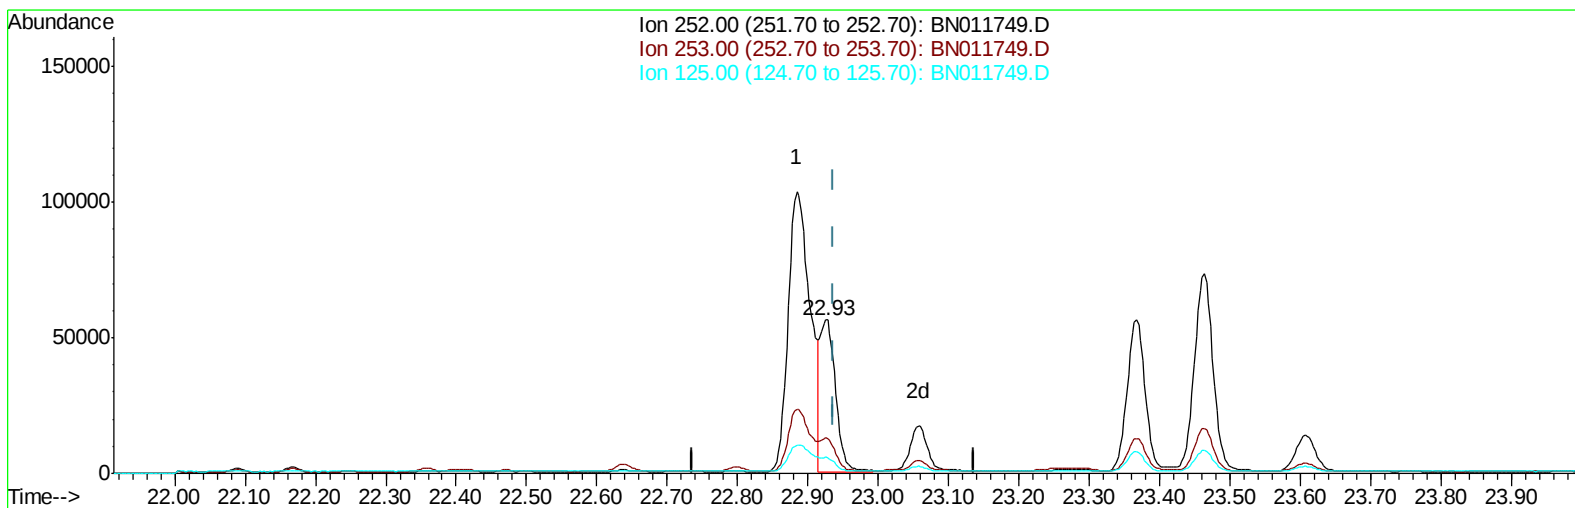

TIC: BN011749.D

(22) Benzo(k)fluoranthene

22.925min (-0.012) 2.03ng/ul m

response 86926

Ion	Exp%	Act%
252.00	100	100
253.00	25.90	23.27
125.00	12.10	10.57
0.00	0.00	0.00