
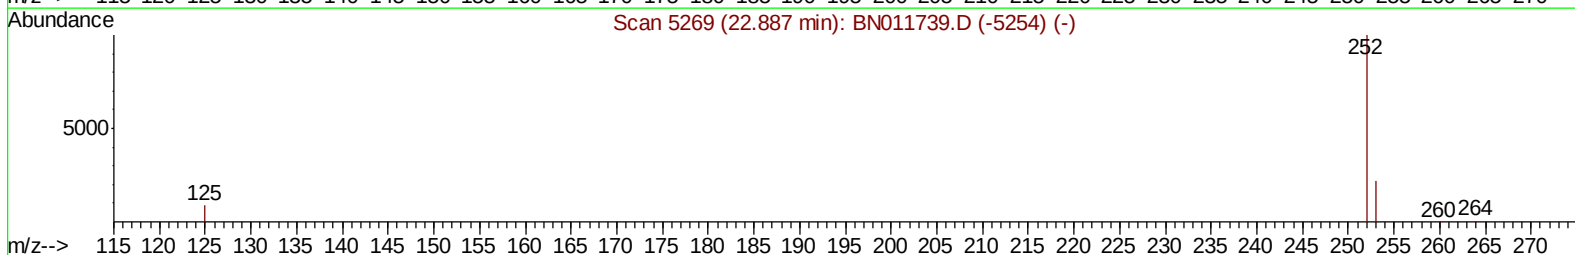
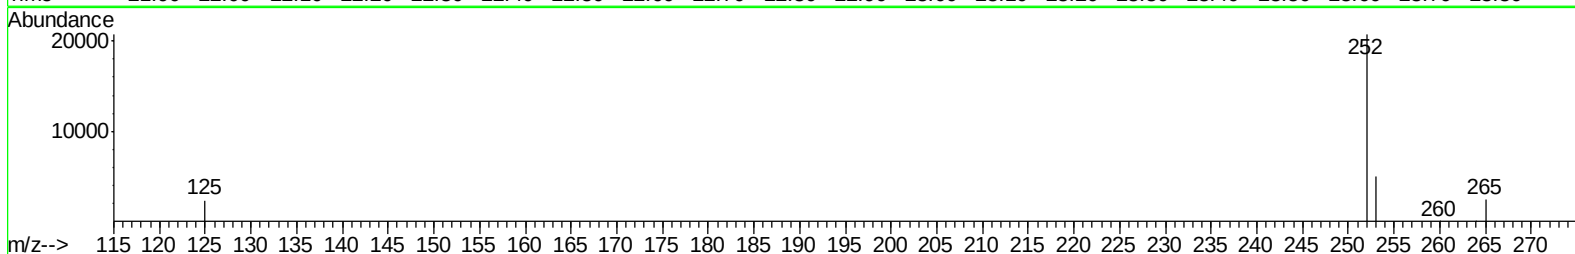


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090820\
Data File : BN011750.D
Acq On : 08 Sep 2020 23:08
Operator : CG/JU
Sample : L3840-14DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Sep 09 06:37:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN090820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 09 06:29:50 2020
Response via : Initial Calibration

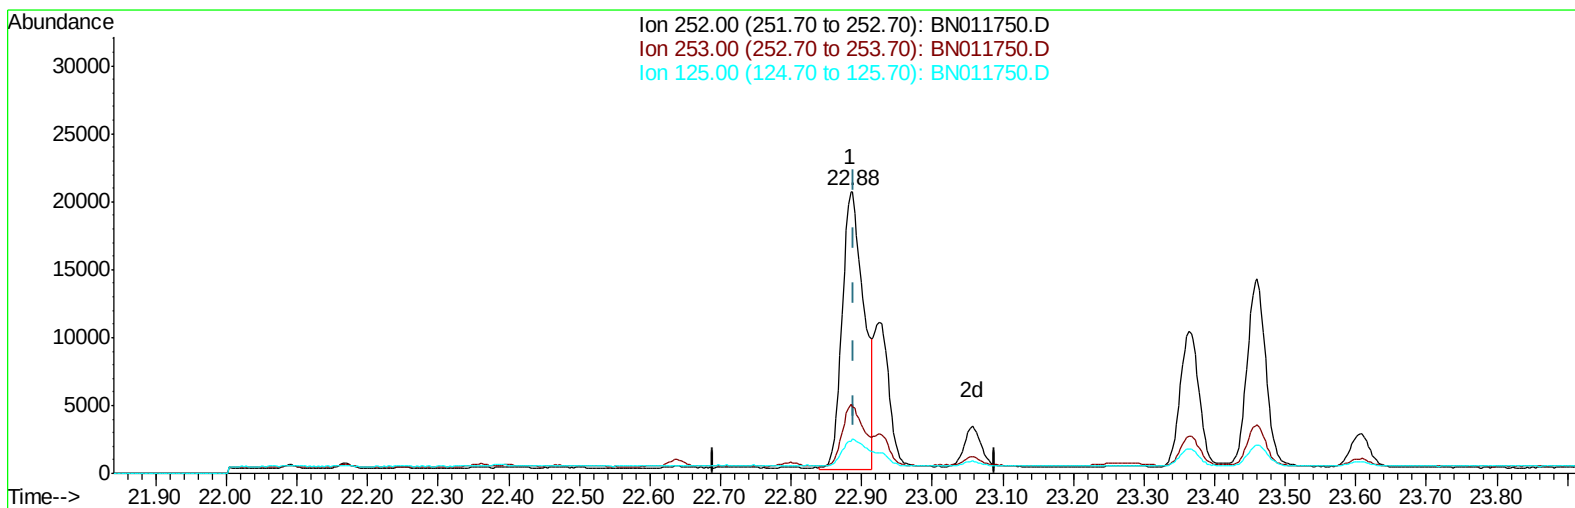

TIC: BN011750.D

(21) Benzo(b)fluoranthene

22.884min (-0.006) 0.99ng/ul m

response 43181

Ion	Exp%	Act%
252.00	100	100
253.00	25.30	24.45
125.00	11.80	11.57
0.00	0.00	0.00