
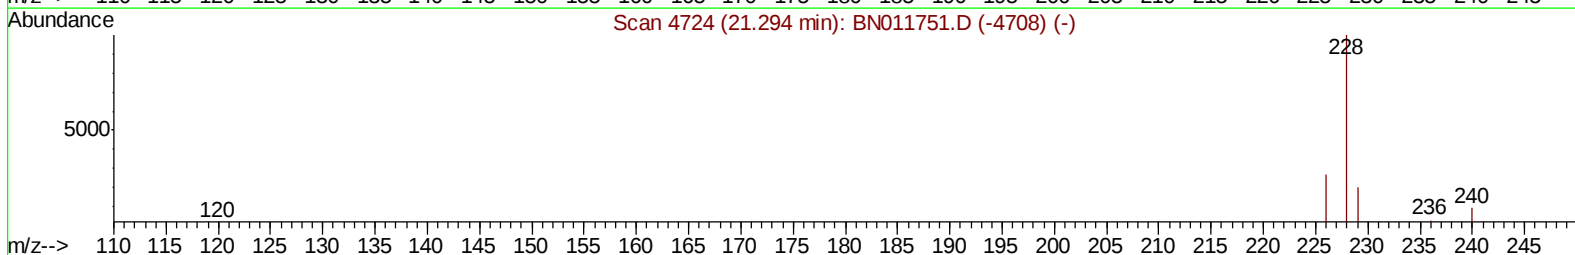
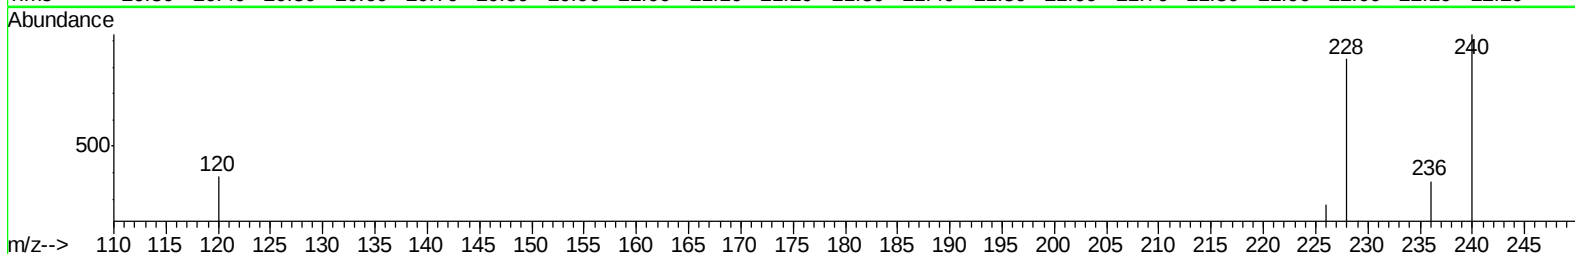


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090820\  
Data File : BN011752.D  
Acq On : 09 Sep 2020 00:56  
Operator : CG/JU  
Sample : L3840-06  
Misc :  
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Sep 09 07:29:15 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN090820.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Sep 09 07:05:35 2020  
Response via : Initial Calibration

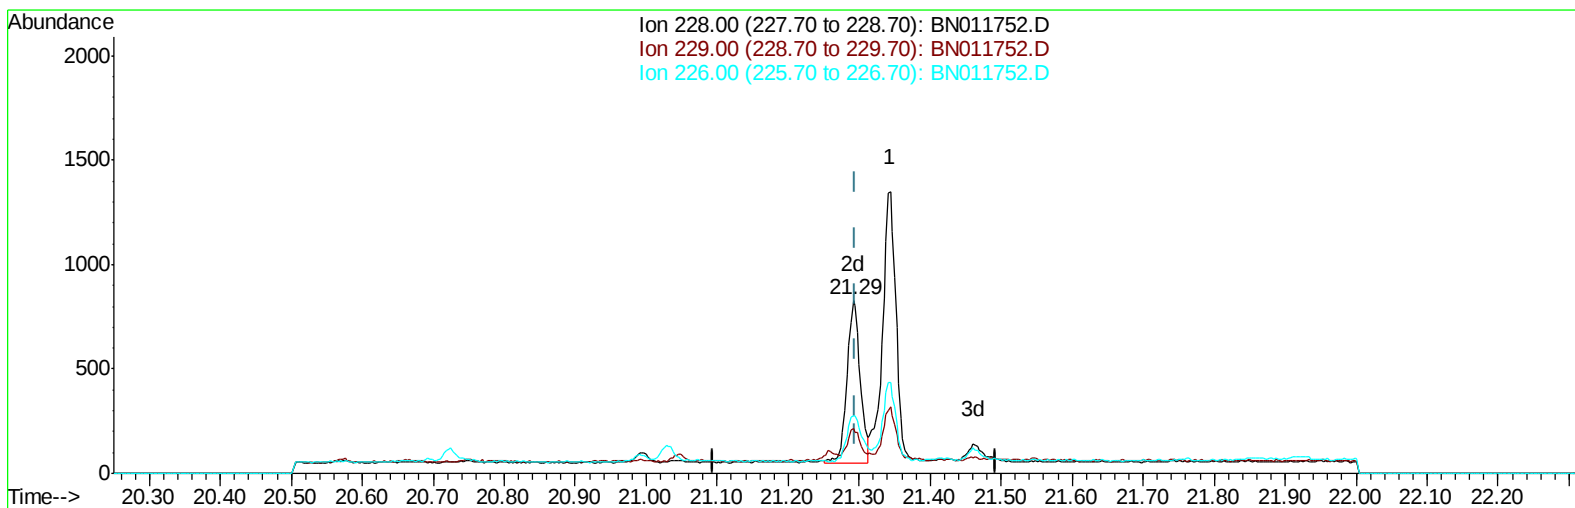

TIC: BN011752.D

(18) Benzo(a)anthracene

21.291min (-0.003) 0.03ng/ul m

response 1007

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 228.00 | 100   | 100    |
| 229.00 | 19.90 | 25.87# |
| 226.00 | 27.40 | 33.57# |
| 0.00   | 0.00  | 0.00   |