
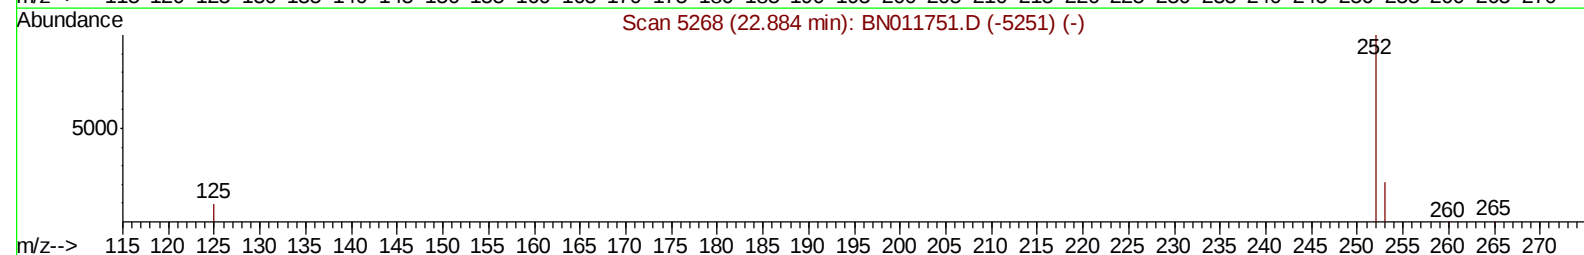
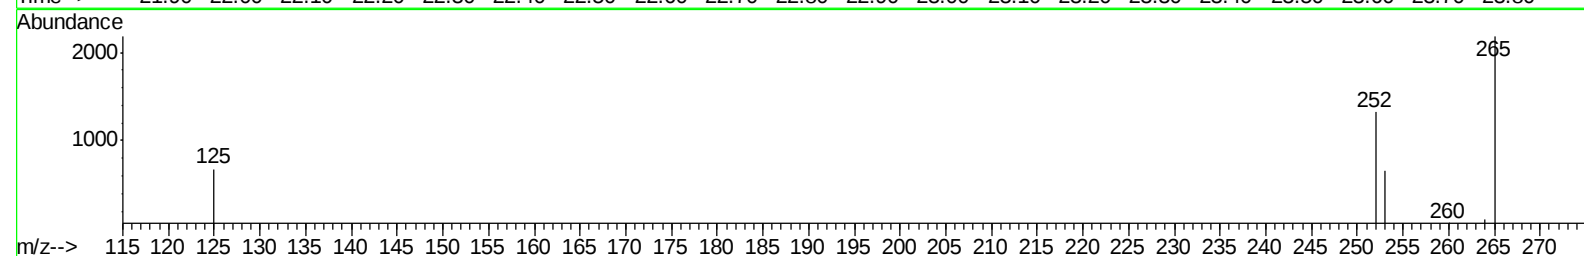


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090820\
Data File : BN011752.D
Acq On : 09 Sep 2020 00:56
Operator : CG/JU
Sample : L3840-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Sep 09 07:29:15 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN090820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 09 07:05:35 2020
Response via : Initial Calibration

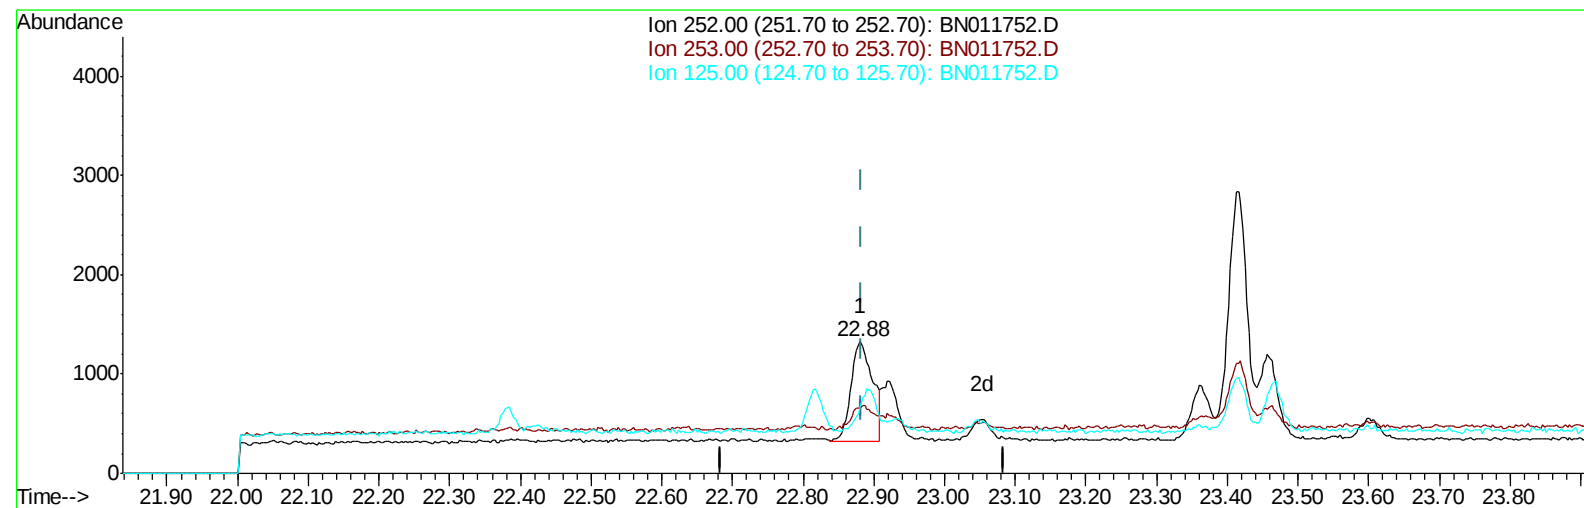

TIC: BN011752.D

(21) Benzo(b)fluoranthene

22.881min (-0.003) 0.05ng/ul m

response 2128

Ion	Exp%	Act%
252.00	100	100
253.00	25.30	50.08
125.00	11.80	51.13#
0.00	0.00	0.00