
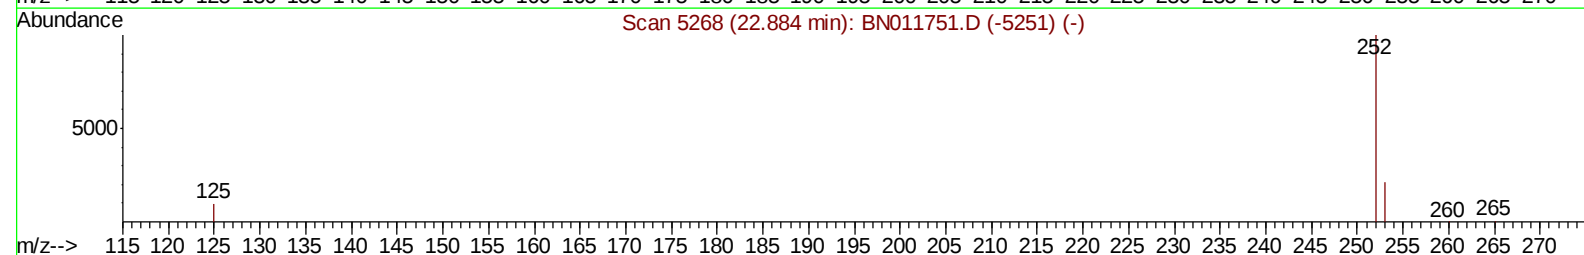
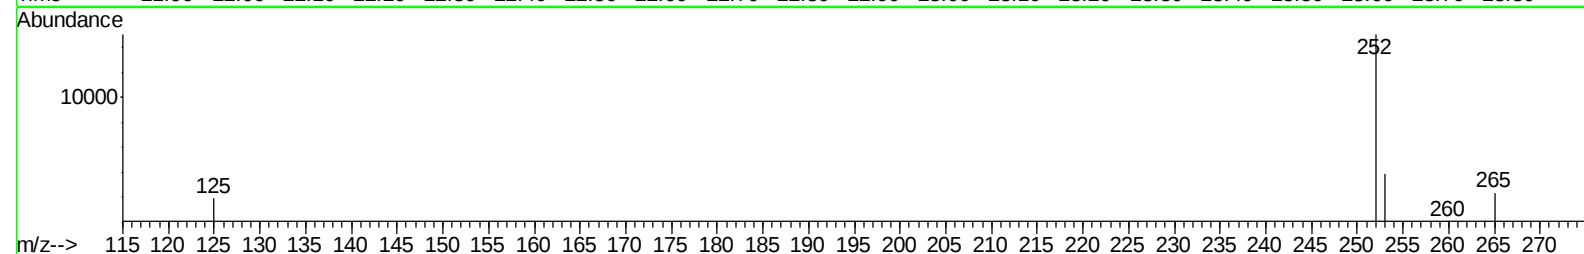


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090820\  
 Data File : BN011753.D  
 Acq On : 09 Sep 2020 01:32  
 Operator : CG/JU  
 Sample : L3843-01  
 Misc :  
 ALS Vial : 26 Sample Multiplier: 1

Quant Time: Sep 09 07:32:12 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN090820.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Sep 09 07:05:35 2020  
 Response via : Initial Calibration

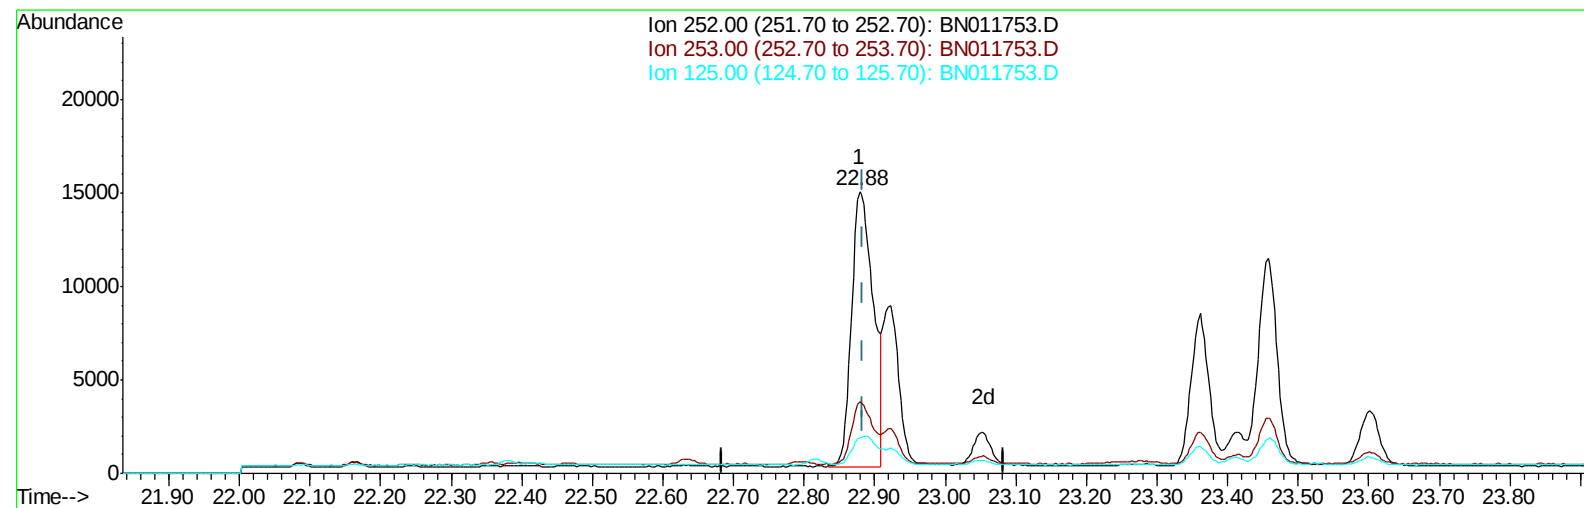

TIC: BN011753.D

(21) Benzo(b)fluoranthene

22.878min (-0.006) 0.70ng/ul m

response 31053

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 252.00 | 100   | 100   |
| 253.00 | 25.30 | 25.50 |
| 125.00 | 11.80 | 12.64 |
| 0.00   | 0.00  | 0.00  |