
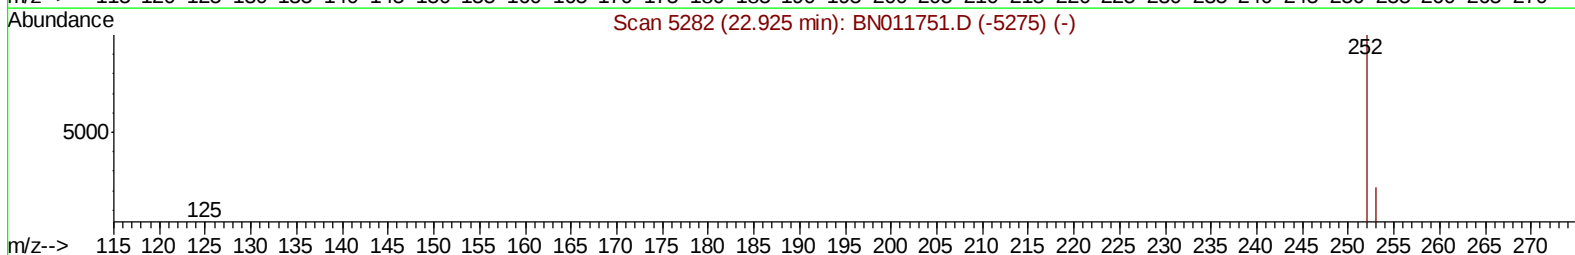
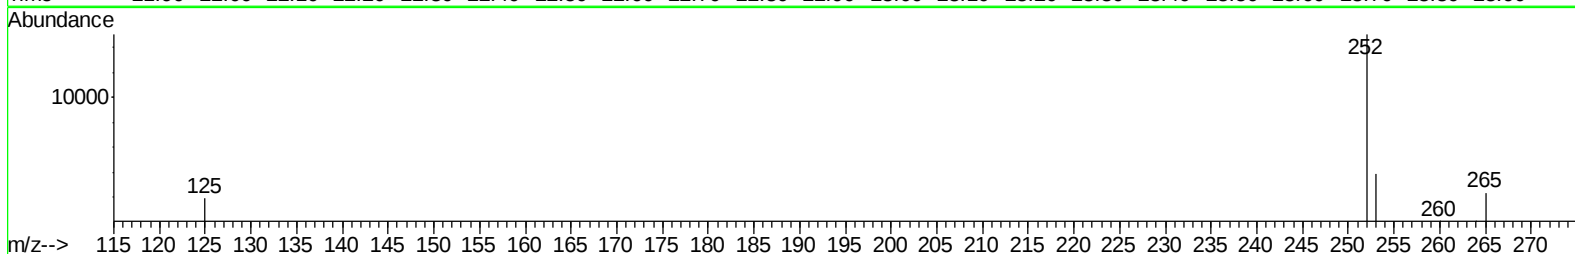


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090820\
Data File : BN011753.D
Acq On : 09 Sep 2020 01:32
Operator : CG/JU
Sample : L3843-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Sep 09 07:32:12 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN090820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 09 07:05:35 2020
Response via : Initial Calibration

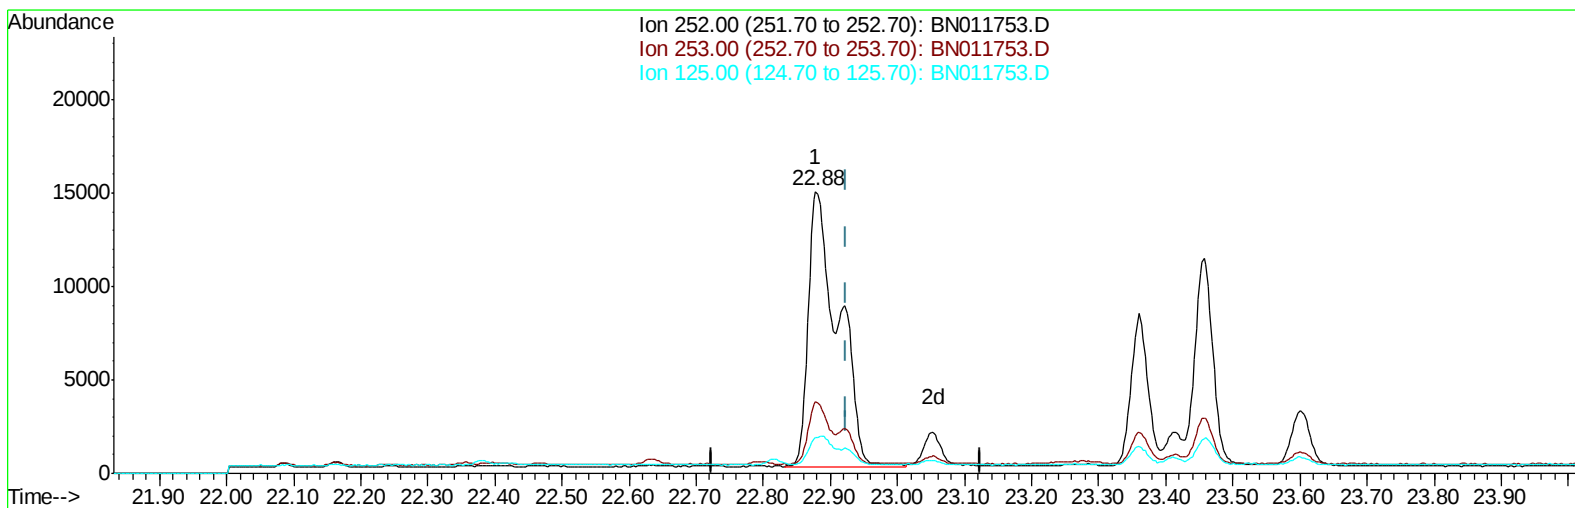

TIC: BN011753.D

(22) Benzo(k)fluoranthene
22.878min (-0.046) 0.99ng/ul
response 44947

Ion	Exp%	Act%
252.00	100	100
253.00	25.90	25.50
125.00	12.10	12.64
0.00	0.00	0.00