
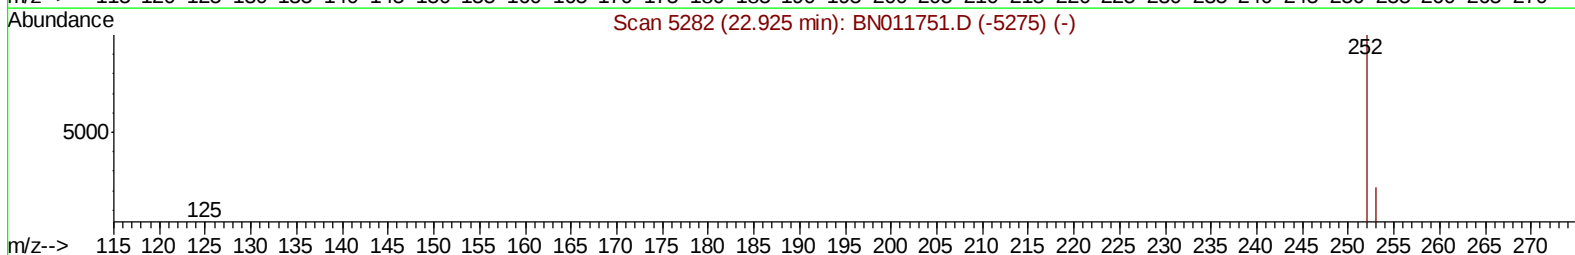
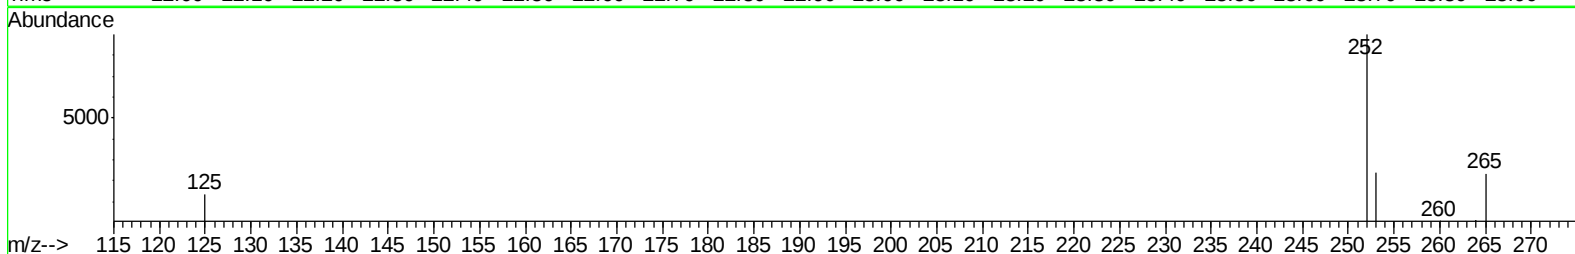


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090820\  
 Data File : BN011753.D  
 Acq On : 09 Sep 2020 01:32  
 Operator : CG/JU  
 Sample : L3843-01  
 Misc :  
 ALS Vial : 26 Sample Multiplier: 1

Quant Time: Sep 09 07:32:12 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN090820.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Sep 09 07:05:35 2020  
 Response via : Initial Calibration

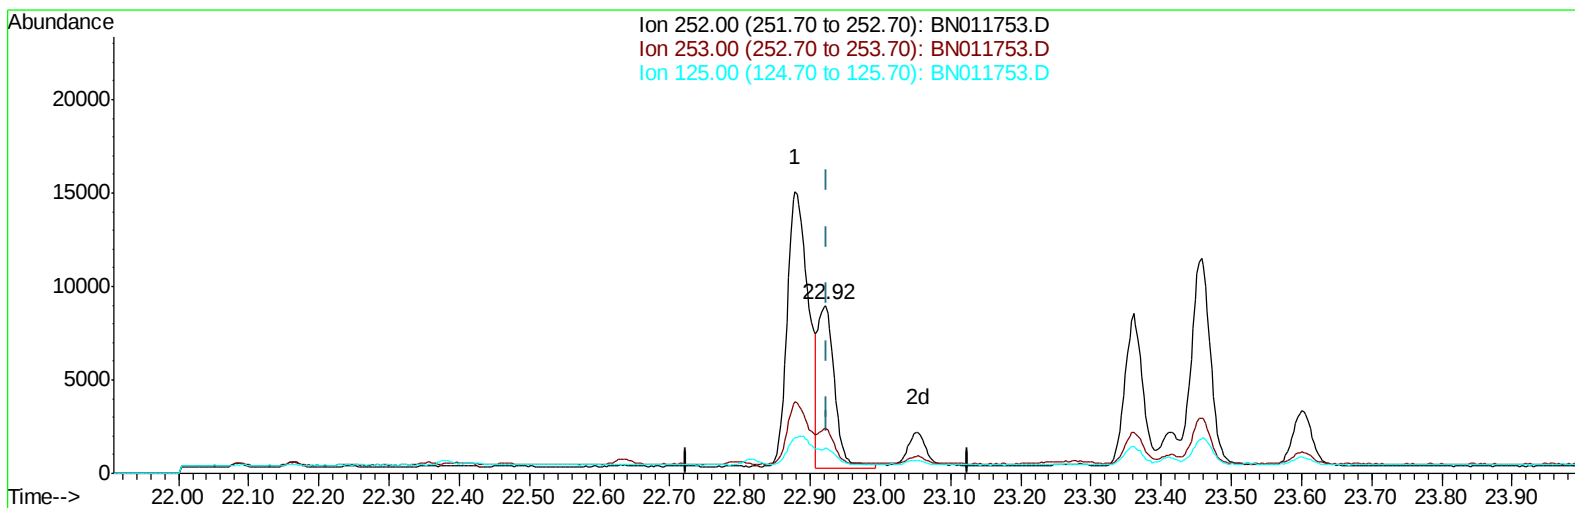

TIC: BN011753.D

(22) Benzo(k)fluoranthene

22.922min (-0.003) 0.31ng/ul m

response 14240

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 25.90 | 26.68  |
| 125.00 | 12.10 | 15.05# |
| 0.00   | 0.00  | 0.00   |